

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030824\
 Data File : VX040615.D
 Acq On : 07 Mar 2024 10:21
 Operator : JC/MD
 Sample : VX0308WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

Signal : TIC: VX040615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rBV	89471	93480	13.54%	1.796%
2	1.666	90	95	108	rVB	61597	85905	12.45%	1.650%
3	2.307	194	200	211	rVB	144122	229671	33.28%	4.413%
4	2.508	229	233	239	rVV2	880	1355	0.20%	0.026%
5	2.563	240	242	244	rVB2	325	183	0.03%	0.004%
6	2.788	275	279	284	rVB3	1201	1538	0.22%	0.030%
7	2.934	301	303	309	rVB3	448	783	0.11%	0.015%
8	3.093	327	329	332	rBV2	200	188	0.03%	0.004%
9	3.471	389	391	394	rVB2	246	228	0.03%	0.004%
10	3.508	394	397	401	rVB2	190	251	0.04%	0.005%
11	3.550	401	404	406	rBV	172	238	0.03%	0.005%
12	3.745	434	436	441	rVB2	203	259	0.04%	0.005%
13	3.788	441	443	446	rBV2	193	190	0.03%	0.004%
14	4.203	509	511	515	rVB	216	195	0.03%	0.004%
15	4.294	522	526	527	rBV2	160	187	0.03%	0.004%
16	4.446	543	551	570	rBV	58701	168333	24.39%	3.234%
17	4.678	587	589	590	rBV	289	257	0.04%	0.005%
18	4.721	594	596	598	rVB2	262	195	0.03%	0.004%
19	4.824	608	613	615	rVB2	178	263	0.04%	0.005%
20	4.849	615	617	620	rBV	243	297	0.04%	0.006%
21	4.904	623	626	627	rBV	187	176	0.03%	0.003%
22	5.056	638	651	667	rVV	91534	287804	41.70%	5.529%
23	5.349	696	699	700	rBV2	195	191	0.03%	0.004%
24	5.690	749	755	756	rBV2	309	434	0.06%	0.008%
25	5.849	779	781	783	rBV	197	199	0.03%	0.004%
26	5.964	788	800	816	rBV2	230885	690162	100.00%	13.260%
27	6.641	908	911	912	rBV2	165	199	0.03%	0.004%
28	6.757	921	930	942	rBV2	158054	380407	55.12%	7.309%
29	6.952	959	962	963	rBV	239	248	0.04%	0.005%
30	7.019	970	973	975	rBV2	219	273	0.04%	0.005%
31	7.111	981	988	997	rVB4	2578	5499	0.80%	0.106%
32	7.306	1011	1020	1034	rBV2	142643	314801	45.61%	6.048%
33	7.452	1042	1044	1045	rBV	187	172	0.02%	0.003%
34	7.482	1048	1049	1053	rVB3	382	421	0.06%	0.008%
35	8.025	1136	1138	1141	rVB2	174	225	0.03%	0.004%
36	8.049	1141	1142	1145	rBV	238	218	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030824\
 Data File : VX040615.D
 Acq On : 07 Mar 2024 10:21
 Operator : JC/MD
 Sample : VX0308WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

37	8.086	1145	1148	1151	rBV2	201	207	0.03%	0.004%
38	8.263	1176	1177	1180	rVV	199	197	0.03%	0.004%
39	8.324	1180	1187	1200	rVV	100472	168239	24.38%	3.232%
40	8.440	1204	1206	1208	rVB	236	219	0.03%	0.004%
41	8.482	1210	1213	1217	rVV3	521	754	0.11%	0.014%
42	8.647	1233	1240	1254	rBV	349333	542077	78.54%	10.415%
43	8.805	1265	1266	1269	rVB2	272	182	0.03%	0.003%
44	8.946	1284	1289	1300	rBV	69097	107251	15.54%	2.061%
45	9.092	1309	1313	1314	rBV	324	357	0.05%	0.007%
46	9.214	1328	1333	1335	rVB	242	200	0.03%	0.004%
47	9.269	1341	1342	1344	rVB	273	186	0.03%	0.004%
48	9.378	1355	1360	1375	rBV	245911	366467	53.10%	7.041%
49	9.695	1410	1412	1414	rBV	175	185	0.03%	0.004%
50	9.714	1414	1415	1417	rVV	242	177	0.03%	0.003%
51	9.854	1436	1438	1441	rVB3	351	340	0.05%	0.007%
52	10.049	1465	1470	1486	rVV	290031	415932	60.27%	7.991%
53	10.153	1486	1487	1489	rVB	402	218	0.03%	0.004%
54	10.189	1491	1493	1498	rBB3	258	393	0.06%	0.008%
55	10.549	1550	1552	1554	rBV	276	174	0.03%	0.003%
56	10.634	1564	1566	1568	rVV	195	248	0.04%	0.005%
57	10.653	1568	1569	1570	rVV	468	187	0.03%	0.004%
58	10.829	1594	1598	1599	rBV	179	209	0.03%	0.004%
59	10.909	1609	1611	1613	rVB2	233	213	0.03%	0.004%
60	10.964	1619	1620	1623	rVB2	459	364	0.05%	0.007%
61	11.000	1623	1626	1629	rBV2	192	292	0.04%	0.006%
62	11.085	1636	1640	1649	rBV3	1074	2000	0.29%	0.038%
63	11.189	1652	1657	1667	rVV	273196	349145	50.59%	6.708%
64	11.451	1699	1700	1705	rBV2	431	427	0.06%	0.008%
65	11.598	1722	1724	1728	rBV2	210	201	0.03%	0.004%
66	11.750	1747	1749	1754	rVB2	437	548	0.08%	0.011%
67	11.817	1757	1760	1761	rBV	137	174	0.03%	0.003%
68	11.976	1782	1786	1788	rVB	582	603	0.09%	0.012%
69	12.018	1788	1793	1803	rBV	362284	468403	67.87%	8.999%
70	12.317	1837	1842	1851	rBV	392954	502219	72.77%	9.649%
71	12.494	1870	1871	1874	rBV2	206	238	0.03%	0.005%
72	12.707	1904	1906	1909	rVB2	161	173	0.03%	0.003%
73	12.762	1912	1915	1916	rBV2	236	186	0.03%	0.004%
74	12.945	1943	1945	1948	rBV	211	201	0.03%	0.004%
75	12.994	1951	1953	1957	rVB	224	269	0.04%	0.005%
76	13.030	1957	1959	1962	rBV2	263	331	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030824\
 Data File : VX040615.D
 Acq On : 07 Mar 2024 10:21
 Operator : JC/MD
 Sample : VX0308WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

77	13.116	1971	1973	1976	rVB	485	475	0.07%	0.009%
78	13.512	2036	2038	2042	rVB2	208	267	0.04%	0.005%
79	13.591	2047	2051	2056	rVV3	1035	1493	0.22%	0.029%
80	13.780	2079	2082	2088	rVB2	828	1201	0.17%	0.023%
81	13.963	2110	2112	2117	rVB2	848	882	0.13%	0.017%
82	14.073	2128	2130	2133	rVV	211	196	0.03%	0.004%
83	14.195	2148	2150	2152	rBV	160	188	0.03%	0.004%
84	14.365	2176	2178	2181	rVB2	295	188	0.03%	0.004%
85	14.609	2216	2218	2221	rBV	336	379	0.05%	0.007%
86	14.688	2228	2231	2233	rVV2	224	263	0.04%	0.005%
87	14.713	2233	2235	2241	rVV2	161	255	0.04%	0.005%
88	14.774	2241	2245	2247	rVB2	336	381	0.06%	0.007%
89	14.798	2247	2249	2250	rBV	202	203	0.03%	0.004%
90	15.054	2289	2291	2292	rBV2	251	184	0.03%	0.004%
91	15.164	2307	2309	2311	rBV2	210	230	0.03%	0.004%
92	15.243	2321	2322	2325	rVB	323	250	0.04%	0.005%
93	15.597	2378	2380	2382	rBV	536	393	0.06%	0.008%
94	15.621	2382	2384	2388	rVV	254	309	0.04%	0.006%
95	15.688	2393	2395	2397	rBV2	169	192	0.03%	0.004%
96	15.792	2411	2412	2413	rBV	400	240	0.03%	0.005%
97	15.853	2419	2422	2423	rBV	253	213	0.03%	0.004%
98	15.871	2423	2425	2432	rVV3	227	296	0.04%	0.006%
99	15.981	2441	2443	2445	rBV2	246	218	0.03%	0.004%
100	16.725	2564	2565	2566	rBV	384	207	0.03%	0.004%




Sum of corrected areas: 5204914

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030824\
Data File : VX040615.D
Acq On : 07 Mar 2024 10:21
Operator : JC/MD
Sample : VX0308WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK663

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

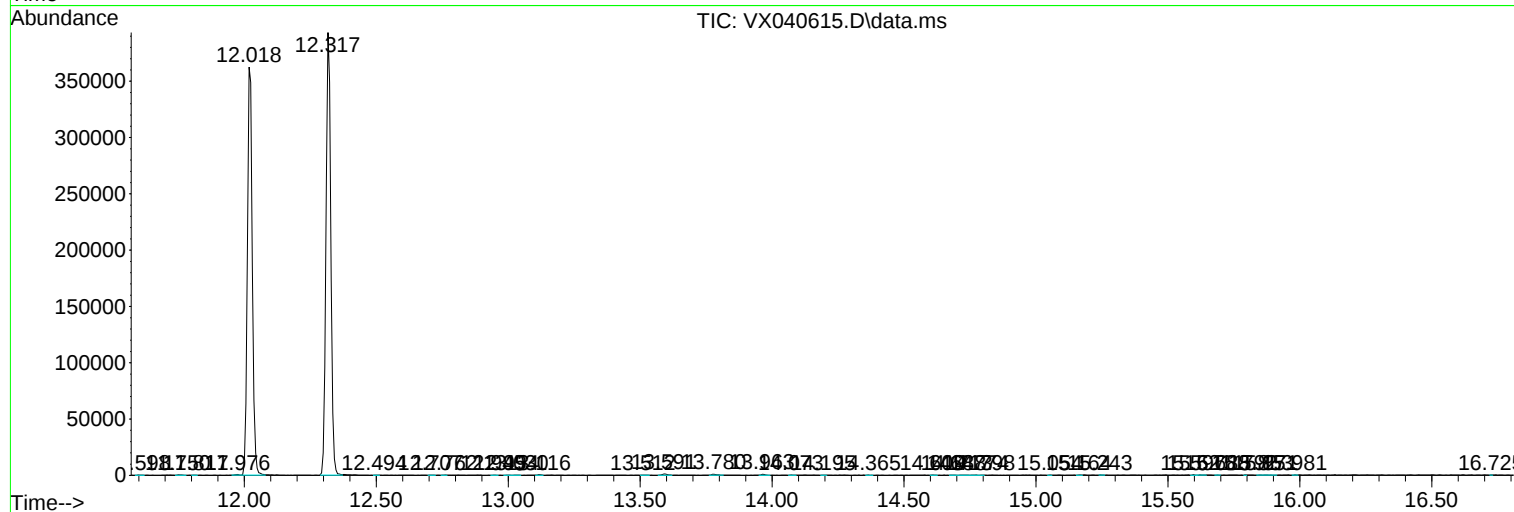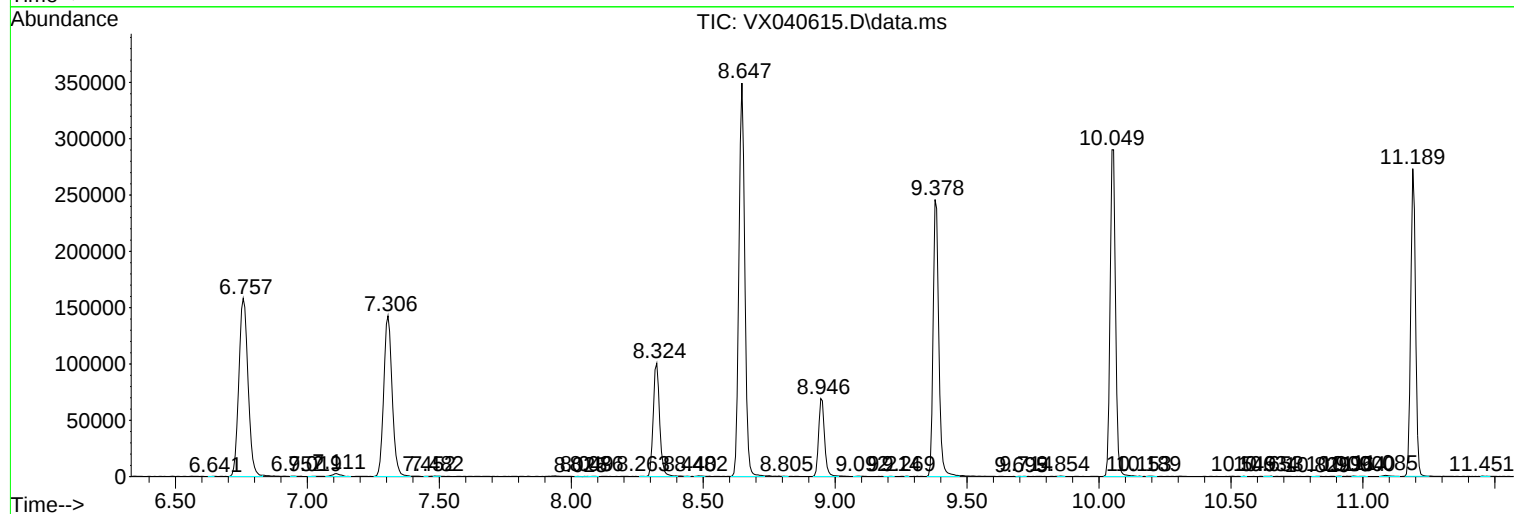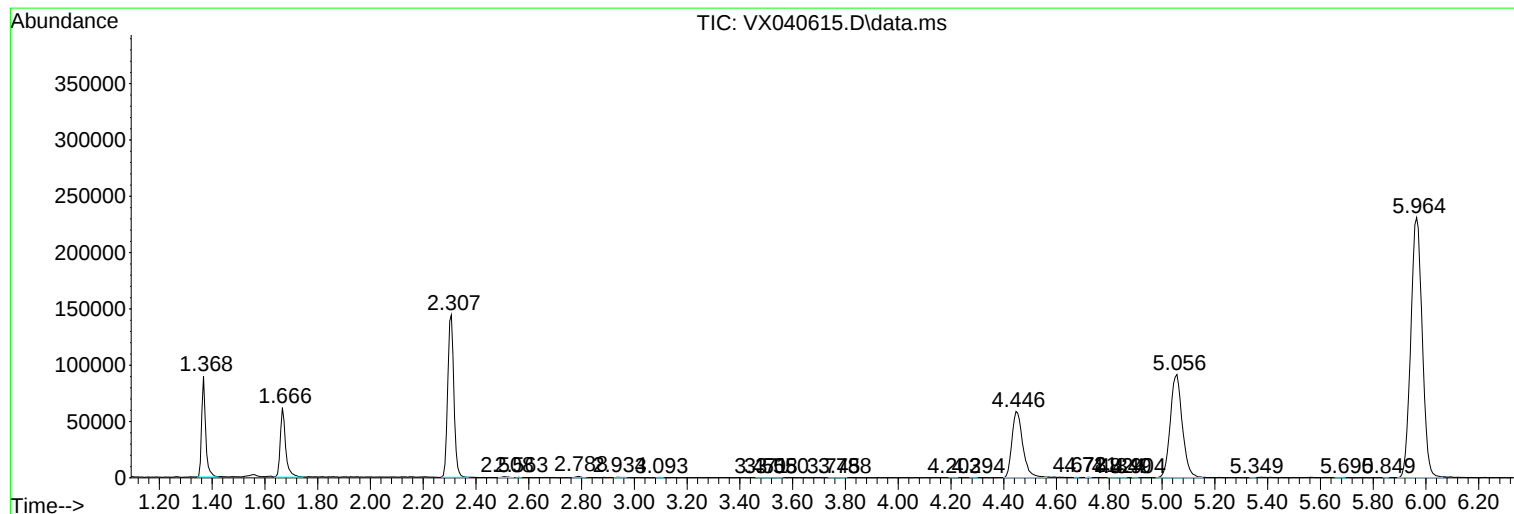

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030824\
Data File : VX040615.D
Acq On : 07 Mar 2024 10:21
Operator : JC/MD
Sample : VX0308WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK663

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030824\
Data File : VX040615.D
Acq On : 07 Mar 2024 10:21
Operator : JC/MD
Sample : VX0308WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK663

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------