
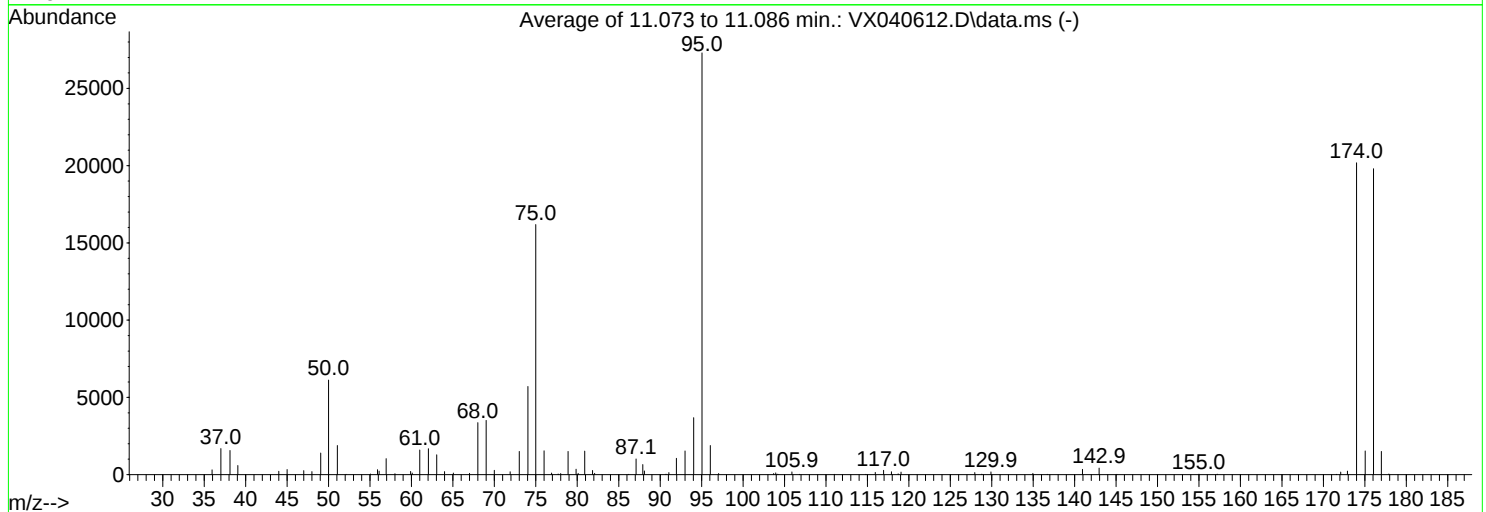


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030824\
Data File : VX040612.D
Acq On : 07 Mar 2024 08:16
Operator : JC/MD
Sample : BFB666
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB666

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM030724WMA.M
Title : VOC Analysis
Last Update : Fri Mar 08 01:27:40 2024

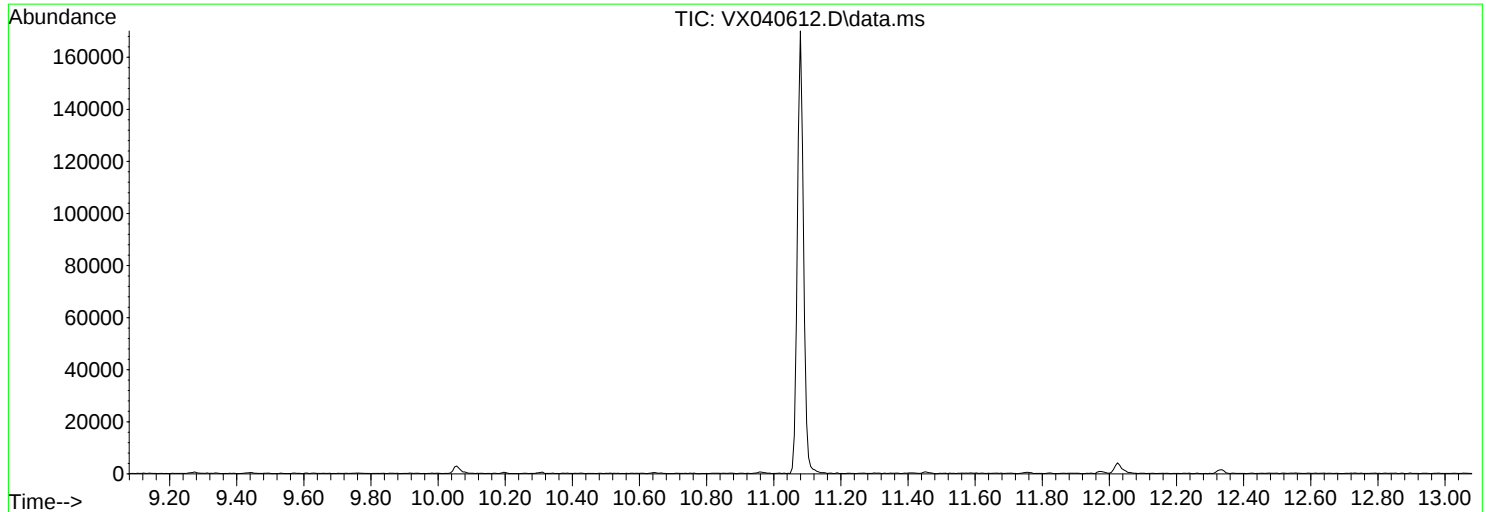

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	6121	PASS
75	95	30	80	59.3	16184	PASS
95	95	100	100	100.0	27301	PASS
96	95	5	9	6.9	1890	PASS
173	174	0.00	2	1.1	227	PASS
174	95	50	120	73.9	20183	PASS
175	174	5	9	7.6	1532	PASS
176	174	95	101	98.1	19801	PASS
177	176	5	9	7.6	1497	PASS

m/z	Abundance
40.10	161.0
44.00	64.0

Instrument :
MSVOA_X
ClientSampleId :
BFB666

m/z	Abundance
35.90	370.0
37.00	1742.0
38.10	1683.0
39.10	603.0
40.00	112.0
44.00	263.0
45.10	365.0
47.00	402.0
48.00	230.0
49.00	1335.0
50.00	5883.0
51.00	1791.0
55.10	68.0
55.90	540.0
57.00	938.0
58.10	89.0
59.90	285.0
61.00	1459.0
62.00	1822.0
63.10	1597.0
64.00	129.0
65.00	186.0
67.00	69.0
68.00	3283.0
69.00	3721.0
70.00	266.0
71.90	195.0
73.10	1372.0
74.00	5222.0
75.00	15640.0
76.00	1696.0
77.00	104.0
78.90	1532.0
79.80	320.0
80.10	265.0
80.90	1543.0
81.80	385.0
86.20	68.0
87.10	995.0
87.90	667.0
90.70	99.0
91.10	111.0
92.00	872.0
93.00	1580.0
94.10	3461.0
95.10	25160.0
96.10	1628.0
97.10	120.0
103.70	215.0
104.20	83.0
106.00	140.0
106.80	61.0
111.00	56.0
116.00	129.0
116.90	264.0
118.00	144.0
118.70	159.0
119.20	133.0
127.90	127.0
129.90	102.0
135.00	84.0
140.90	237.0
143.00	328.0
155.00	53.0
171.60	52.0
172.10	105.0
172.90	198.0
174.00	16310.0
175.00	1250.0
176.00	15410.0
177.00	1258.0
177.90	53.0

Instrument :
MSVOA_X
ClientSampleId :
BFB666

m/z	Abundance
36.00	342.0
37.00	2098.0
38.10	1866.0
39.00	722.0
40.00	145.0
44.10	399.0
44.90	352.0
46.90	179.0
48.10	190.0
49.10	1628.0
50.00	7516.0
51.10	2432.0
52.10	53.0
55.00	57.0
56.10	675.0
57.00	1319.0
57.90	87.0
59.90	343.0
61.00	1886.0
62.10	1960.0
63.00	1268.0
64.00	262.0
65.10	121.0
67.00	95.0
68.00	4183.0
69.00	3765.0
70.00	388.0
71.90	261.0
73.00	1900.0
74.10	7175.0
75.00	19320.0
76.00	1715.0
76.90	128.0
78.00	209.0
78.90	1675.0
79.90	462.0
80.90	1905.0
81.90	410.0
87.10	1242.0
87.90	1291.0
91.00	171.0
91.90	1205.0
93.00	1858.0
94.00	4439.0
95.00	32688.0
96.10	2183.0
97.00	96.0
103.90	215.0
105.90	186.0
114.80	53.0
115.90	210.0
117.00	332.0
117.90	198.0
119.00	182.0
128.00	123.0
128.80	82.0
129.80	134.0
130.00	134.0
134.90	99.0
136.70	72.0
141.00	445.0
142.90	563.0
155.00	56.0
157.20	100.0
172.00	200.0
172.80	128.0
173.00	123.0
174.00	24104.0
175.00	1923.0
176.10	24000.0
177.00	1667.0
177.90	85.0

Instrument :
MSVOA_X
ClientSampleId :
BFB666

m/z	Abundance
35.90	228.0
37.00	1224.0
38.10	1133.0
39.00	455.0
39.90	154.0
44.10	168.0
45.00	263.0
47.10	190.0
47.90	164.0
49.00	1244.0
50.00	4963.0
51.00	1426.0
55.90	428.0
56.90	836.0
60.10	312.0
61.00	1441.0
62.10	1241.0
63.00	1002.0
64.00	194.0
67.00	89.0
68.00	2634.0
69.00	3063.0
70.10	201.0
72.00	107.0
72.90	1240.0
74.00	4724.0
75.00	13591.0
76.00	1212.0
76.80	94.0
77.70	116.0
78.90	1312.0
79.90	280.0
81.00	1109.0
82.10	258.0
87.10	801.0
88.10	712.0
91.00	139.0
92.00	1083.0
93.00	1145.0
94.10	3150.0
95.10	24056.0
96.00	1859.0
104.00	143.0
105.80	191.0
115.90	109.0
117.00	232.0
117.80	221.0
119.00	199.0
127.90	168.0
129.90	160.0
134.90	78.0
141.00	352.0
143.00	396.0
145.10	78.0
172.20	198.0
172.90	231.0
174.00	20136.0
175.10	1423.0
176.00	19992.0
177.00	1565.0

Instrument :
MSVOA_X
ClientSampleId :
BFB666