

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX030920\  
 Data File : VX015145.D  
 Acq On : 09 Mar 2020 16:06  
 Operator : JC/SP  
 Sample : L1842-11  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 RE132D6-20200304

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X030420W.M

Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.070       | 26            | 30          | 43           | rBV      | 702669         | 900667        | 1.92%           | 1.557%        |
| 2         | 2.375       | 236           | 244         | 257          | rBV2     | 354356         | 706903        | 1.51%           | 1.222%        |
| 3         | 5.490       | 745           | 755         | 767          | rBV      | 200696         | 572184        | 1.22%           | 0.989%        |
| 4         | 5.655       | 769           | 782         | 794          | rVV      | 327352         | 906805        | 1.93%           | 1.568%        |
| 5         | 6.057       | 837           | 848         | 860          | rBV      | 220748         | 576112        | 1.23%           | 0.996%        |
| 6         | 6.849       | 969           | 978         | 995          | rBV      | 524130         | 1222266       | 2.60%           | 2.114%        |
| 7         | 7.209       | 1025          | 1037        | 1059         | rBV      | 22075460       | 46946502      | 100.00%         | 81.180%       |
| 8         | 8.709       | 1276          | 1283        | 1292         | rBV      | 1141571        | 1735081       | 3.70%           | 3.000%        |
| 9         | 10.105      | 1504          | 1512        | 1523         | rBV      | 1113705        | 1536494       | 3.27%           | 2.657%        |
| 10        | 11.135      | 1675          | 1681        | 1687         | rBV      | 887056         | 1189089       | 2.53%           | 2.056%        |
| 11        | 12.074      | 1830          | 1835        | 1841         | rBV      | 1282424        | 1537811       | 3.28%           | 2.659%        |


Sum of corrected areas: 57829914

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX030920\  
Data File : VX015145.D  
Acq On : 09 Mar 2020 16:06  
Operator : JC/SP  
Sample : L1842-11  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RE132D6-20200304

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X030420W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

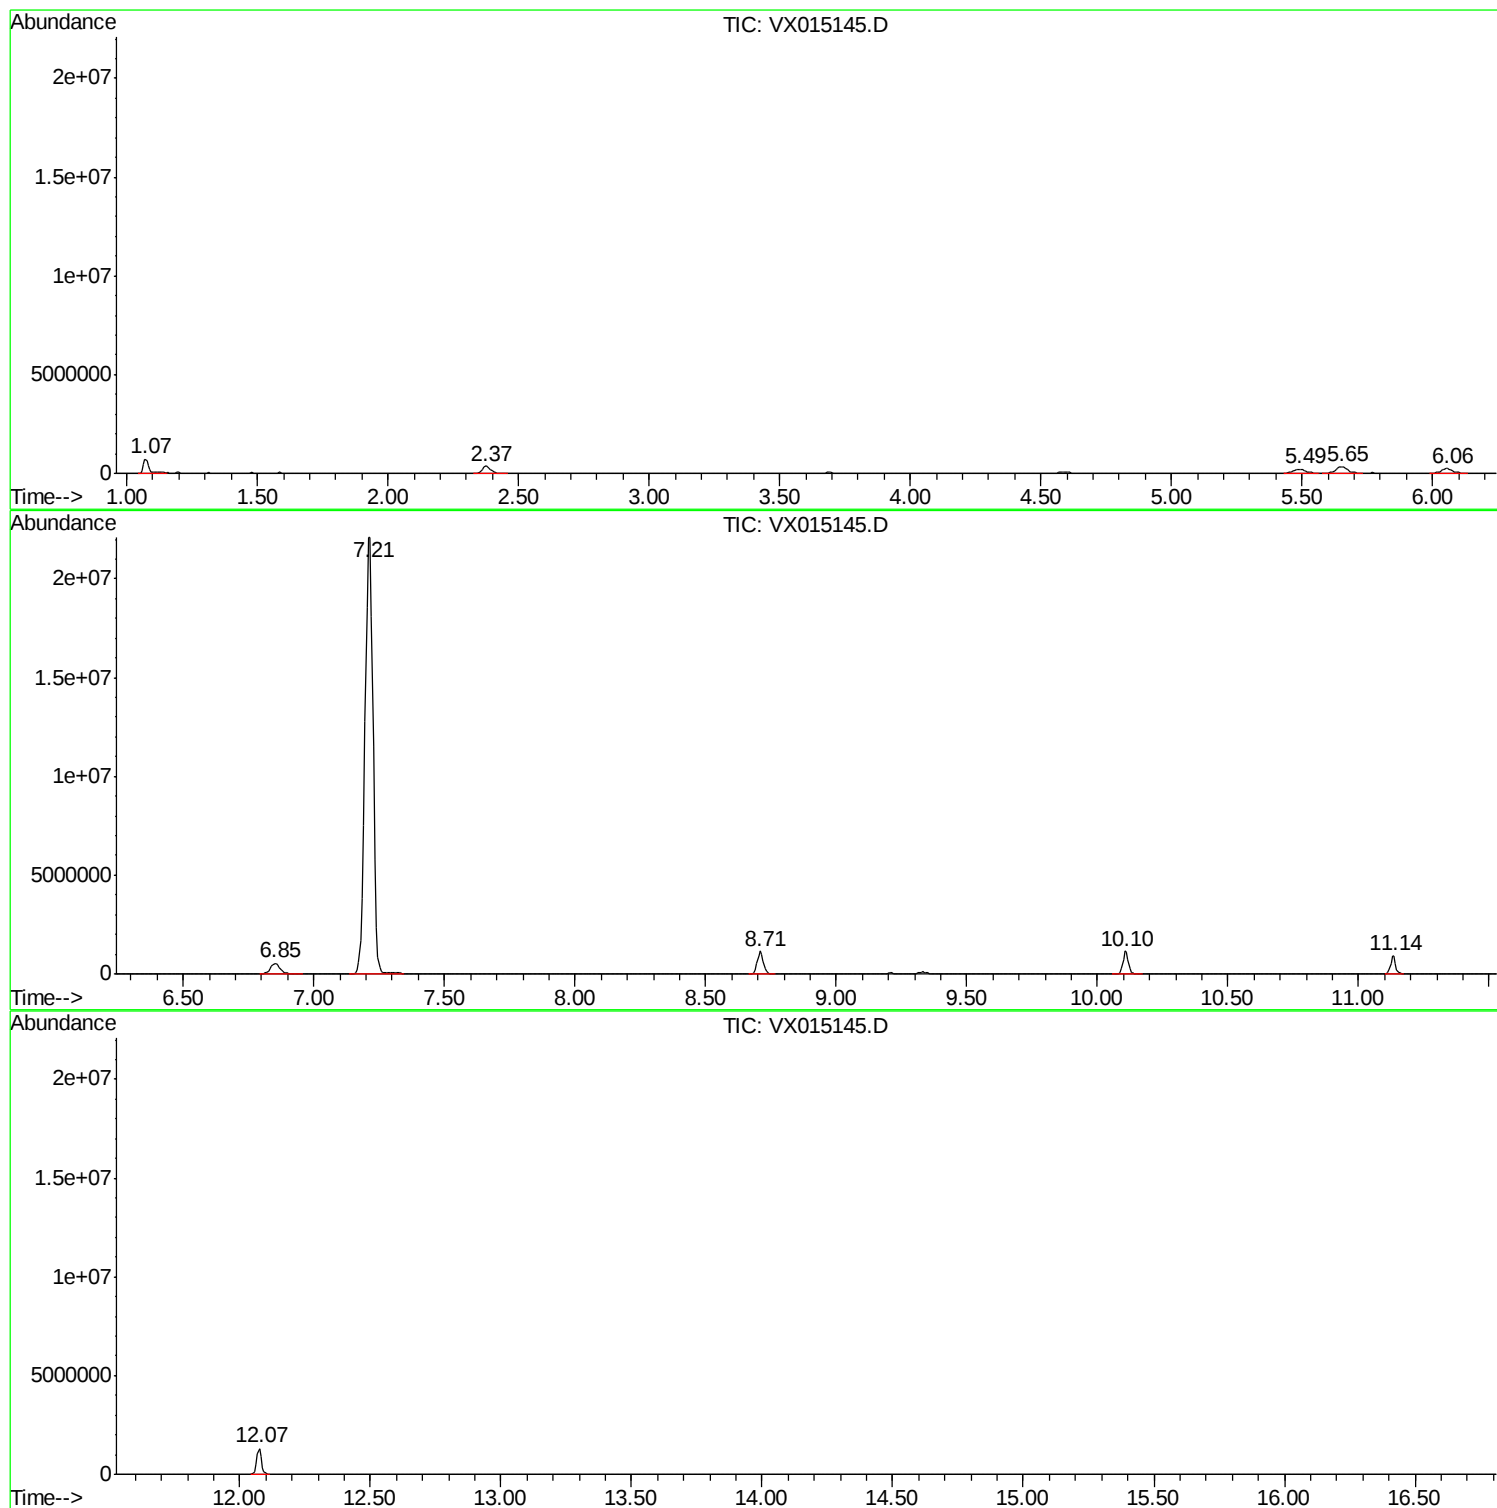

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX030920\  
Data File : VX015145.D  
Acq On : 09 Mar 2020 16:06  
Operator : JC/SP  
Sample : L1842-11  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RE132D6-20200304

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X030420W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX030920\  
Data File : VX015145.D  
Acq On : 09 Mar 2020 16:06  
Operator : JC/SP  
Sample : L1842-11  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RE132D6-20200304

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X030420W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | ---Internal Standard--- |
|------------------|----|---------|-------|----------|-------------------------|
|                  |    |         |       |          | # RT Resp Conc          |