

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030921\
 Data File : VX021110.D
 Acq On : 09 Mar 2021 15:50
 Operator : JC/MD
 Sample : M1578-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-1

Quant Time: Mar 10 00:31:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 24 13:50:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.629	168	199130	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.829	114	366283	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.094	117	367398	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.059	152	175887	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.035	65	135074	50.22	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 100.44%	
35) Dibromofluoromethane	5.464	113	117690	52.88	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 105.76%	
50) Toluene-d8	8.694	98	468436	53.98	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 107.96%	
62) 4-Bromofluorobenzene	11.118	95	178217	55.54	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 111.08%	


Target Compounds						Qvalue
5) Bromomethane	1.634	94	390	Below Cal	#	63
11) Tert butyl alcohol	3.005	59	29755	49.68	ug/l	99
13) Acrolein	2.276	56	421	1.14	ug/l #	65
15) Acrylonitrile	2.993	53	399	0.31	ug/l #	9
16) Acetone	2.417	43	28235	25.48	ug/l	100
18) Methyl Acetate	2.752	43	3621	1.38	ug/l	94
25) 2-Butanone	4.641	43	5402	3.21	ug/l #	87
29) Tetrahydrofuran	5.117	42	380	0.35	ug/l #	31
31) Cyclohexane	5.635	56	3962	1.02	ug/l #	1
36) 1,1-Dichloropropene	5.623	75	14950	4.29	ug/l #	48
38) Carbon Tetrachloride	5.629	117	19264	5.71	ug/l #	17
40) Benzene	6.117	78	11370	1.09	ug/l	95
44) Trichloroethene	7.188	130	1790	0.65	ug/l	95
48) Methyl methacrylate	7.629	41	26569	9.40	ug/l #	35
49) 1,4-Dioxane	7.723	88	1006	15.25	ug/l #	58
51) 4-Methyl-2-Pentanone	8.623	43	809	0.25	ug/l	98
52) Toluene	8.765	92	15877	2.44	ug/l	100
56) Ethyl methacrylate	9.224	69	905	0.22	ug/l #	36
59) 2-Hexanone	9.471	43	603	0.25	ug/l	92
67) Ethyl Benzene	10.235	91	4867	0.35	ug/l	94
68) m/p-Xylenes	10.341	106	8243	1.60	ug/l	97
69) o-Xylene	10.683	106	3703	0.73	ug/l	96
74) N-amyl acetate	10.894	43	1137	0.20	ug/l #	40
75) 1,1,2,2-Tetrachloroethane	11.318	83	1919	0.43	ug/l #	26
76) 1,2,3-Trichloropropane	11.118	75	85701	22.65	ug/l #	39
80) 1,3,5-Trimethylbenzene	11.489	105	2634	0.23	ug/l	92
81) trans-1,4-Dichloro-2-b...	11.118	75	85701	50.15	ug/l #	12
84) 1,2,4-Trimethylbenzene	11.789	105	12732	1.09	ug/l	90
85) sec-Butylbenzene	11.789	105	12732	0.96	ug/l #	57
90) Hexachloroethane	12.624	117	624	0.27	ug/l #	9
95) Naphthalene	13.818	128	11339	0.88	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030921\
Data File : VX021110.D
Acq On : 09 Mar 2021 15:50
Operator : JC/MD
Sample : M1578-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-1

Quant Time: Mar 10 00:31:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 24 13:50:55 2021
Response via : Initial Calibration




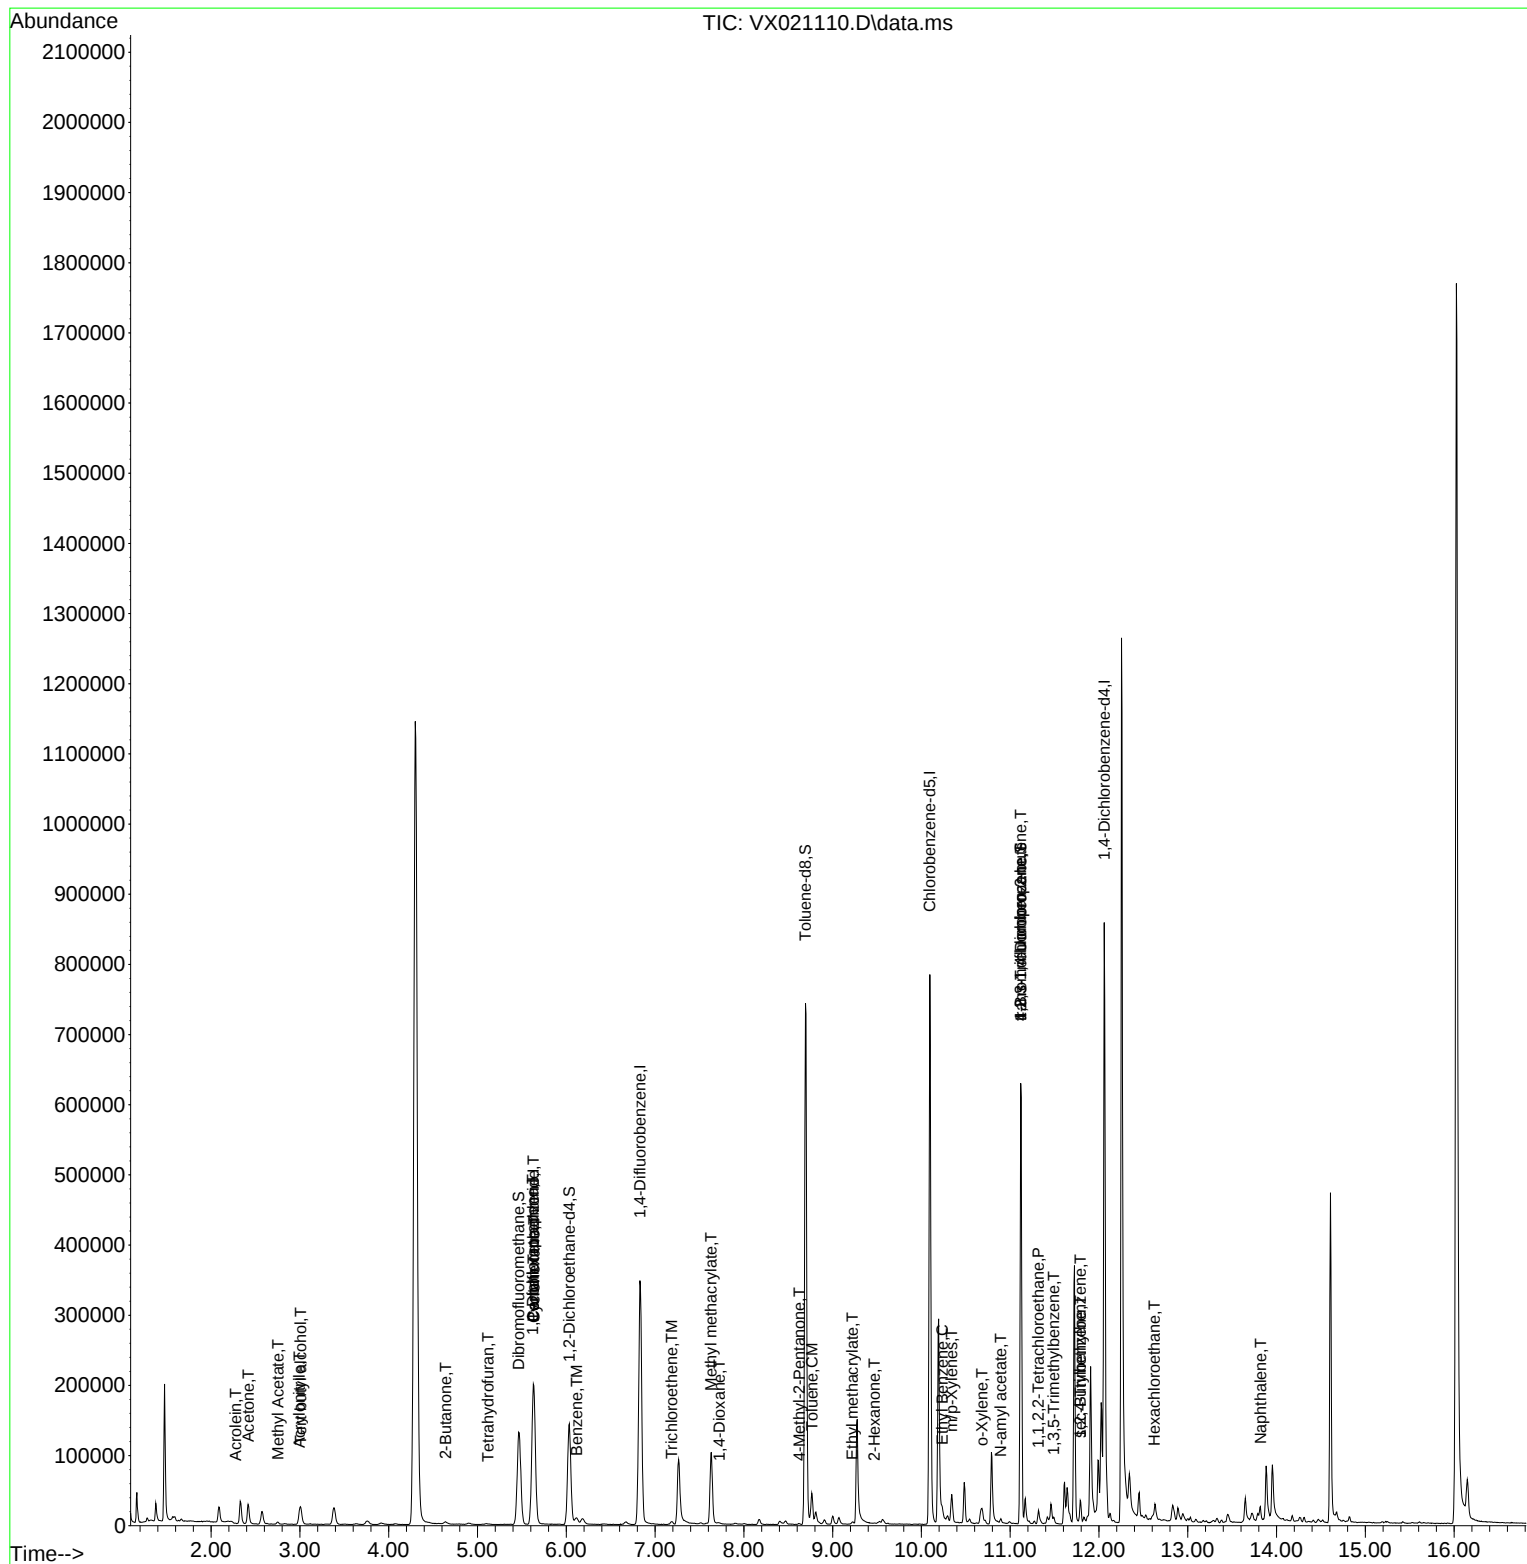




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 772
Delta R.T. 0.006 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50




Instrument :
MSVOA_X
ClientSampleId :
COMP-1


Tgt Ion:168 Resp: 199130
Ion Ratio Lower Upper
168 100
99 55.4 45.8 68.6

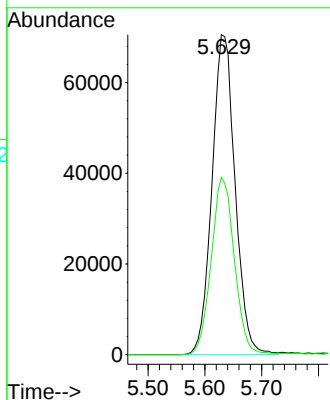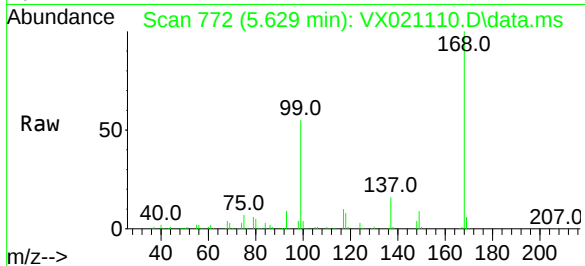

#5
Bromomethane
Concen: Below Cal
RT: 1.634 min Scan# 93
Delta R.T. 0.011 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50

Tgt Ion: 94 Resp: 390
Ion Ratio Lower Upper
94 100
96 59.2 76.4 114.6#


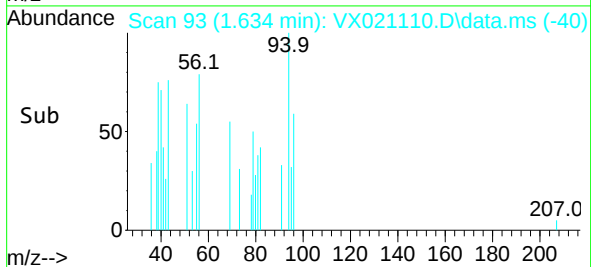
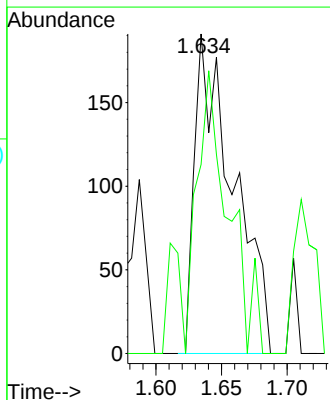
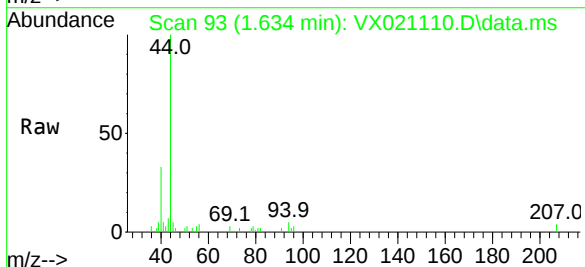




#11
Tert butyl alcohol
Concen: 49.68 ug/l
RT: 3.005 min Scan# 326
Delta R.T. -0.012 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50




Instrument :
MSVOA_X
ClientSampled :
COMP-1


Tgt Ion: 59 Resp: 29755
Ion Ratio Lower Upper
59 100
57 10.2 7.8 11.8



#13
Acrolein
Concen: 1.14 ug/l
RT: 2.276 min Scan# 202
Delta R.T. -0.000 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50


Tgt Ion: 56 Resp: 421
Ion Ratio Lower Upper
56 100
55 42.0 56.4 84.6#

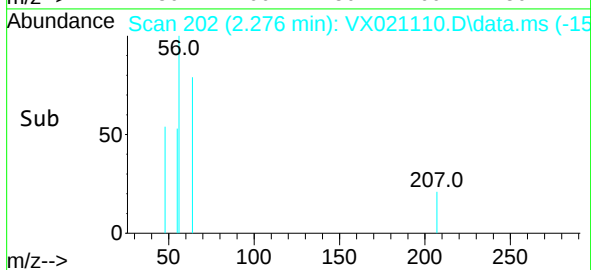






#15
Acrylonitrile
Concen: 0.31 ug/l
RT: 2.993 min Scan# 324
Delta R.T. -0.124 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50

Instrument :
MSVOA_X
ClientSampled :
COMP-1







Tgt Ion: 53	Resp: 399
Ion Ratio	Lower Upper
53	100
52	10.3 65.3 97.9#
51	103.8 28.2 42.2#



#16
Acetone
Concen: 25.48 ug/l
RT: 2.417 min Scan# 226
Delta R.T. -0.006 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50

Tgt Ion: 43	Resp: 28235
Ion Ratio	Lower Upper
43	100
58	34.9 27.8 41.8


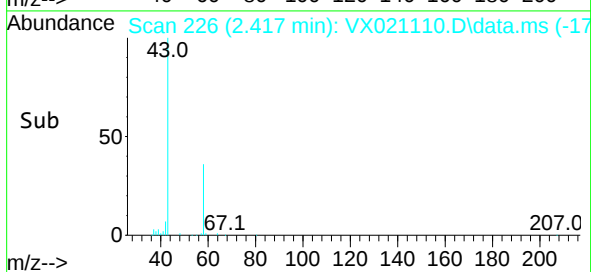




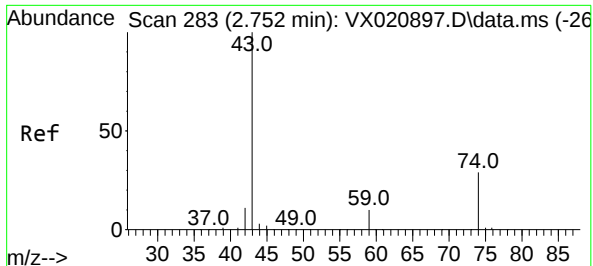

#18
Methyl Acetate
Concen: 1.38 ug/l
RT: 2.752 min Scan# 283
Delta R.T. -0.000 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50




Instrument :
MSVOA_X
ClientSampled :
COMP-1


Tgt Ion: 43 Resp: 3621
Ion Ratio Lower Upper
43 100
74 30.3 21.9 32.9

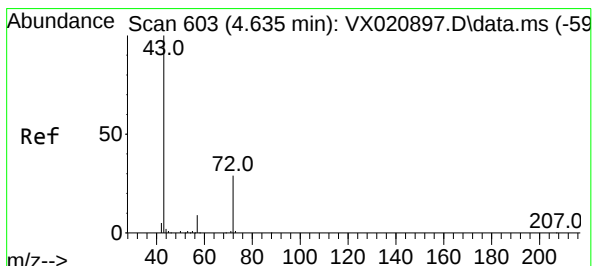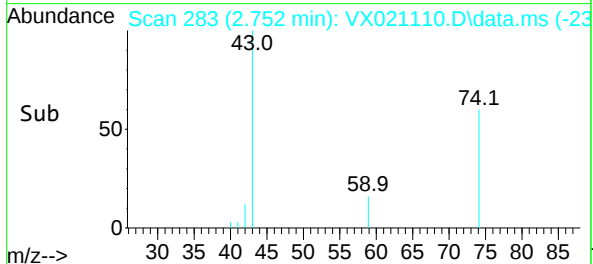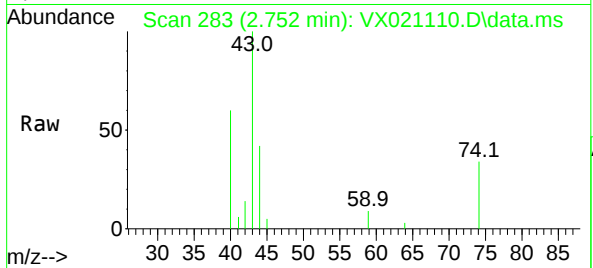

#25
2-Butanone
Concen: 3.21 ug/l
RT: 4.641 min Scan# 604
Delta R.T. 0.006 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50

Tgt Ion: 43 Resp: 5402
Ion Ratio Lower Upper
43 100
72 36.6 23.7 35.5#

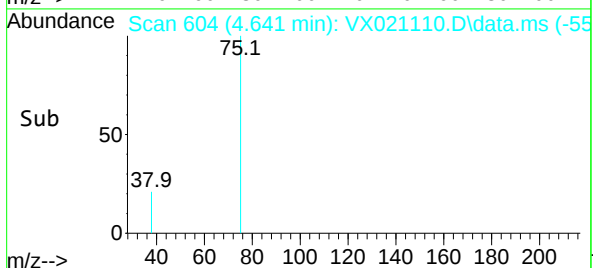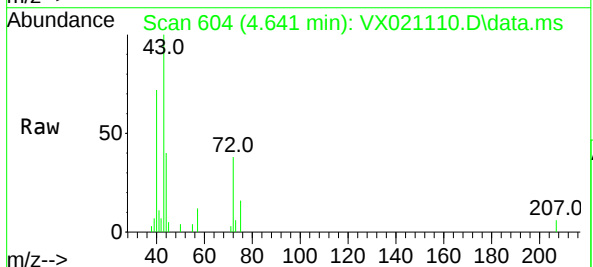



#29

Tetrahydrofuran

Concen: 0.35 ug/l

RT: 5.117 min Scan# 685

Delta R.T. 0.029 min

Lab File: VX021110.D

Acq: 09 Mar 2021 15:50





Instrument :

MSVOA_X

ClientSampleId :

COMP-1

Tgt Ion:	42	Resp:	380
Ion	Ratio	Lower	Upper
42	100		
72	5.0	41.7	62.5#
71	0.0	38.4	57.6#

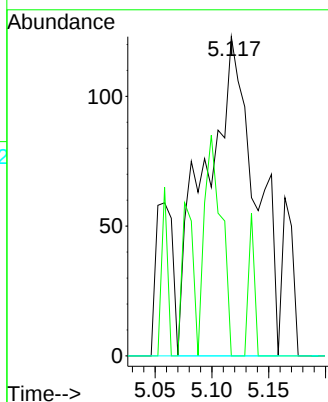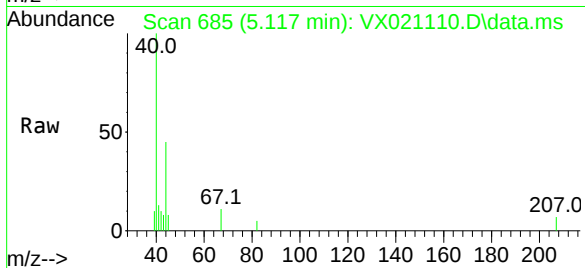

#31

Cyclohexane

Concen: 1.02 ug/l




RT: 5.635 min Scan# 773


Delta R.T. 0.088 min

Lab File: VX021110.D

Acq: 09 Mar 2021 15:50

Tgt Ion:	56	Resp:	3962
Ion	Ratio	Lower	Upper
56	100		
69	166.5	25.3	37.9#
84	168.1	71.4	107.0#


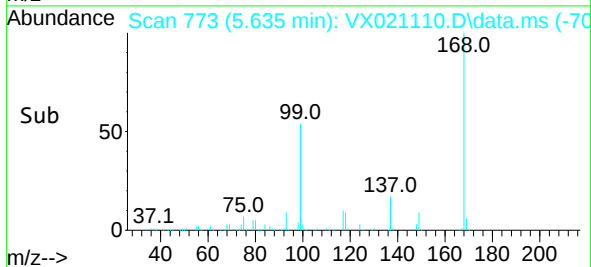
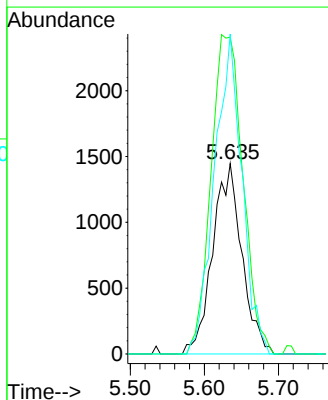
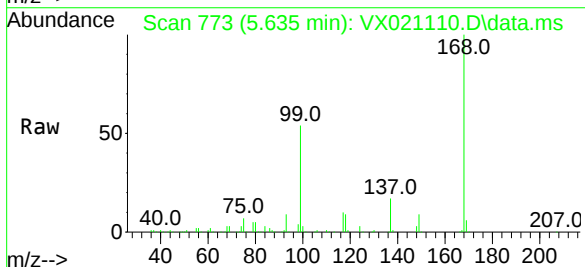




#33
1,2-Dichloroethane-d4
Concen: 50.22 ug/l
RT: 6.035 min Scan# 841
Delta R.T. 0.006 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50




Instrument :
MSVOA_X
ClientSampleId :
COMP-1


Tgt Ion: 65 Resp: 135074
Ion Ratio Lower Upper
65 100
67 52.7 0.0 105.4



#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.829 min Scan# 976
Delta R.T. -0.000 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50

Tgt Ion: 114 Resp: 366283
Ion Ratio Lower Upper
114 100
63 20.2 0.0 40.8
88 16.0 0.0 32.8

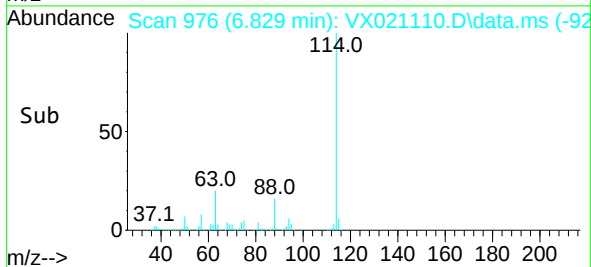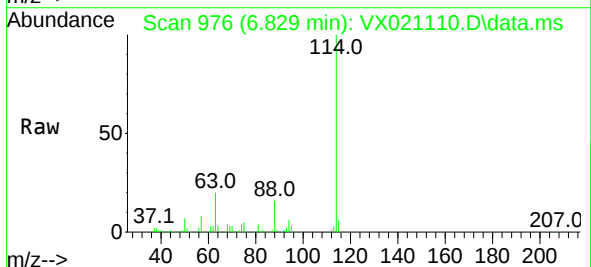

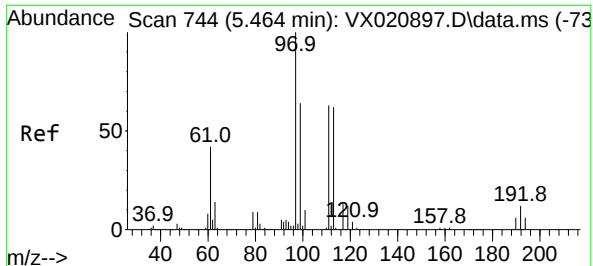

#35

Dibromofluoromethane

Concen: 52.88 ug/l

RT: 5.464 min Scan# 744

Delta R.T. -0.000 min

Lab File: VX021110.D

Acq: 09 Mar 2021 15:50





Tgt Ion:113 Resp: 117690

Ion Ratio Lower Upper

113 100

111 101.2 81.9 122.9

192 20.0 16.7 25.1

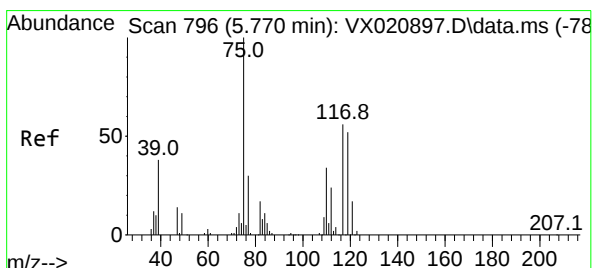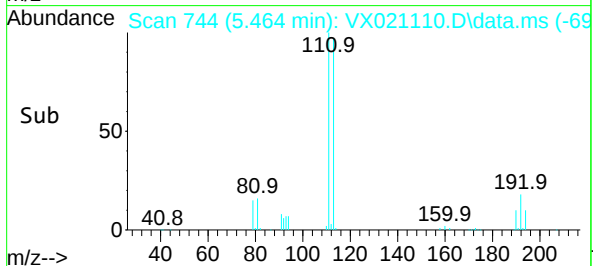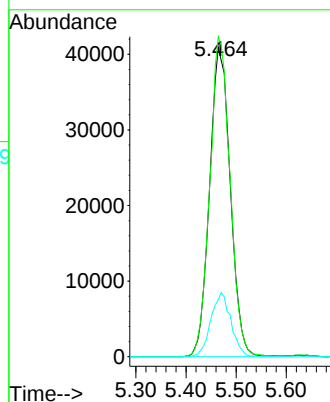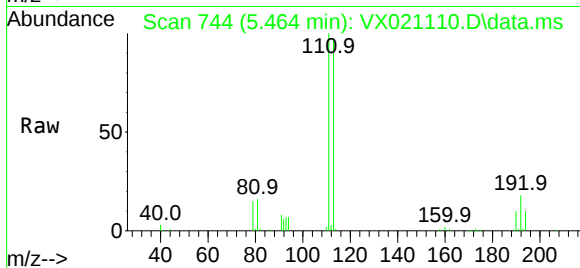

#36

1,1-Dichloropropene

Concen: 4.29 ug/l

RT: 5.623 min Scan# 771

Delta R.T. -0.147 min

Lab File: VX021110.D

Acq: 09 Mar 2021 15:50




Tgt Ion: 75 Resp: 14950


Ion Ratio Lower Upper

75 100

110 7.9 18.1 54.4#

77 0.0 25.3 37.9#


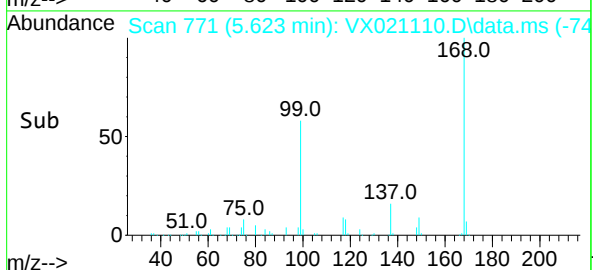
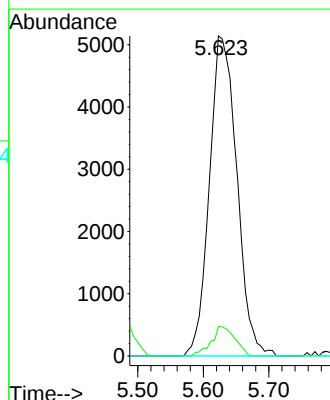
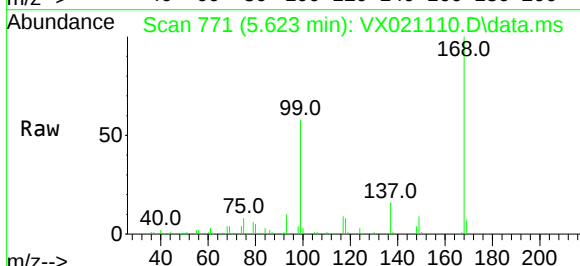


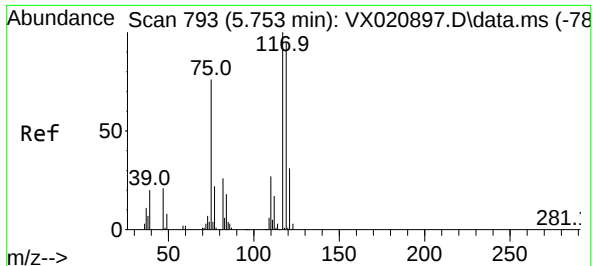

#38
Carbon Tetrachloride
Concen: 5.71 ug/l
RT: 5.629 min Scan# 772
Delta R.T. -0.124 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50




Instrument :
MSVOA_X
ClientSampled :
COMP-1


Tgt Ion:117 Resp: 19264
Ion Ratio Lower Upper
117 100
119 5.6 76.2 114.2#
121 0.0 24.8 37.2#

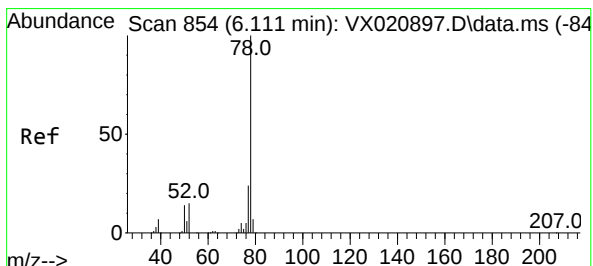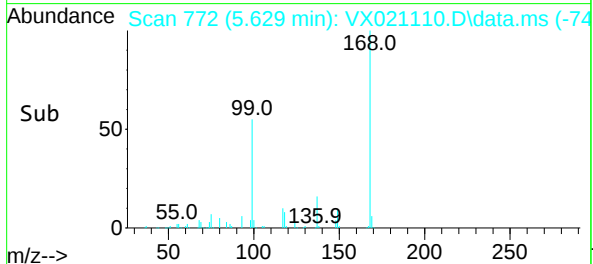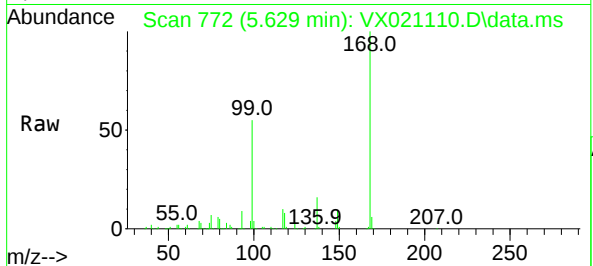

#40
Benzene
Concen: 1.09 ug/l
RT: 6.117 min Scan# 855
Delta R.T. 0.006 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50

Tgt Ion: 78 Resp: 11370
Ion Ratio Lower Upper
78 100
77 26.2 18.9 28.3


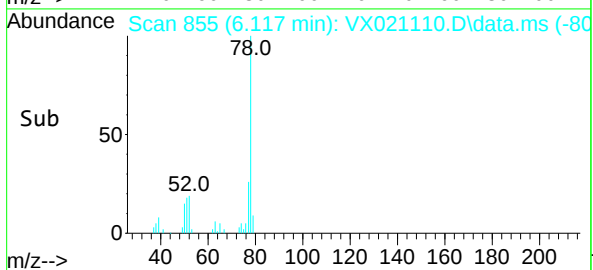

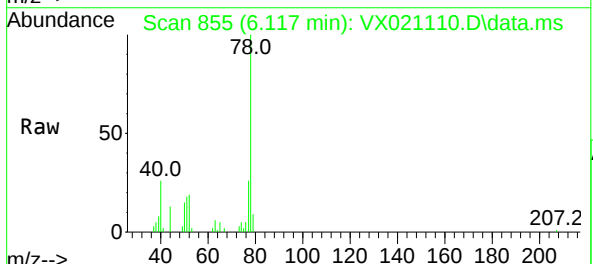


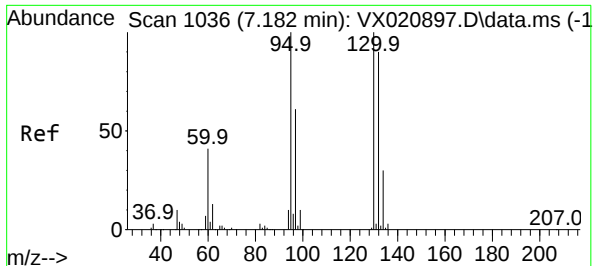

#44
Trichloroethene
Concen: 0.65 ug/l
RT: 7.188 min Scan# 1037
Delta R.T. 0.006 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50




Instrument :
MSVOA_X
ClientSampled :
COMP-1


Tgt Ion:130 Resp: 1790
Ion Ratio Lower Upper
130 100
95 104.0 0.0 198.0

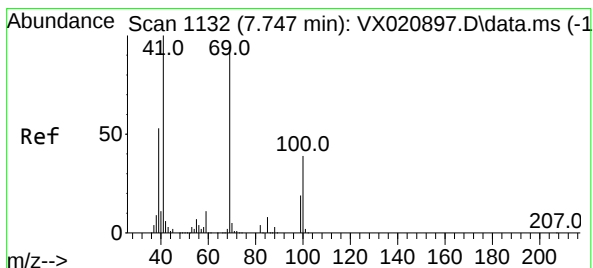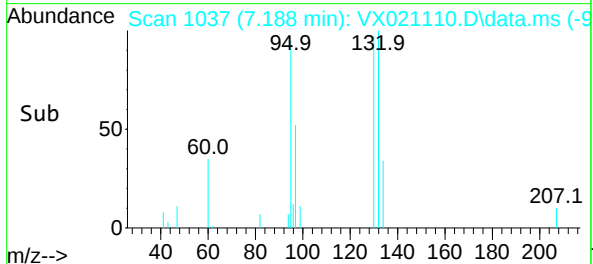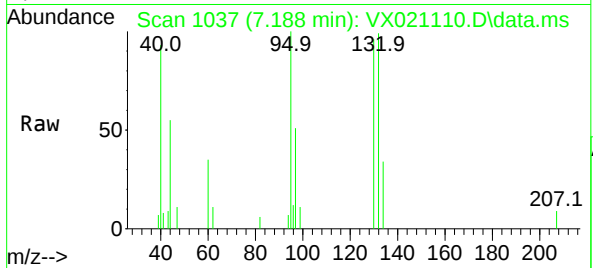

#48
Methyl methacrylate
Concen: 9.40 ug/l
RT: 7.629 min Scan# 1112
Delta R.T. -0.118 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50

Tgt Ion: 41 Resp: 26569
Ion Ratio Lower Upper
41 100
69 0.9 76.0 114.0#
39 48.9 44.6 67.0


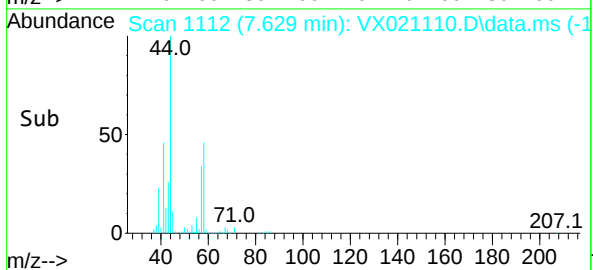

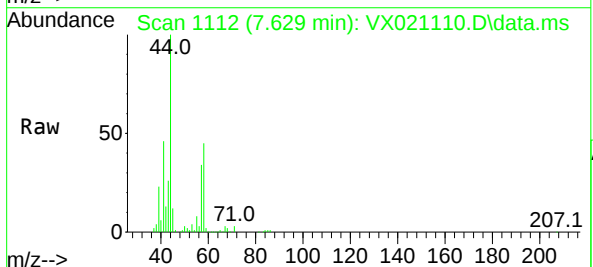


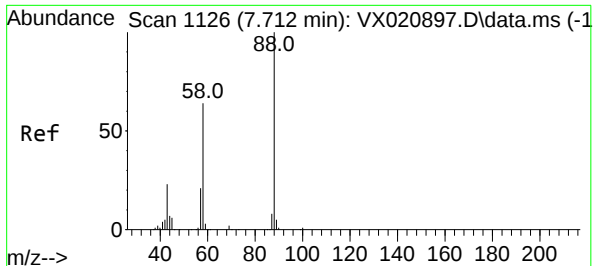

#49
1,4-Dioxane
Concen: 15.25 ug/l
RT: 7.723 min Scan# 1128
Delta R.T. 0.012 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50




Instrument :
MSVOA_X
ClientSampleId :
COMP-1


Tgt Ion: 88 Resp: 1006
Ion Ratio Lower Upper
88 100
43 61.4 23.2 34.8#
58 95.9 55.0 82.4#

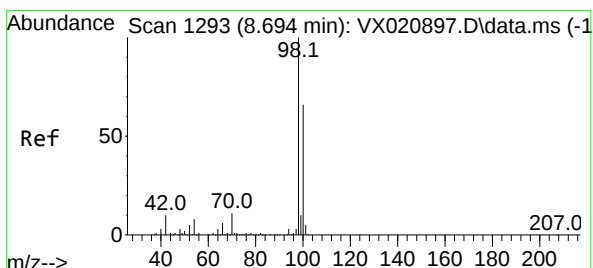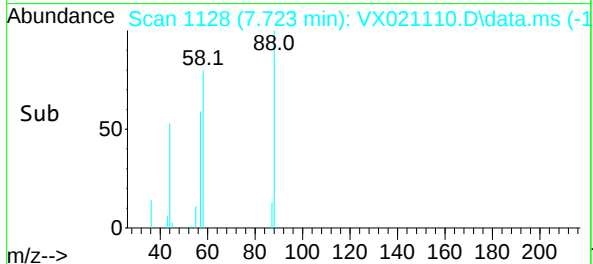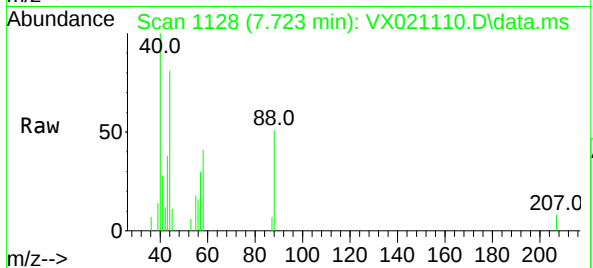

#50
Toluene-d8
Concen: 53.98 ug/l
RT: 8.694 min Scan# 1293
Delta R.T. -0.000 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50

Tgt Ion: 98 Resp: 468436
Ion Ratio Lower Upper
98 100
100 67.0 51.9 77.9


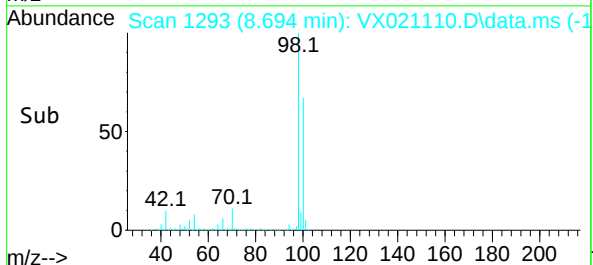

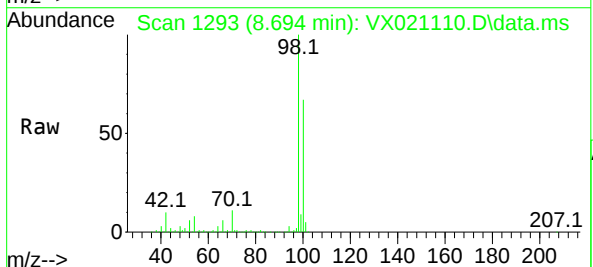




#51
4-Methyl-2-Pentanone
Concen: 0.25 ug/l
RT: 8.623 min Scan# 1281
Delta R.T. 0.006 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50




Instrument :
MSVOA_X
ClientSampleId :
COMP-1


Tgt Ion: 43 Resp: 809
Ion Ratio Lower Upper
43 100
58 45.7 35.4 53.0



#52
Toluene
Concen: 2.44 ug/l
RT: 8.765 min Scan# 1305
Delta R.T. 0.000 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50

Tgt Ion: 92 Resp: 15877
Ion Ratio Lower Upper
92 100
91 171.9 137.1 205.7


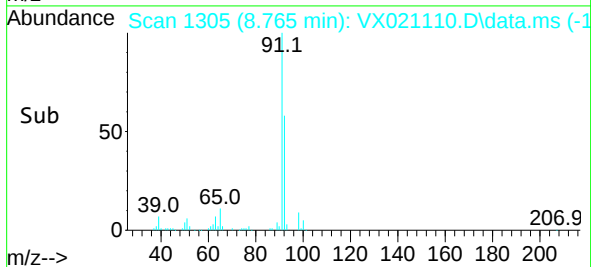

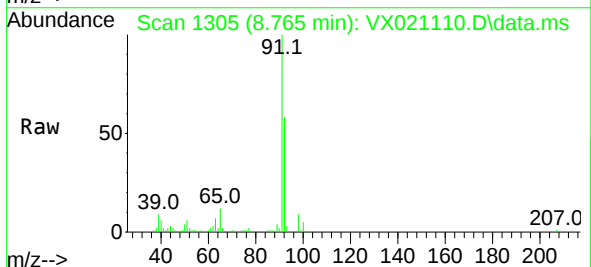




#56
Ethyl methacrylate
Concen: 0.22 ug/l
RT: 9.224 min Scan# 1383
Delta R.T. 0.065 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50




Instrument :
MSVOA_X
ClientSampleId :
COMP-1


Tgt Ion: 69 Resp: 905
Ion Ratio Lower Upper
69 100
41 0.0 46.8 70.2#
39 51.0 24.7 37.1#

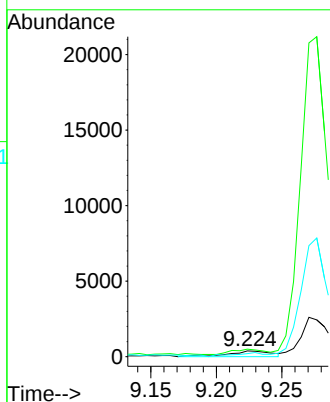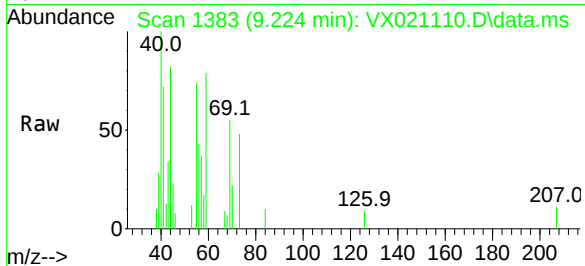

#59
2-Hexanone
Concen: 0.25 ug/l
RT: 9.471 min Scan# 1425
Delta R.T. -0.000 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50

Tgt Ion: 43 Resp: 603
Ion Ratio Lower Upper
43 100
58 68.2 30.9 92.8


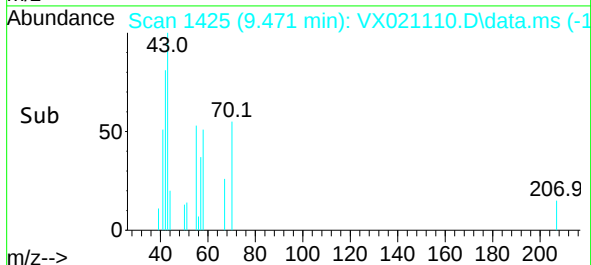
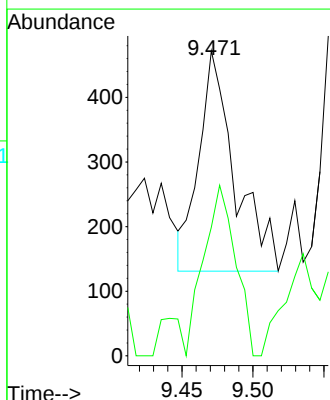
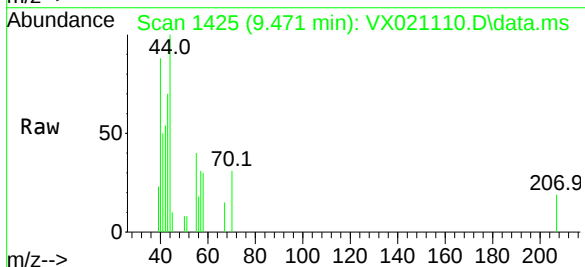




#62
4-Bromofluorobenzene
Concen: 55.54 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.000 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50




Instrument :
MSVOA_X
ClientSampleId :
COMP-1


Tgt Ion: 95 Resp: 178217
Ion Ratio Lower Upper
95 100
174 77.3 0.0 154.6
176 75.1 0.0 155.8



#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.094 min Scan# 1531
Delta R.T. 0.000 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50

Tgt Ion: 117 Resp: 367398
Ion Ratio Lower Upper
117 100
82 57.8 47.4 71.2
119 33.3 26.6 39.8


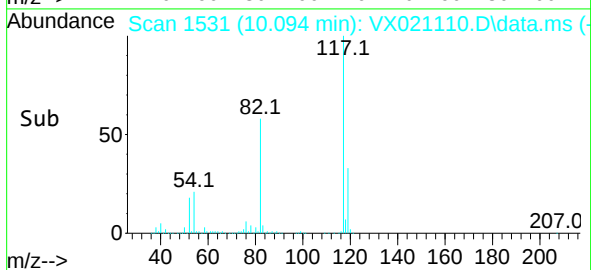




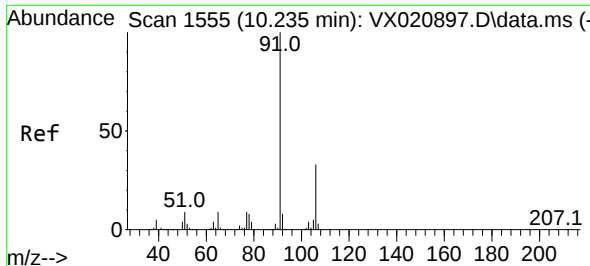

#67
Ethyl Benzene
Concen: 0.35 ug/l
RT: 10.235 min Scan# 1555
Delta R.T. -0.000 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50




Instrument :
MSVOA_X
ClientSampleId :
COMP-1


Tgt Ion: 91 Resp: 4867
Ion Ratio Lower Upper
91 100
106 33.9 24.6 37.0

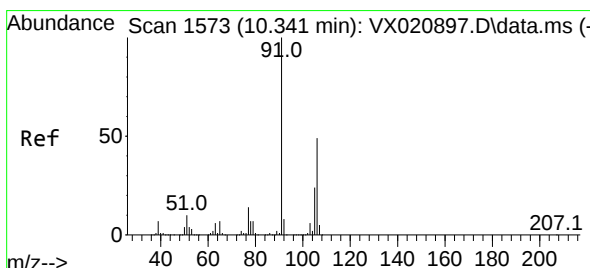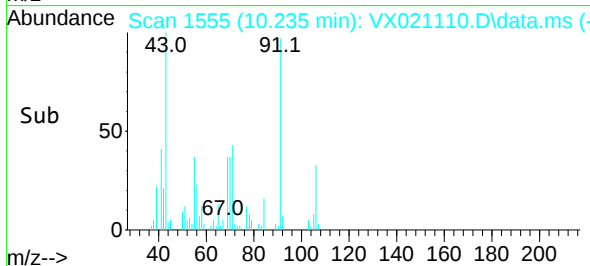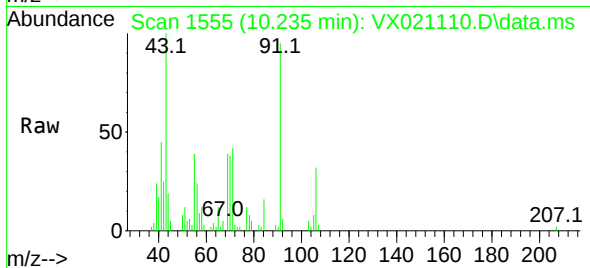

#68
m/p-Xylenes
Concen: 1.60 ug/l
RT: 10.341 min Scan# 1573
Delta R.T. -0.000 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50

Tgt Ion: 106 Resp: 8243
Ion Ratio Lower Upper
106 100
91 199.3 162.8 244.2


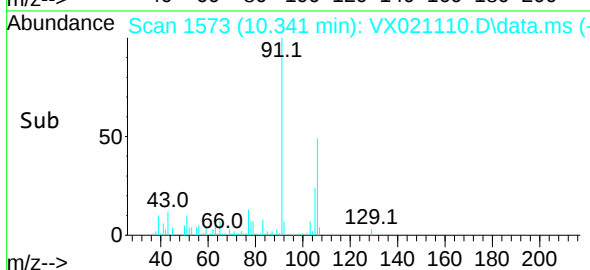

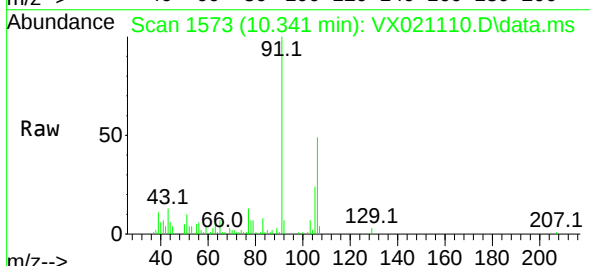




#69
o-Xylene
Concen: 0.73 ug/l
RT: 10.683 min Scan# 1631
Delta R.T. -0.000 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50




Instrument :
MSVOA_X
ClientSampled :
COMP-1


Tgt Ion:106 Resp: 3703
Ion Ratio Lower Upper
106 100
91 209.5 108.1 324.2

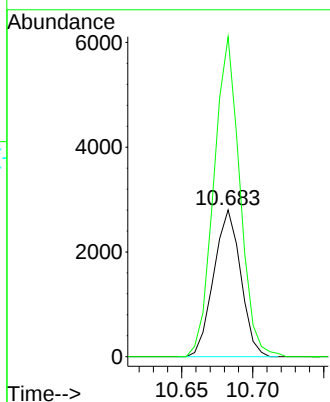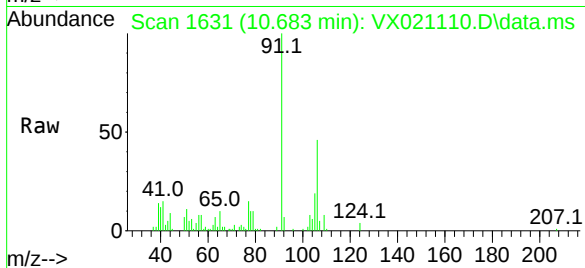

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.059 min Scan# 1865
Delta R.T. -0.006 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50


Tgt Ion:152 Resp: 175887
Ion Ratio Lower Upper
152 100
115 59.1 41.1 123.3
150 160.9 0.0 349.0

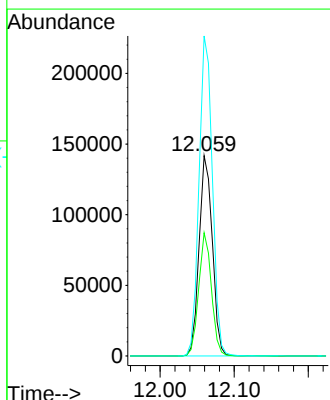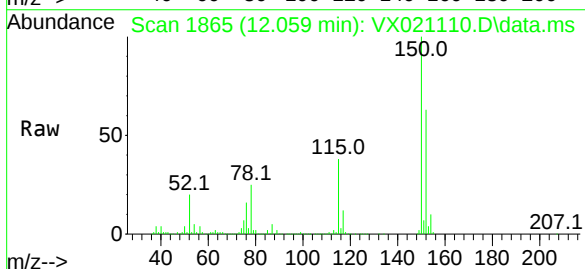



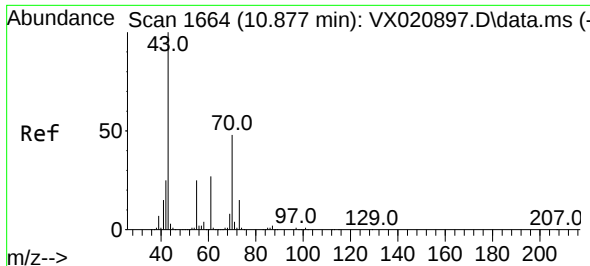


#74
N-amy1 acetate
Concen: 0.20 ug/l
RT: 10.894 min Scan# 1667
Delta R.T. 0.018 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50

Instrument :
MSVOA_X
ClientSampleId :
COMP-1



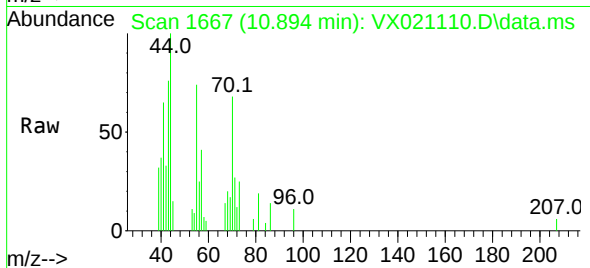



Tgt Ion: 43	Resp: 1137
Ion Ratio	Lower Upper
43 100	
70 95.2	39.0 58.6#
55 0.0	21.5 32.3#
61 0.0	22.1 33.1#

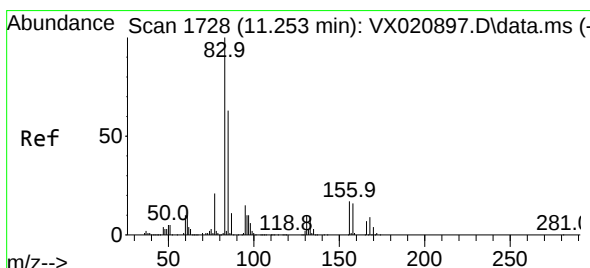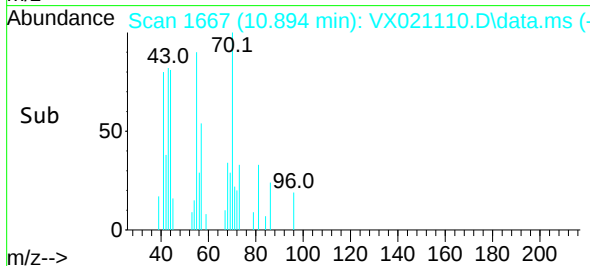

#75
1,1,2,2-Tetrachloroethane
Concen: 0.43 ug/l
RT: 11.318 min Scan# 1739
Delta R.T. 0.065 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50

Tgt Ion: 83	Resp: 1919
Ion Ratio	Lower Upper
83 100	
131 0.0	5.1 15.2#
85 0.0	31.8 95.4#


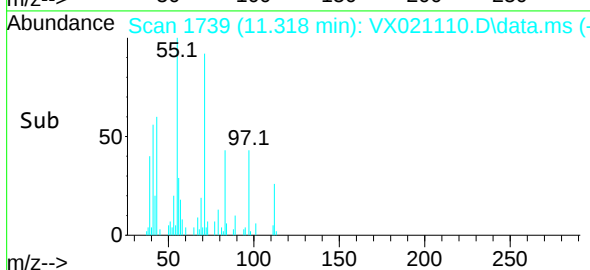

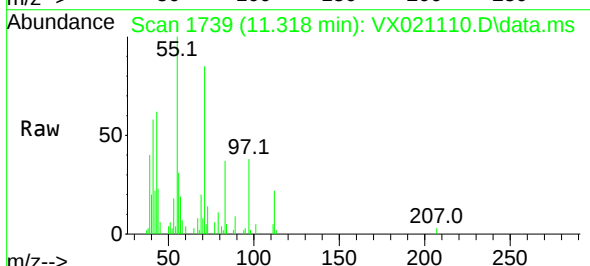


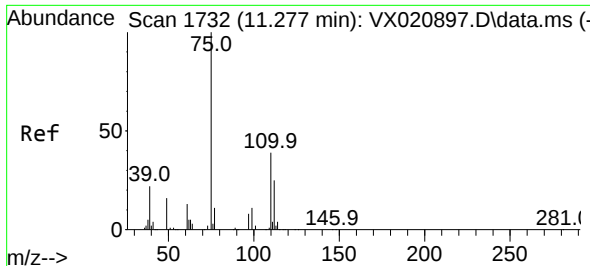

#76
1,2,3-Trichloropropane
Concen: 22.65 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.159 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50




Instrument :
MSVOA_X
ClientSampled :
COMP-1


Tgt Ion: 75 Resp: 85701
Ion Ratio Lower Upper
75 100
77 1.3 19.1 57.5#

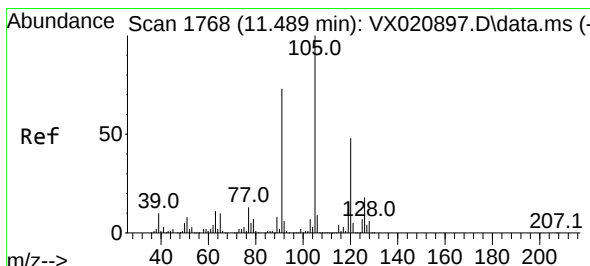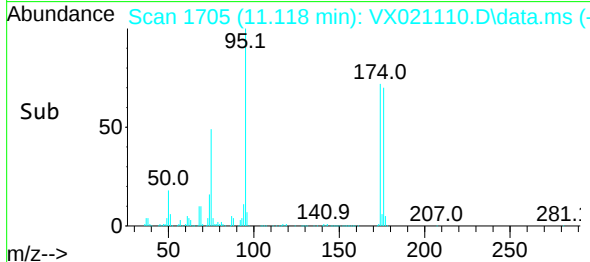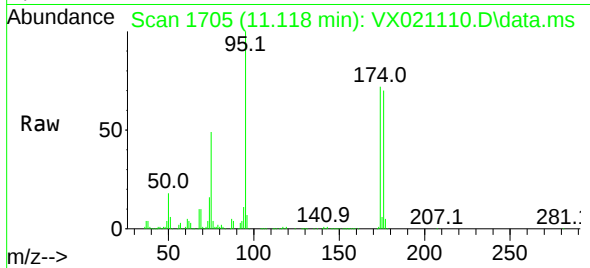

#80
1,3,5-Trimethylbenzene
Concen: 0.23 ug/l
RT: 11.489 min Scan# 1768
Delta R.T. 0.000 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50

Tgt Ion: 105 Resp: 2634
Ion Ratio Lower Upper
105 100
120 53.0 23.8 71.5


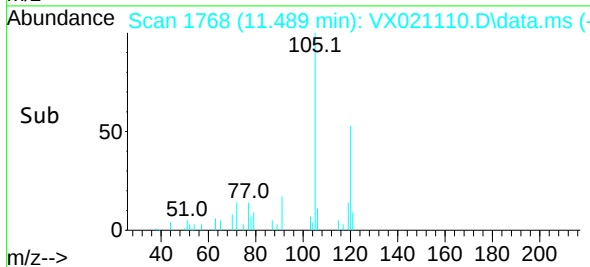

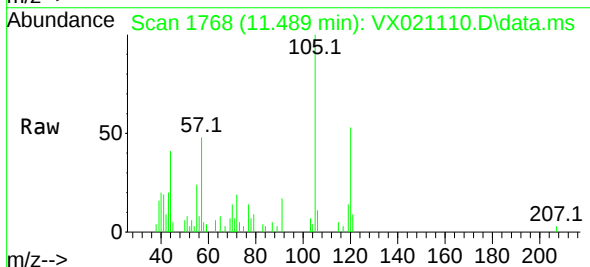




#81
trans-1,4-Dichloro-2-butene
Concen: 50.15 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. 0.059 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50




Instrument :
MSVOA_X
ClientSampleId :
COMP-1


Tgt Ion: 75 Resp: 85701
Ion Ratio Lower Upper
75 100
53 0.1 74.5 111.7#
89 0.0 37.9 56.9#

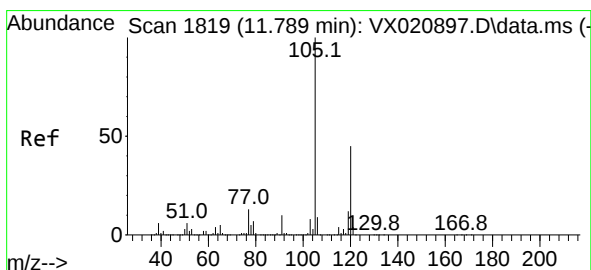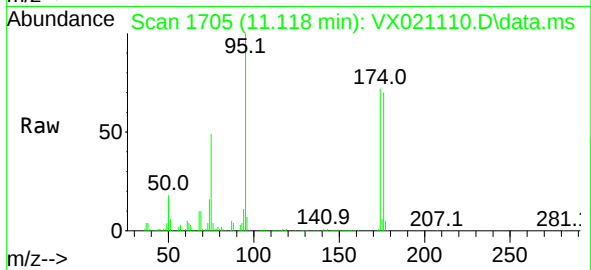

#84
1,2,4-Trimethylbenzene
Concen: 1.09 ug/l
RT: 11.789 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50

Tgt Ion: 105 Resp: 12732
Ion Ratio Lower Upper
105 100
120 38.3 22.4 67.3




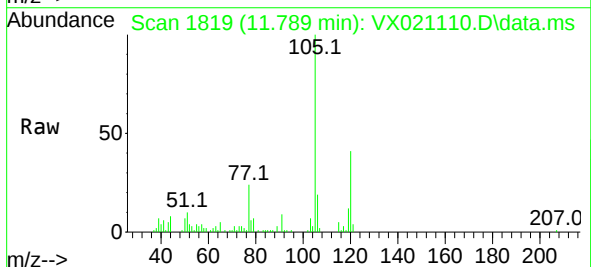




#85
 sec-Butylbenzene
 Concen: 0.96 ug/l
 RT: 11.789 min Scan# 1819
 Delta R.T. -0.141 min
 Lab File: VX021110.D
 Acq: 09 Mar 2021 15:50




Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-1


Tgt Ion:105 Resp: 12732
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.0 29.8#

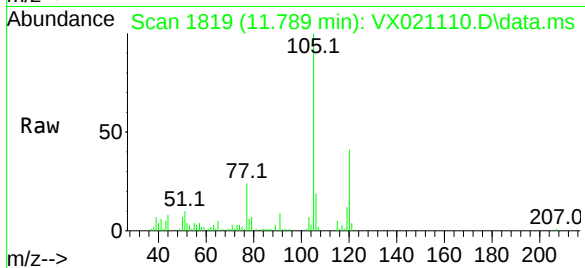

#90
 Hexachloroethane
 Concen: 0.27 ug/l
 RT: 12.624 min Scan# 1961
 Delta R.T. 0.047 min
 Lab File: VX021110.D
 Acq: 09 Mar 2021 15:50


Tgt Ion:117 Resp: 624
 Ion Ratio Lower Upper
 117 100
 201 0.0 40.4 121.2#

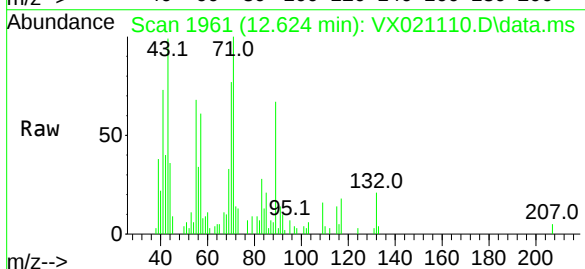

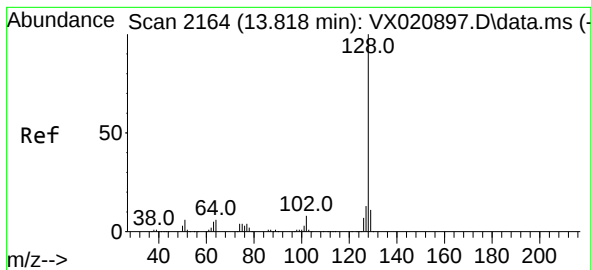

#95
Naphthalene
Concen: 0.88 ug/l
RT: 13.818 min Scan# 2164
Delta R.T. 0.000 min
Lab File: VX021110.D
Acq: 09 Mar 2021 15:50

Instrument :
MSVOA_X
ClientSampleId :
COMP-1

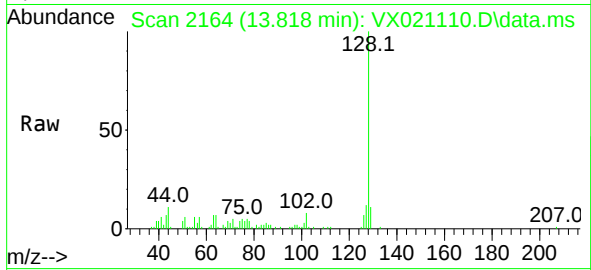

Tgt Ion:128 Resp: 11339
Ion Ratio Lower Upper
128 100
127 12.1 10.3 15.5
129 11.2 8.8 13.2

