

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030921\
 Data File : VX021107.D
 Acq On : 09 Mar 2021 14:48
 Operator : JC/MD
 Sample : M1611-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB-01-030921

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M

Title : SW846 8260

Signal : TIC: VX021107.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.417	220	226	236	rBV	8694	16207	1.30%	0.257%
2	2.576	245	253	264	rBV	7370	15758	1.26%	0.250%
3	2.840	291	298	305	rVB2	9865	19326	1.55%	0.307%
4	5.470	733	745	761	rBV2	135606	391753	31.40%	6.216%
5	5.629	761	772	793	rBV	211061	590013	47.29%	9.362%
6	6.035	829	841	857	rBV	147355	388649	31.15%	6.167%
7	6.835	966	977	996	rBV	356572	873025	69.98%	13.852%
8	8.700	1286	1294	1312	rBV	773141	1247558	100.00%	19.795%
9	10.094	1525	1531	1548	rBV	791438	1074364	86.12%	17.047%
10	11.118	1700	1705	1717	rBV	603381	793696	63.62%	12.594%
11	12.059	1860	1865	1875	rBV	712299	892069	71.51%	14.154%




Sum of corrected areas: 6302418

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030921\
Data File : VX021107.D
Acq On : 09 Mar 2021 14:48
Operator : JC/MD
Sample : M1611-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-01-030921

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

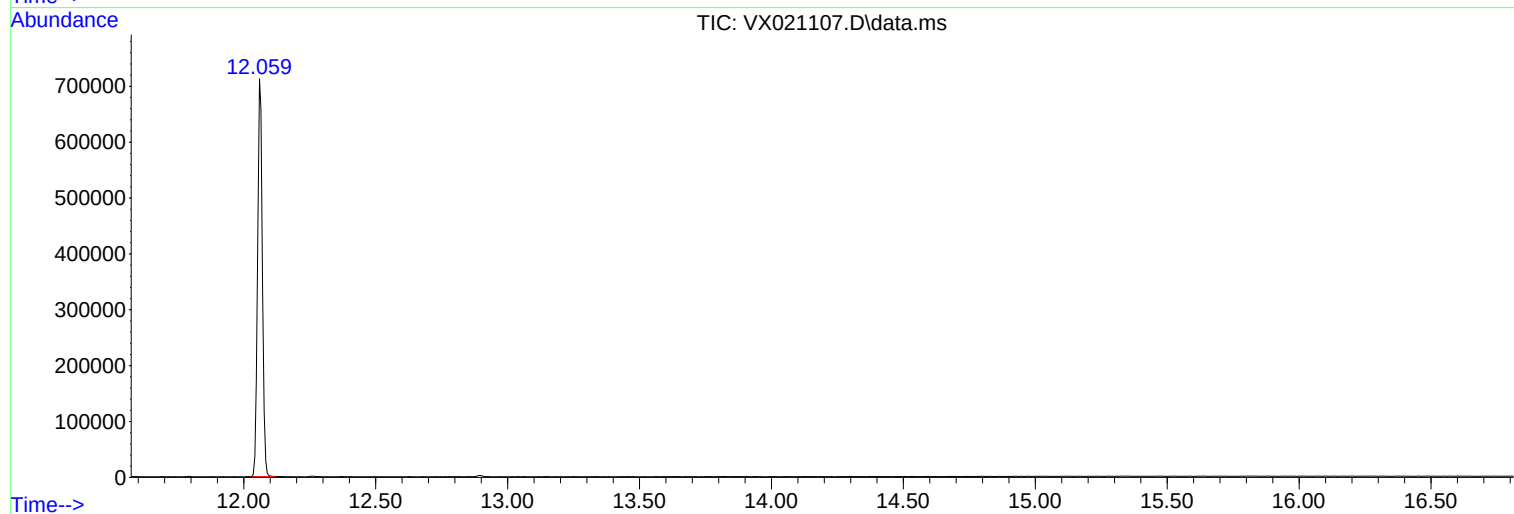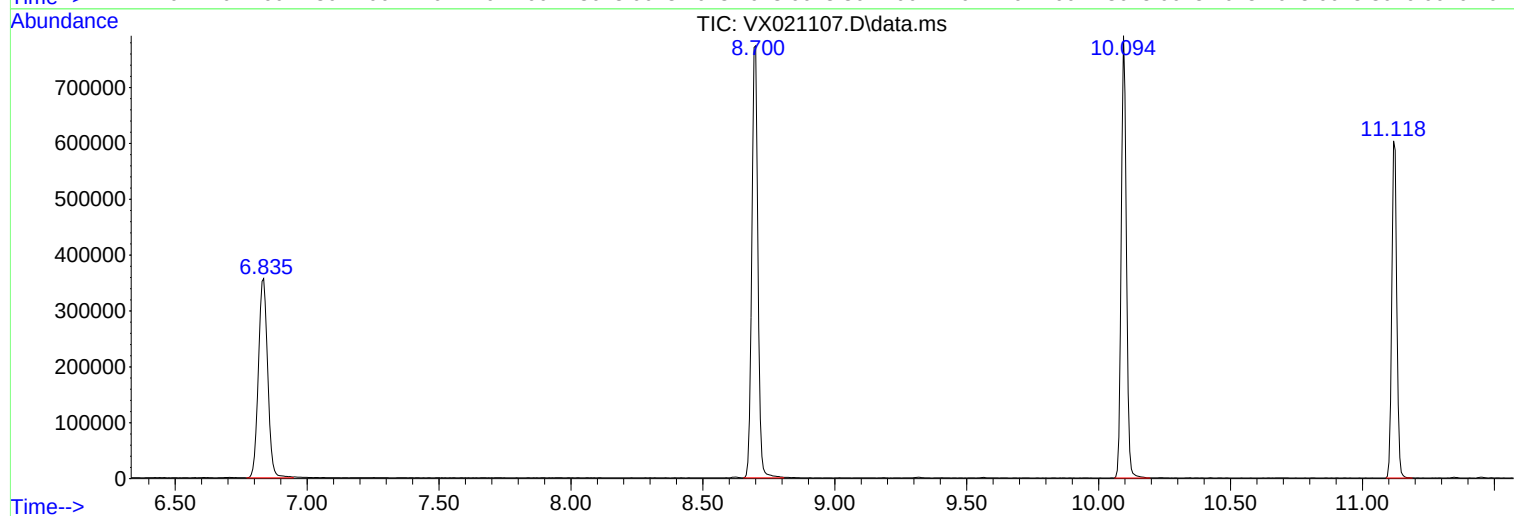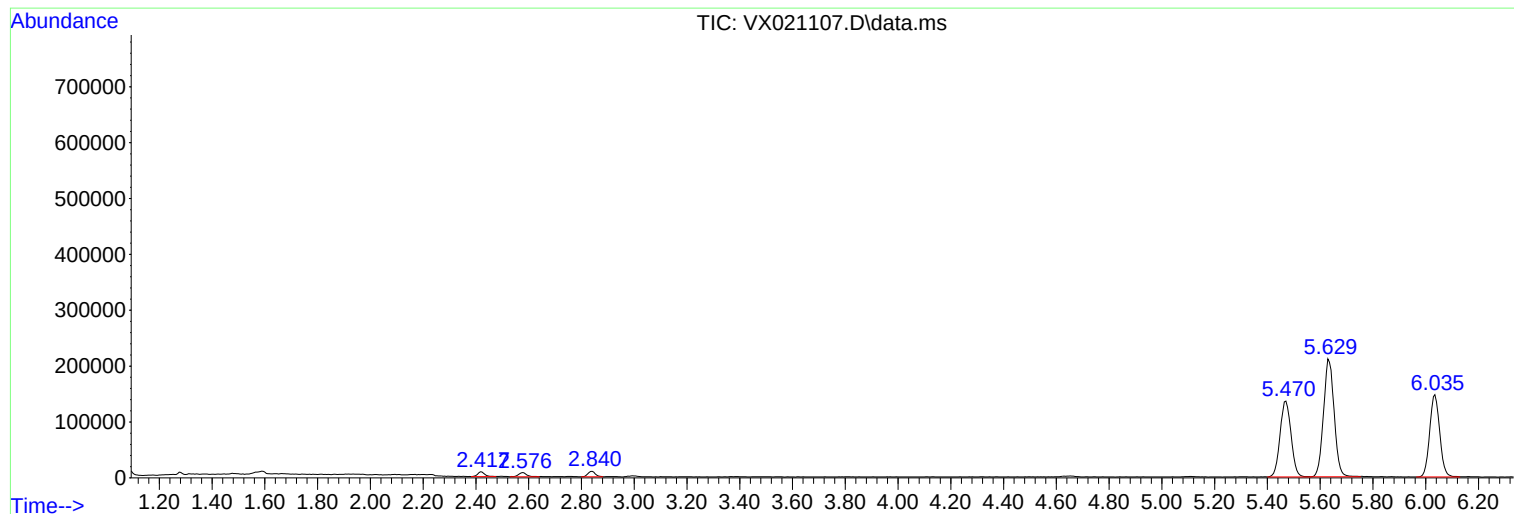

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030921\
Data File : VX021107.D
Acq On : 09 Mar 2021 14:48
Operator : JC/MD
Sample : M1611-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-01-030921

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030921\
Data File : VX021107.D
Acq On : 09 Mar 2021 14:48
Operator : JC/MD
Sample : M1611-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-01-030921

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
