
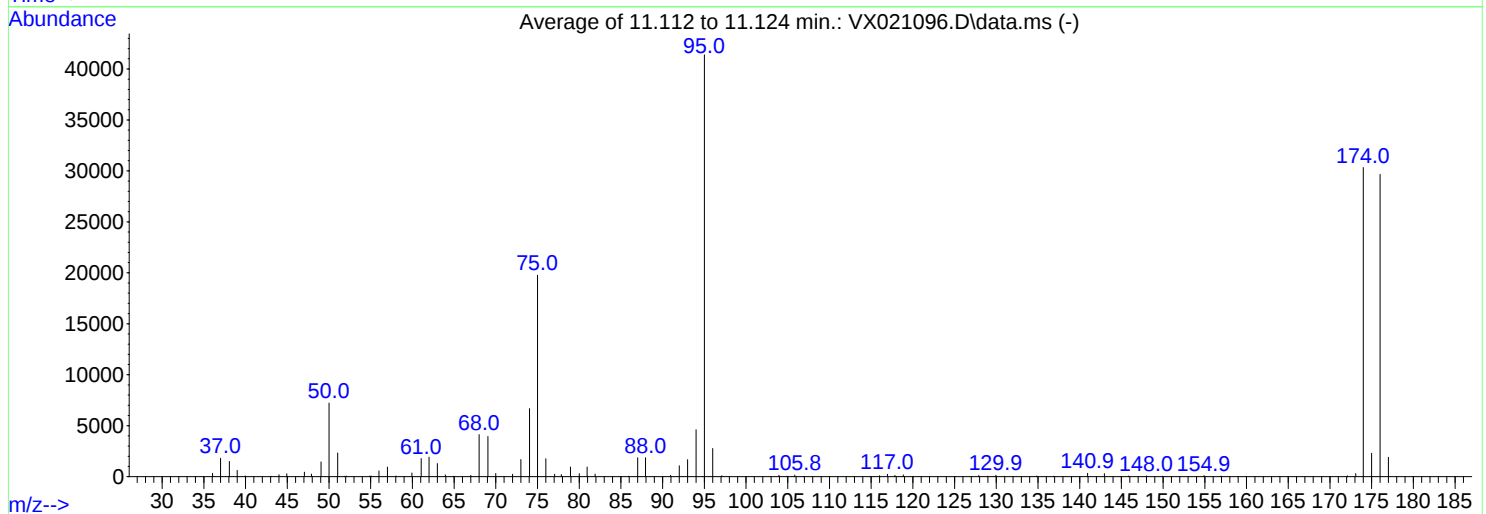


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030921\
 Data File : VX021096.D
 Acq On : 09 Mar 2021 09:17
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
 Title : SW846 8260
 Last Update : Wed Feb 24 13:50:55 2021

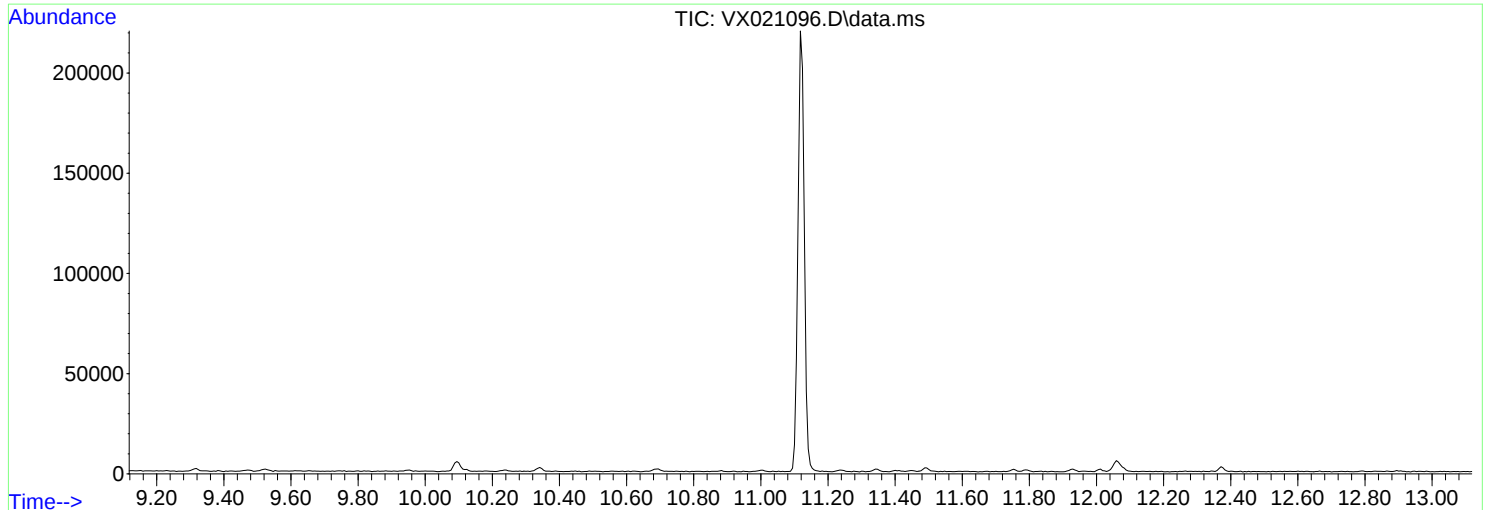

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1698

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	7225	PASS
75	95	30	60	47.8	19763	PASS
95	95	100	100	100.0	41387	PASS
96	95	5	9	6.7	2765	PASS
173	174	0.00	2	1.0	295	PASS
174	95	50	100	73.3	30339	PASS
175	174	5	9	7.6	2300	PASS
176	174	95	101	97.8	29664	PASS
177	176	5	9	6.4	1896	PASS