

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030922\
 Data File : VX027359.D
 Acq On : 09 Mar 2022 19:01
 Operator : JC/MD
 Sample : N1800-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANAG

Quant Time: Mar 10 00:36:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 08 15:54:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	402785	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	652150	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	598218	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	270386	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	206739	44.014	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	88.020%
35) Dibromofluoromethane	5.391	113	202990	48.238	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	96.480%
50) Toluene-d8	8.653	98	762504	47.997	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	96.000%
62) 4-Bromofluorobenzene	11.079	95	275605	45.518	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	91.040%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030922\
Data File : VX027359.D
Acq On : 09 Mar 2022 19:01
Operator : JC/MD
Sample : N1800-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Time: Mar 10 00:36:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 08 15:54:34 2022
Response via : Initial Calibration




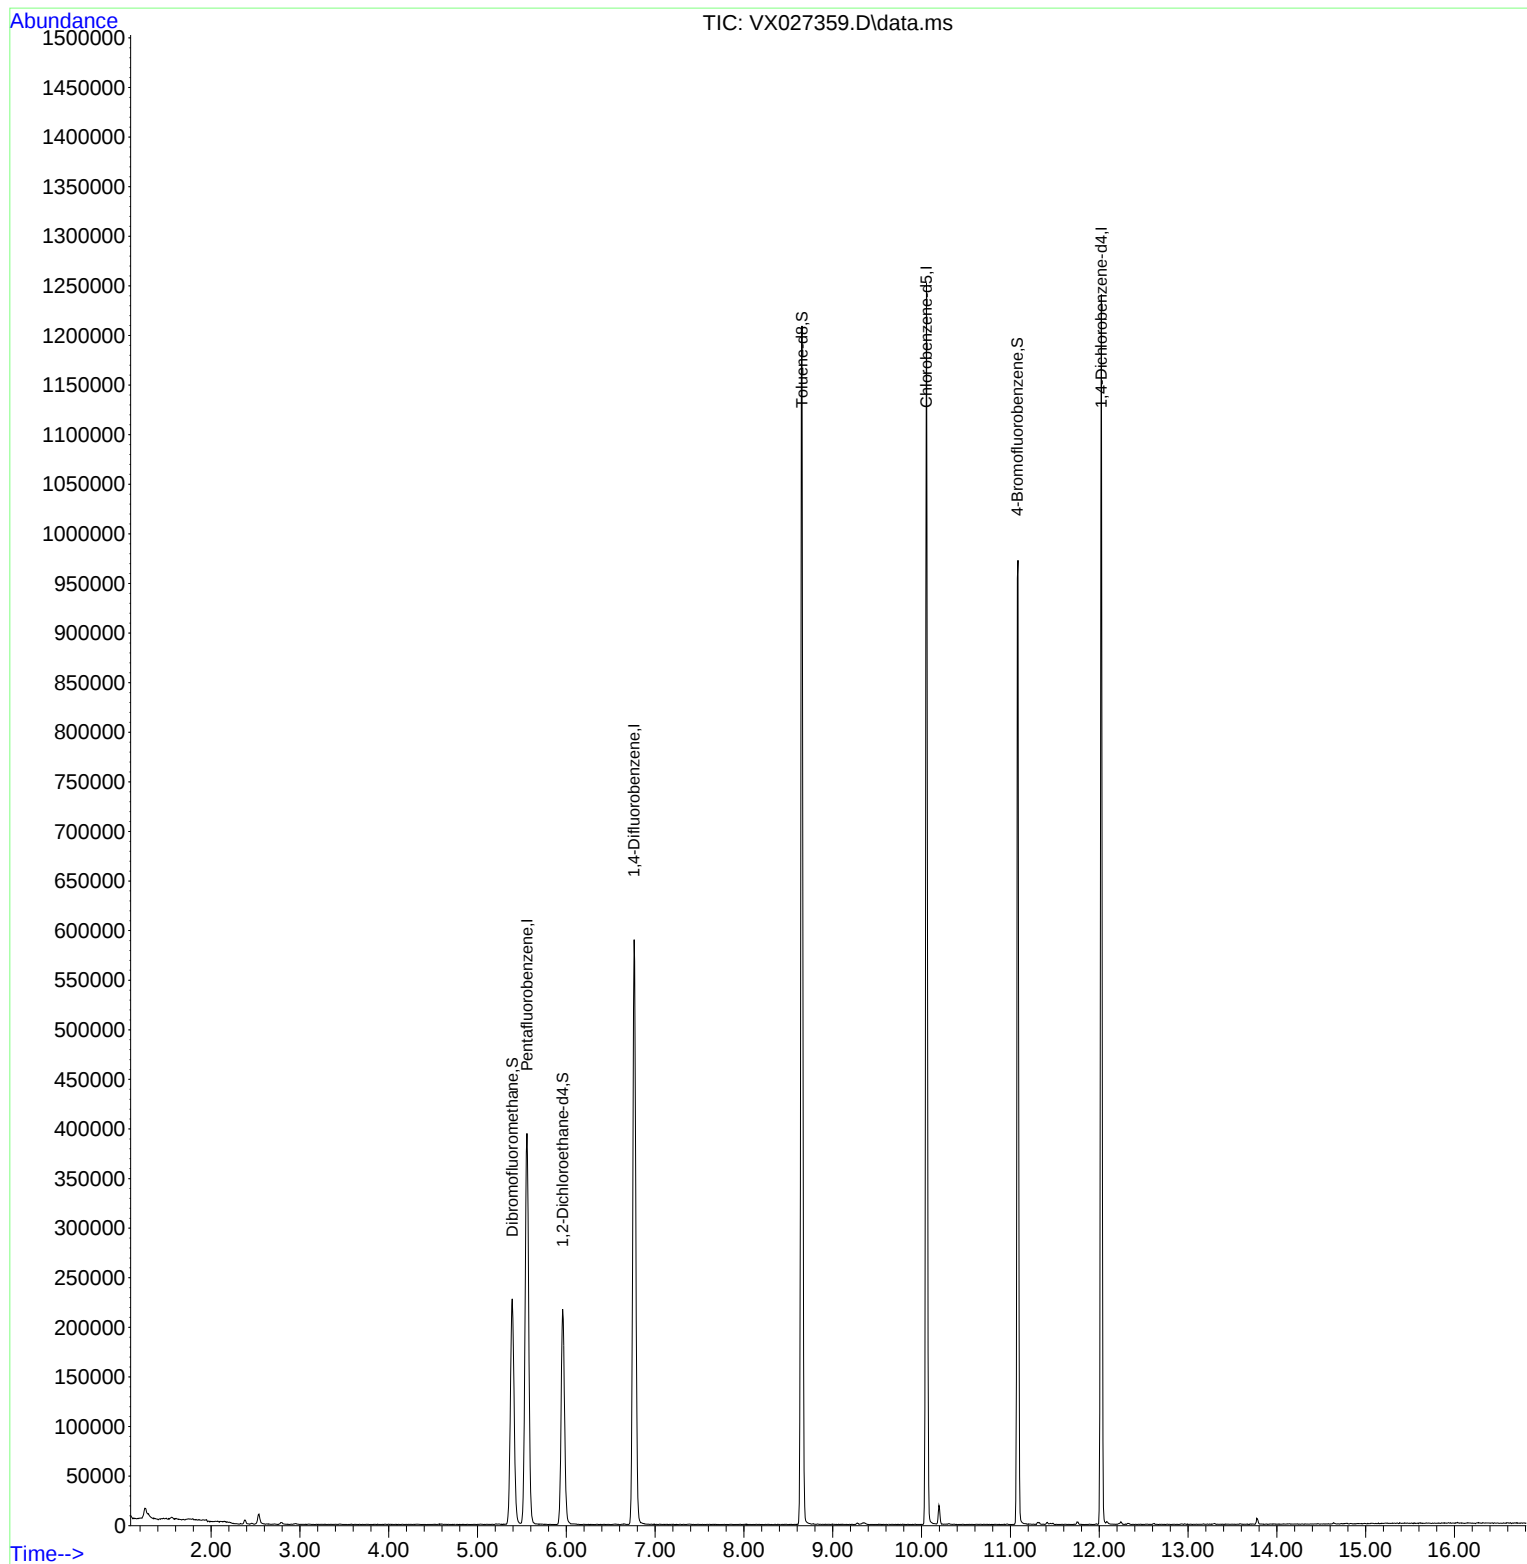


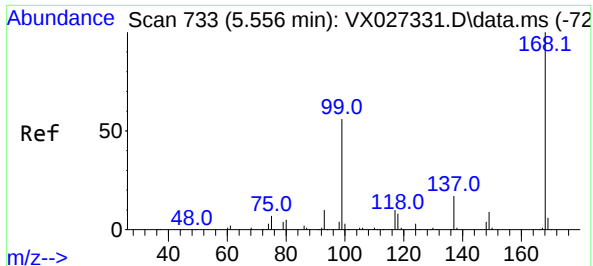

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 713
Delta R.T. -0.000 min
Lab File: VX027359.D
Acq: 09 Mar 2022 19:01




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion:168 Resp: 402785
Ion Ratio Lower Upper
168 100
99 52.9 41.7 62.5

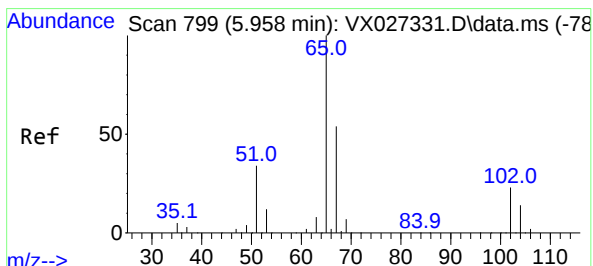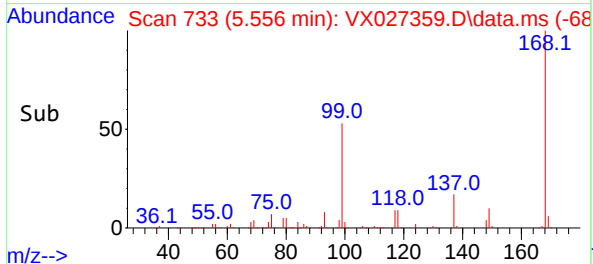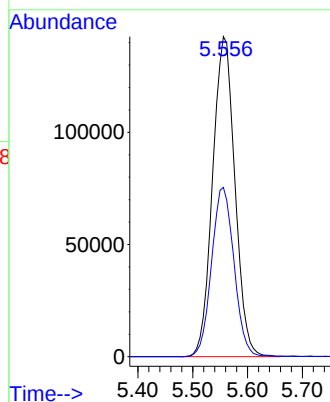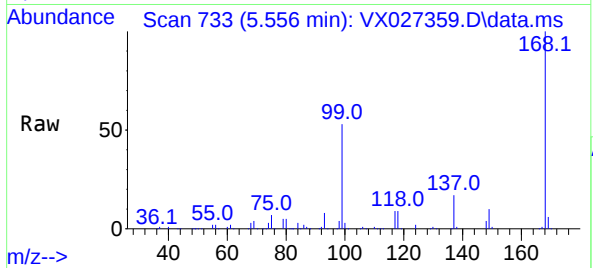

#33
1,2-Dichloroethane-d4
Concen: 44.014 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX027359.D
Acq: 09 Mar 2022 19:01

Tgt Ion: 65 Resp: 206739
Ion Ratio Lower Upper
65 100
67 54.7 0.0 107.4


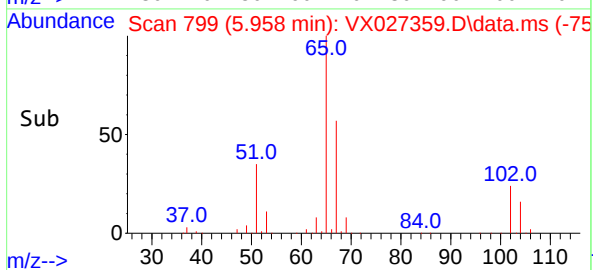
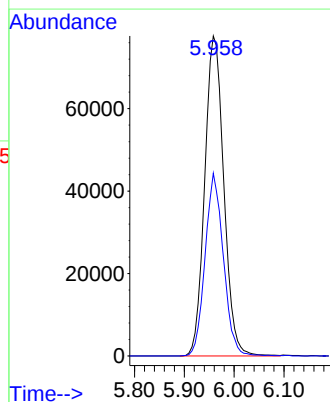
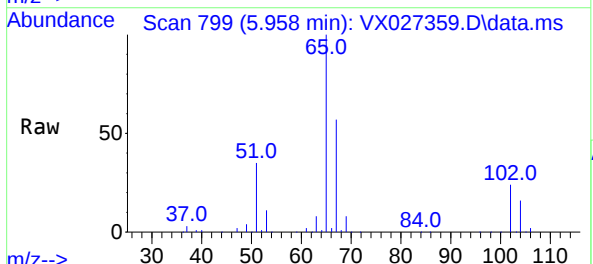


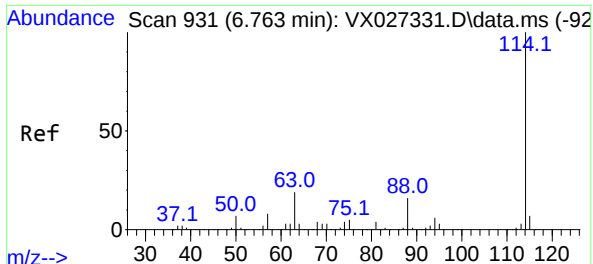

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX027359.D
Acq: 09 Mar 2022 19:01




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion:114 Resp: 652150
Ion Ratio Lower Upper
114 100
63 17.6 0.0 36.8
88 16.1 0.0 32.4

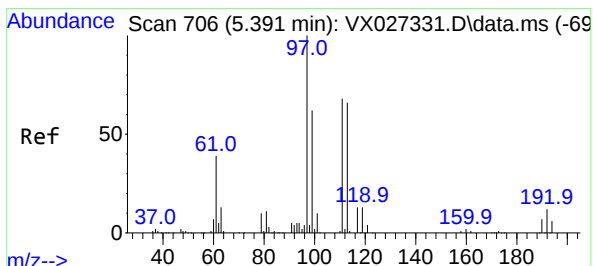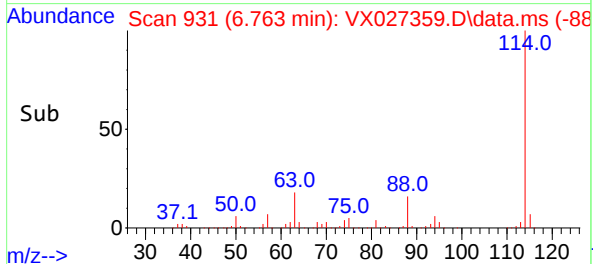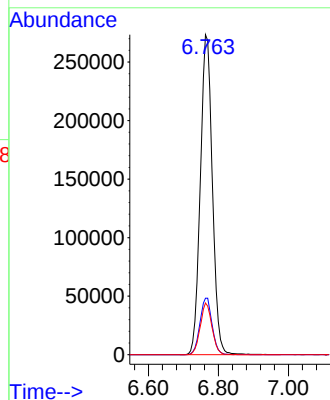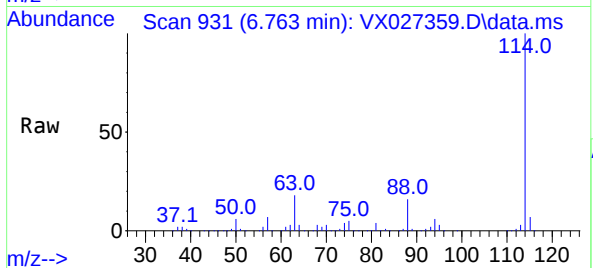

#35
Dibromofluoromethane
Concen: 48.238 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX027359.D
Acq: 09 Mar 2022 19:01

Tgt Ion:113 Resp: 202990
Ion Ratio Lower Upper
113 100
111 103.4 82.8 124.2
192 20.7 16.9 25.3


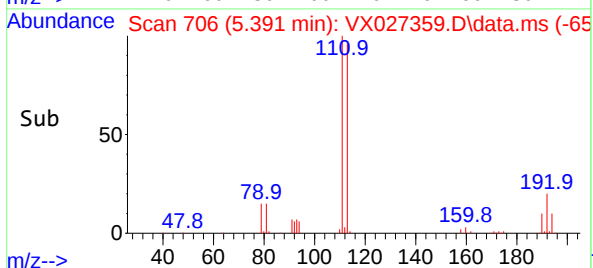
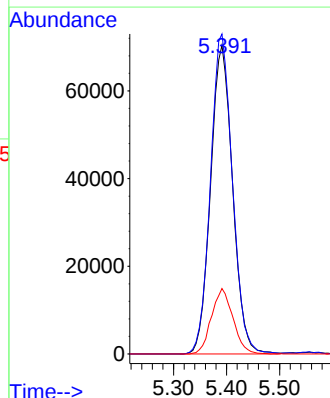
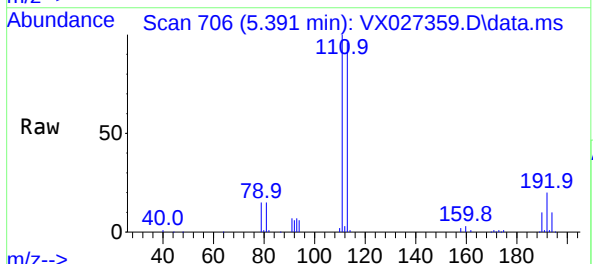


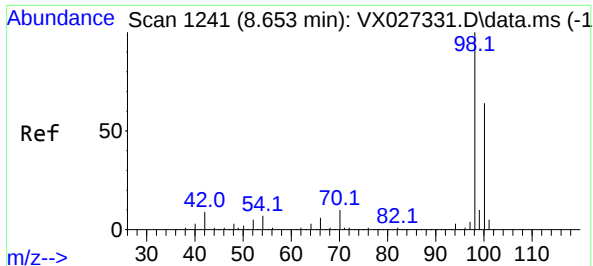

#50
Toluene-d8
Concen: 47.997 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX027359.D
Acq: 09 Mar 2022 19:01




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Tgt Ion: 98 Resp: 762504
Ion Ratio Lower Upper
98 100
100 65.4 52.6 78.8

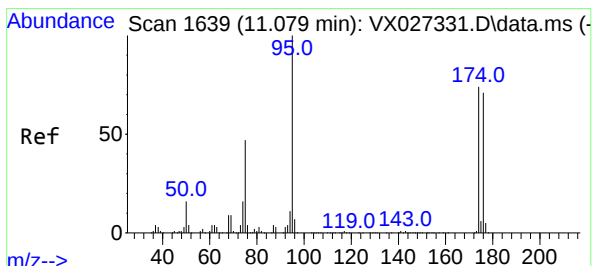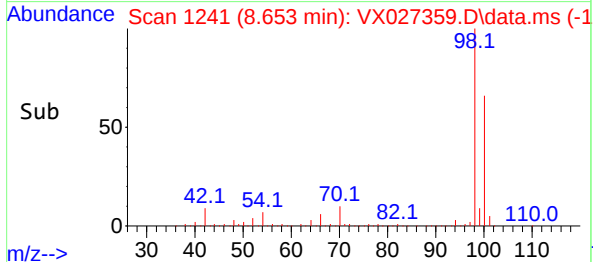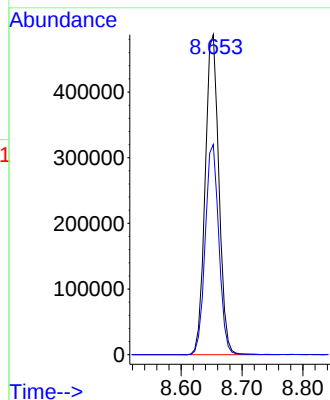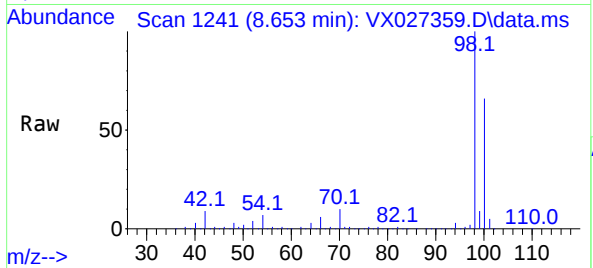

#62
4-Bromofluorobenzene
Concen: 45.518 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX027359.D
Acq: 09 Mar 2022 19:01

Tgt Ion: 95 Resp: 275605
Ion Ratio Lower Upper
95 100
174 83.9 0.0 163.0
176 81.8 0.0 155.0


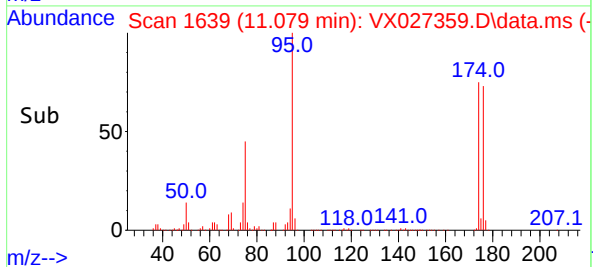
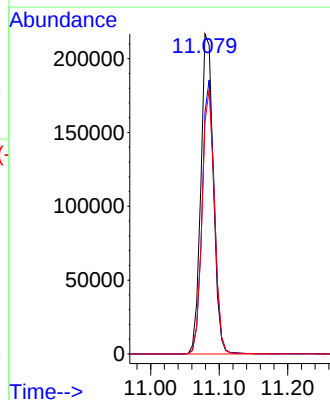
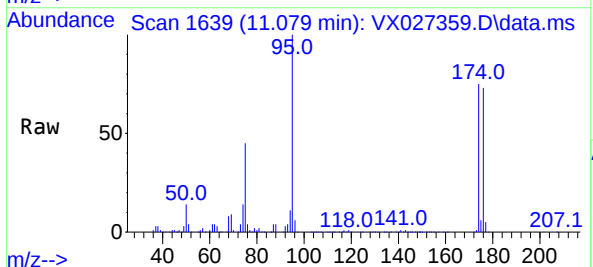




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX027359.D
Acq: 09 Mar 2022 19:01

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Tgt Ion:117 Resp: 598218
Ion Ratio Lower Upper
117 100
82 54.1 41.8 62.8
119 32.5 24.8 37.2

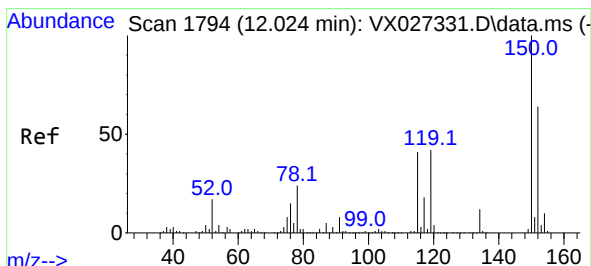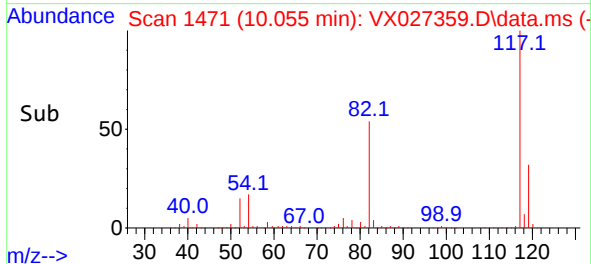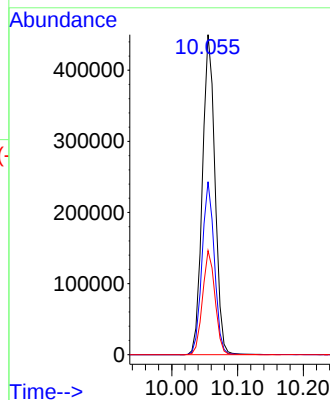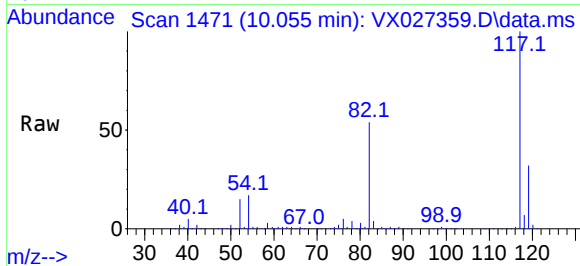

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX027359.D
Acq: 09 Mar 2022 19:01

Tgt Ion:152 Resp: 270386
Ion Ratio Lower Upper
152 100
115 58.8 37.5 112.7
150 156.4 0.0 338.2

