

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030922\
 Data File : VX027359.D
 Acq On : 09 Mar 2022 19:01
 Operator : JC/MD
 Sample : N1800-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANAG

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M

Title : SW846 8260

Signal : TIC: VX027359.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	22	27	33	rBV3	10001	24090	1.27%	0.238%
2	2.538	229	238	245	rBV	10214	20109	1.06%	0.199%
3	5.391	695	706	722	rBV	227133	655190	34.53%	6.469%
4	5.556	722	733	749	rVB	393698	1107385	58.35%	10.934%
5	5.958	788	799	814	rBV	217356	577064	30.41%	5.698%
6	6.763	921	931	948	rBV	589604	1397016	73.62%	13.793%
7	8.653	1233	1241	1258	rBV	1208236	1897724	100.00%	18.737%
8	10.055	1465	1471	1483	rBV	1250906	1651688	87.04%	16.308%
9	10.195	1490	1494	1499	rVB	19009	24423	1.29%	0.241%
10	11.085	1634	1640	1652	rBV	971977	1263015	66.55%	12.470%
11	12.024	1789	1794	1802	rBV	1239154	1510526	79.60%	14.914%




Sum of corrected areas: 10128230

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030922\
Data File : VX027359.D
Acq On : 09 Mar 2022 19:01
Operator : JC/MD
Sample : N1800-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

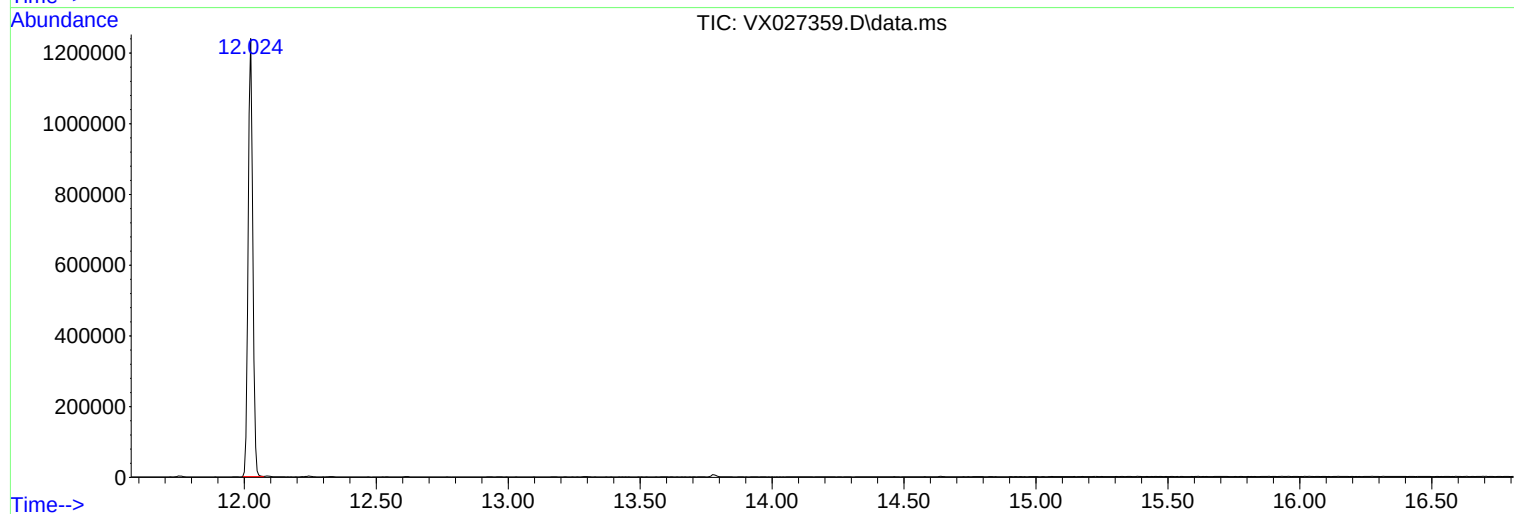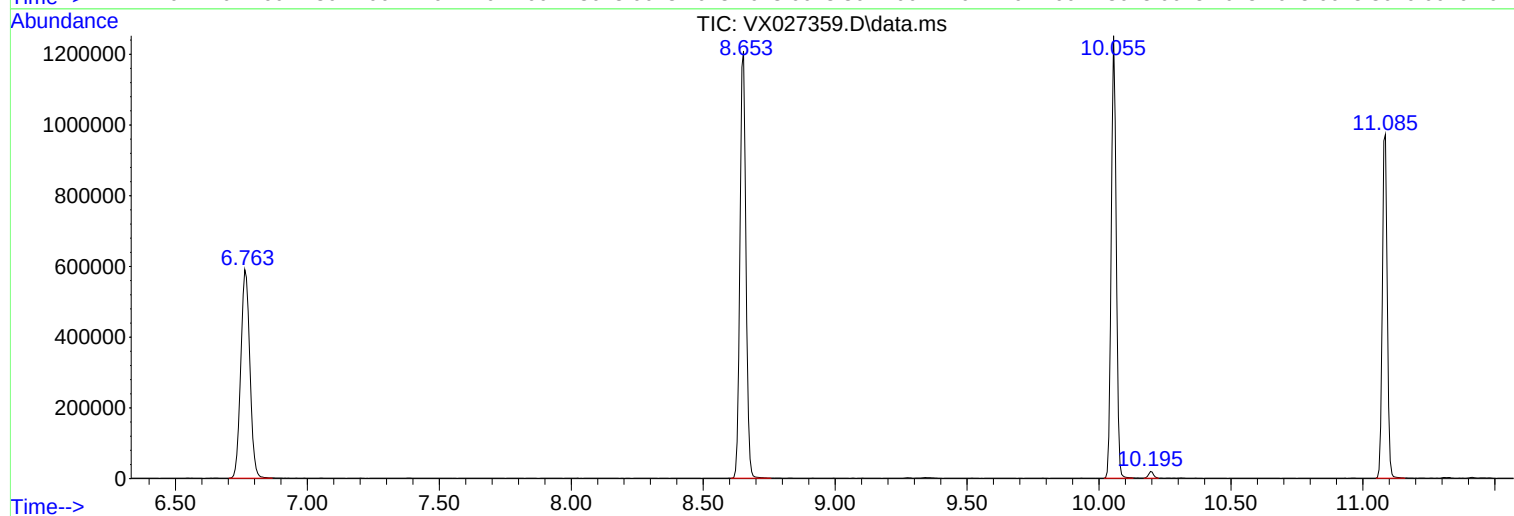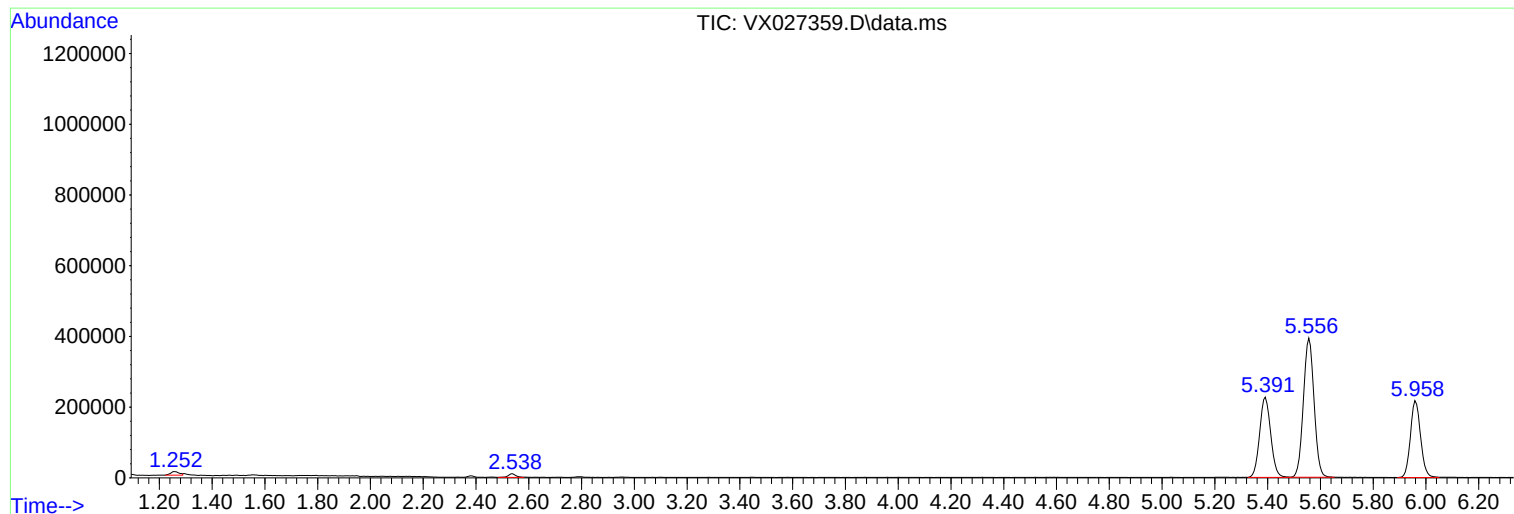

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030922\
Data File : VX027359.D
Acq On : 09 Mar 2022 19:01
Operator : JC/MD
Sample : N1800-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030922\
Data File : VX027359.D
Acq On : 09 Mar 2022 19:01
Operator : JC/MD
Sample : N1800-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc