

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030922\
 Data File : VX027361.D
 Acq On : 09 Mar 2022 19:47
 Operator : JC/MD
 Sample : N1814-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DTW-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
 Title : SW846 8260

Signal : TIC: VX027361.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	22	28	34	rBV	11055	25042	1.38%	0.252%
2	2.538	231	238	250	rVB	13377	26368	1.46%	0.266%
3	5.391	693	706	717	rBV	216721	629705	34.76%	6.348%
4	5.556	722	733	747	rVB	376058	1057045	58.35%	10.656%
5	5.958	788	799	815	rBV	211167	553214	30.54%	5.577%
6	6.763	920	931	945	rBV	563628	1337073	73.81%	13.479%
7	7.379	1023	1032	1042	rVB2	14341	36058	1.99%	0.364%
8	8.653	1234	1241	1255	rVB	1176856	1811447	100.00%	18.261%
9	9.458	1365	1373	1378	rBV	15798	25294	1.40%	0.255%
10	10.055	1465	1471	1480	rBV	1178251	1579483	87.19%	15.923%
11	10.299	1504	1511	1518	rVB4	10765	22362	1.23%	0.225%
12	10.872	1597	1605	1615	rBV2	11375	23126	1.28%	0.233%
13	11.085	1634	1640	1650	rBV	932905	1220678	67.39%	12.306%
14	11.171	1650	1654	1660	rVB	18068	24824	1.37%	0.250%
15	12.024	1789	1794	1800	rBV	1193618	1470668	81.19%	14.826%
16	13.347	2007	2011	2015	rBV	24561	31062	1.71%	0.313%
17	13.548	2040	2044	2047	rBV	22088	27580	1.52%	0.278%
18	13.658	2057	2062	2068	rVB6	8577	18573	1.03%	0.187%




Sum of corrected areas: 9919602

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030922\
Data File : VX027361.D
Acq On : 09 Mar 2022 19:47
Operator : JC/MD
Sample : N1814-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DTW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

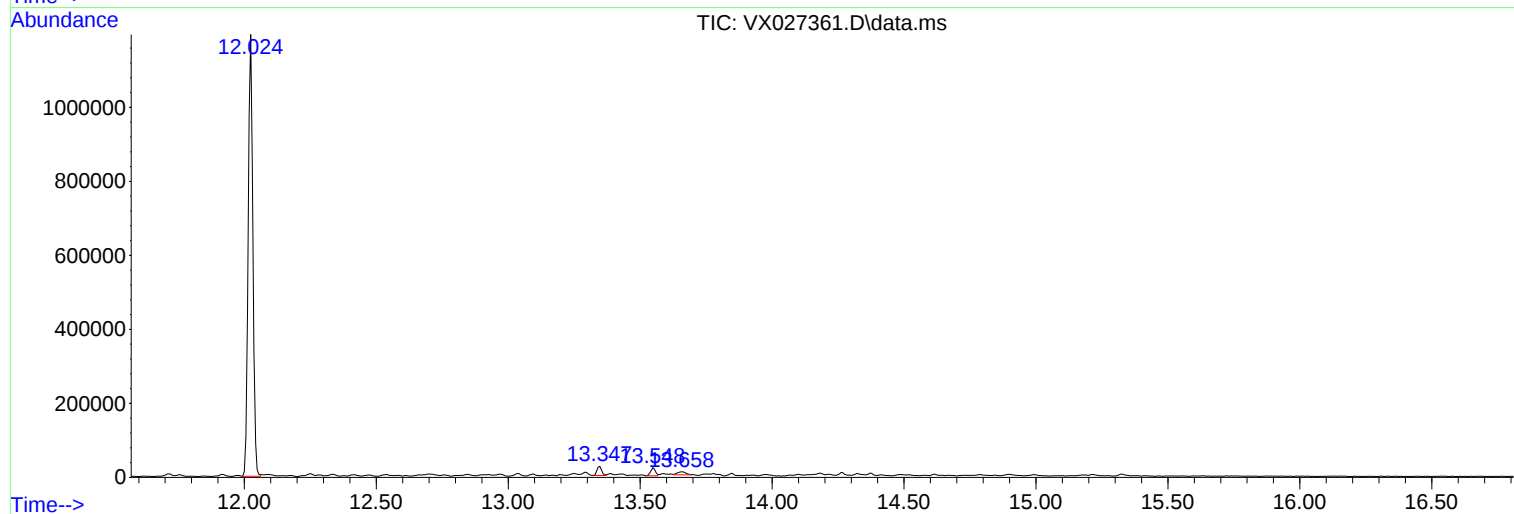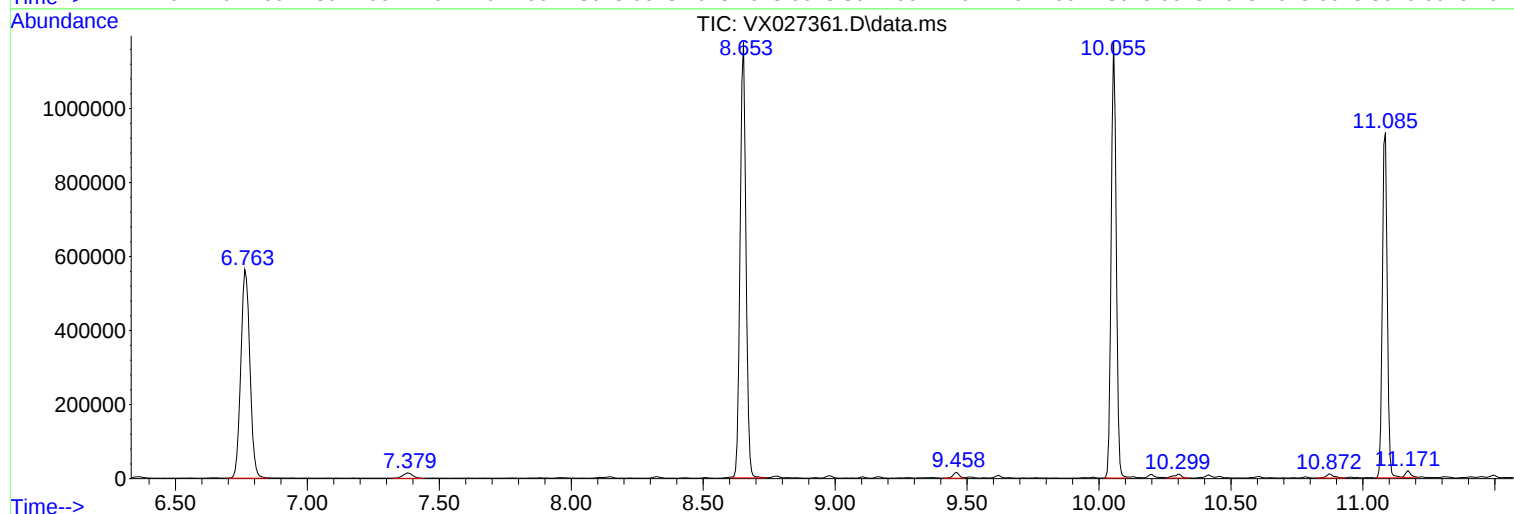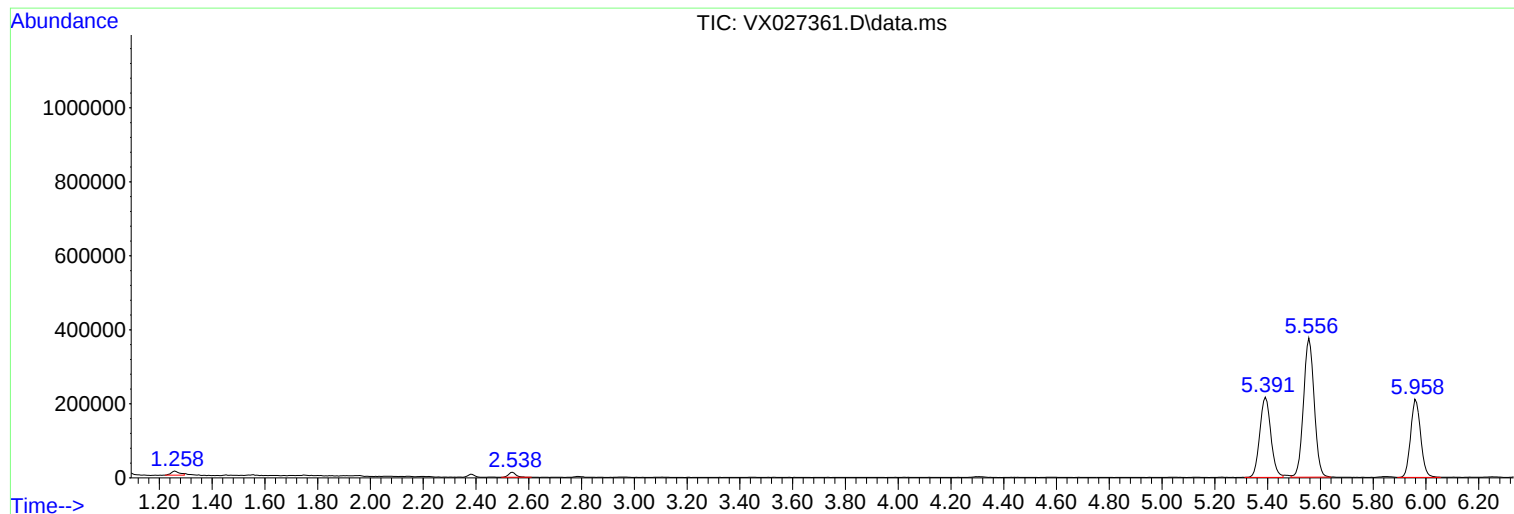

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030922\
Data File : VX027361.D
Acq On : 09 Mar 2022 19:47
Operator : JC/MD
Sample : N1814-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DTW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030922\
Data File : VX027361.D
Acq On : 09 Mar 2022 19:47
Operator : JC/MD
Sample : N1814-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DTW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------