

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX031020\
 Data File : VX015170.D
 Acq On : 10 Mar 2020 14:56
 Operator : JC/SP
 Sample : L1842-17DL 5X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE132D4-20200305DL


Quant Time: Mar 11 07:30:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X030420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 04 14:19:10 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	334673	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	549584	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	535440	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	273299	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.06	65	207480	52.26	ug/l	0.00
Spiked Amount						
			Recovery	=	104.52%	
35) Dibromofluoromethane	5.49	113	173167	49.94	ug/l	0.00
Spiked Amount						
			Recovery	=	99.88%	
50) Toluene-d8	8.71	98	674078	51.11	ug/l	0.00
Spiked Amount						
			Recovery	=	102.22%	
62) 4-Bromofluorobenzene	11.13	95	245121	52.11	ug/l	0.00
Spiked Amount						
			Recovery	=	104.22%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) 1,1,2-Trichlorotrifluoroet	2.38	101	5258	1.669	ug/l	97
11) Tert butyl alcohol	3.01	59	1760	2.555	ug/l #	86
12) 1,1-Dichloroethene	2.37	96	1274	0.392	ug/l #	66
13) Acrolein	2.28	56	139	0.215	ug/l #	1
15) Acrylonitrile	3.11	53	493	0.287	ug/l #	35
16) Acetone	2.45	43	1222	0.760	ug/l #	50
25) 2-Butanone	4.67	43	616	0.262	ug/l #	49
27) cis-1,2-Dichloroethene	4.59	96	2460	0.631	ug/l	83
29) Tetrahydrofuran	5.12	42	459	0.302	ug/l #	10
36) 1,1-Dichloropropene	5.65	75	23827	4.690	ug/l #	52
38) Carbon Tetrachloride	5.65	117	30577	6.376	ug/l #	16
44) Trichloroethene	7.21	130	195229	46.506	ug/l	100
49) 1,4-Dioxane	7.64	88	258	2.828	ug/l	96
58) 2-Chloroethyl Vinyl ether	8.12	63	644	0.218	ug/l	98
64) Tetrachloroethene	9.33	164	4603	1.040	ug/l	87
76) 1,2,3-Trichloropropane	11.13	75	120672	22.136	ug/l #	33
81) trans-1,4-Dichloro-2-buten	11.13	75	120672	62.821	ug/l #	11
95) Naphthalene	13.82	128	554	1.450	ug/l #	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 782

Delta R.T. -0.00 min

Lab File: VX015170.D

Acq: 10 Mar 2020 14:56

Instrument :

MSVOA_X

ClientSampleId :


RE132D4-20200305DL

Tot Ion:168 Resp: 334673

Ion Ratio Lower Upper

168 100

99 51.5 39.4 59.2



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0



5.65

100000

50000

0

Time--> 5.50 5.60 5.70 5.80

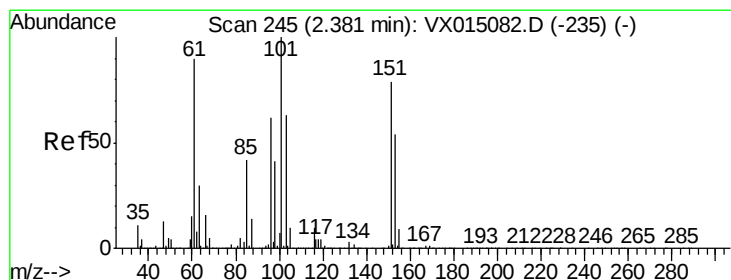

#9

1,1,2-Trichlorotrifluoroethane

Concen: 1.669 ug/l

RT: 2.38 min Scan# 245

Delta R.T. -0.00 min

Lab File: VX015170.D

Acq: 10 Mar 2020 14:56


Tgt Ion:101 Resp: 5258

Ion Ratio Lower Upper

101 100

85 38.0 33.7 50.5

151 81.6 64.0 96.0



Abundance Ion 100.90 (100.60 to 101.60): V

Ion 84.90 (84.60 to 85.60): VX0

Ion 150.80 (150.50 to 151.50): V

2.38


3000


2000

1000

0

Time--> 2.30 2.35 2.40 2.45







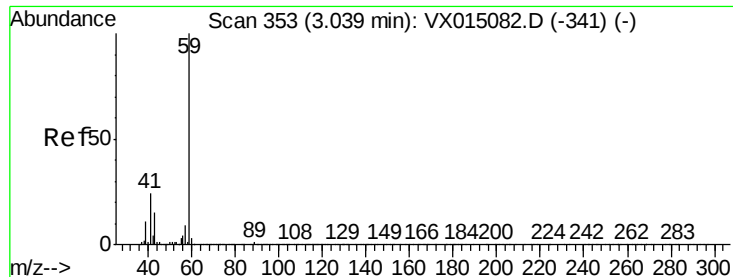

#11
Tert butyl alcohol
Concen: 2.555 ug/l
RT: 3.01 min Scan# 349
Delta R.T. -0.02 min
Lab File: VX015170.D
Acq: 10 Mar 2020 14:56




Instrument :
MSVOA_X
ClientSampleId :
RE132D4-20200305DL


Tot Ion: 59 Resp: 1760
Ion Ratio Lower Upper
59 100
57 5.1 8.2 12.4#

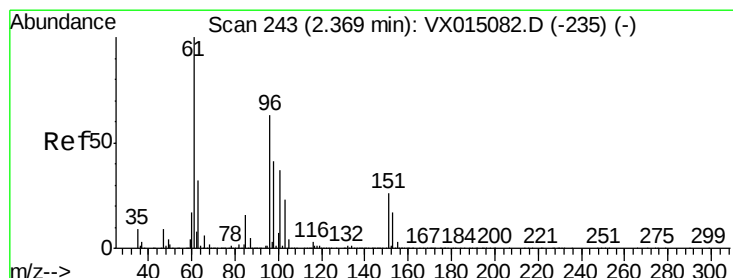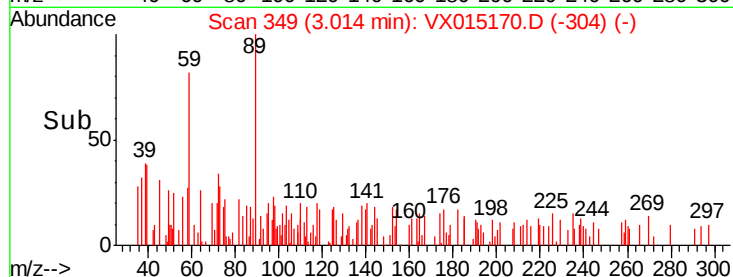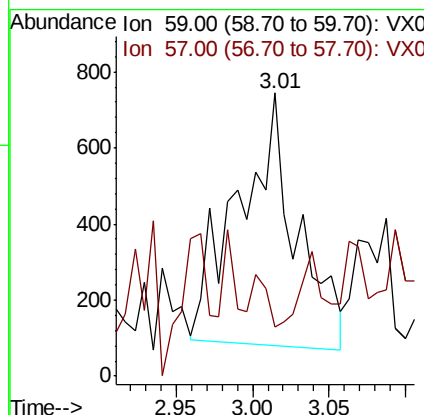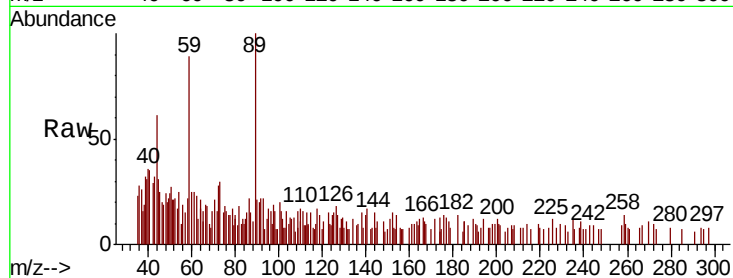

#12
1,1-Dichloroethene
Concen: 0.392 ug/l
RT: 2.37 min Scan# 243
Delta R.T. -0.00 min
Lab File: VX015170.D
Acq: 10 Mar 2020 14:56

Tgt Ion: 96 Resp: 1274
Ion Ratio Lower Upper
96 100
61 110.4 126.2 189.4#
98 41.8 51.4 77.0#


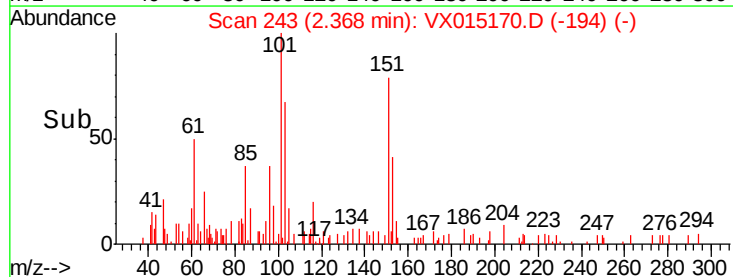
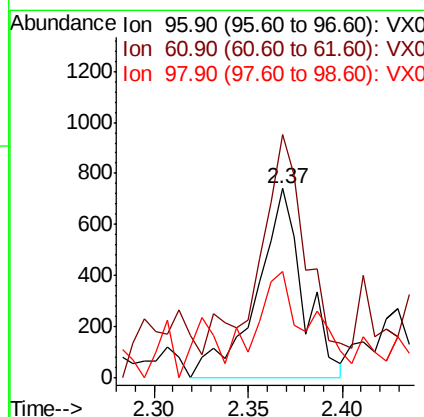
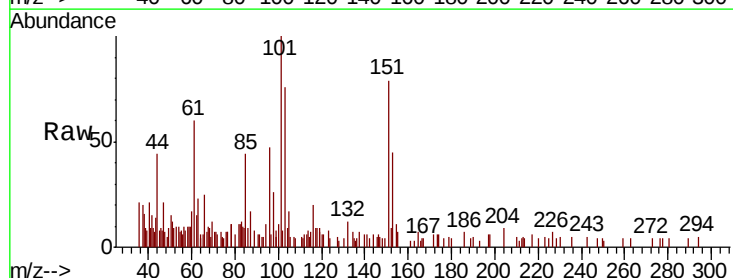


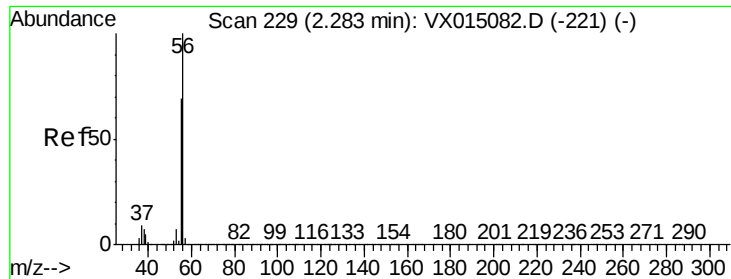

#13
Acrolein
Concen: 0.215 ug/l
RT: 2.28 min Scan# 228
Delta R.T. -0.01 min
Lab File: VX015170.D
Acq: 10 Mar 2020 14:56




Instrument :
MSVOA_X
ClientSampleId :
RE132D4-20200305DL


Tot Ion: 56 Resp: 139
Ion Ratio Lower Upper
56 100
55 163.3 55.4 83.0#

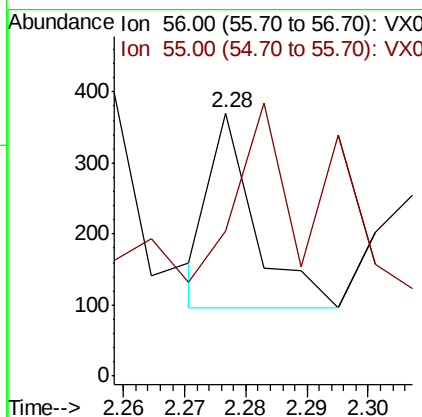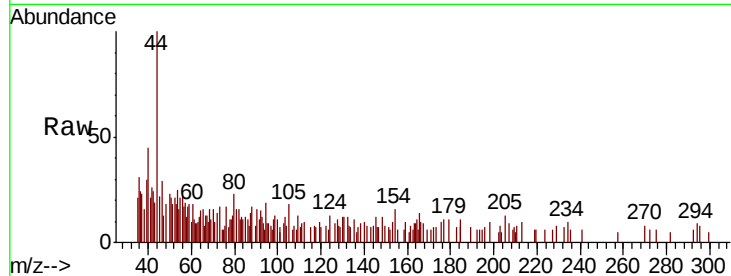

#15
Acrylonitrile
Concen: 0.287 ug/l
RT: 3.11 min Scan# 364
Delta R.T. -0.02 min
Lab File: VX015170.D
Acq: 10 Mar 2020 14:56

Tgt Ion: 53 Resp: 493
Ion Ratio Lower Upper
53 100
52 0.0 66.6 100.0#
51 38.1 29.0 43.6



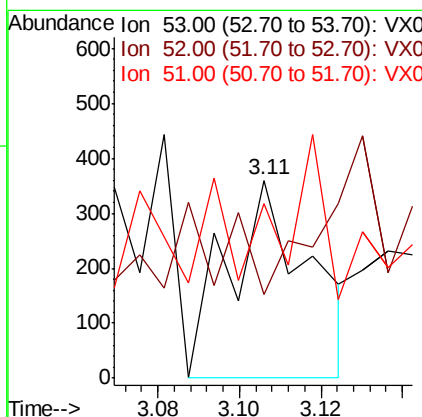





#16
Acetone
Concen: 0.760 ug/l
RT: 2.45 min Scan# 256
Delta R.T. 0.01 min
Lab File: VX015170.D
Acq: 10 Mar 2020 14:56




Instrument :
MSVOA_X
ClientSampleId :
RE132D4-20200305DL


Tot Ion: 43 Resp: 1222
Ion Ratio Lower Upper
43 100
58 3.6 24.8 37.2#

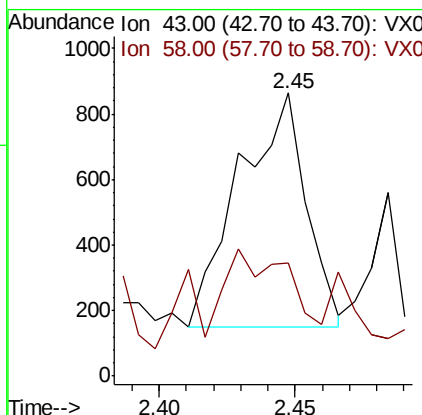

#25
2-Butanone
Concen: 0.262 ug/l
RT: 4.67 min Scan# 621
Delta R.T. 0.01 min
Lab File: VX015170.D
Acq: 10 Mar 2020 14:56

Tgt Ion: 43 Resp: 616
Ion Ratio Lower Upper
43 100
72 0.0 20.6 30.8#

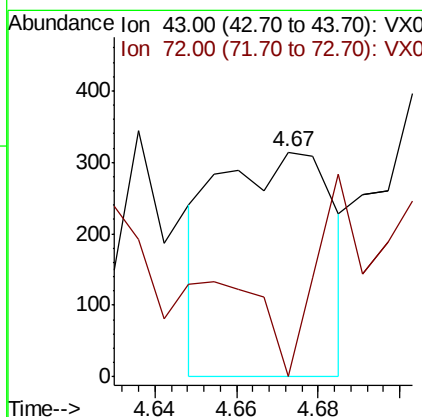

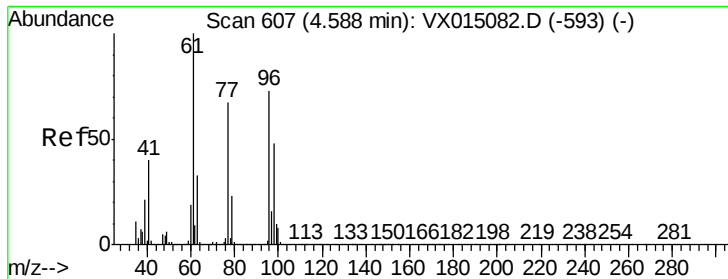


#27




cis-1,2-Dichloroethene
 Concen: 0.631 ug/l
 RT: 4.59 min Scan# 607
 Delta R.T. -0.00 min
 Lab File: VX015170.D
 Acq: 10 Mar 2020 14:56

Instrument :
 MSVOA_X
 ClientSampleId :
 RE132D4-20200305DL

Tot Ion	Ratio	Lower	Upper
96	100		
61	116.2	0.0	286.8
98	60.4	0.0	128.4

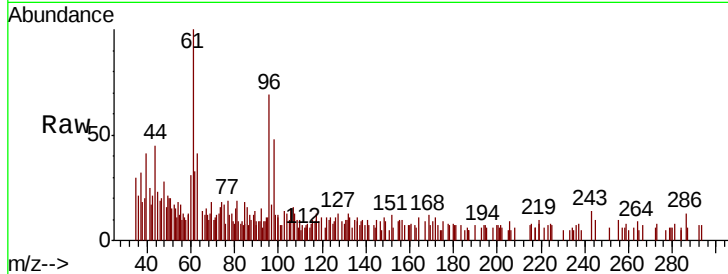


Abundance Ion 95.90 (95.60 to 96.60): VX0
 Ion 60.90 (60.60 to 61.60): VX0
 Ion 97.90 (97.60 to 98.60): VX0

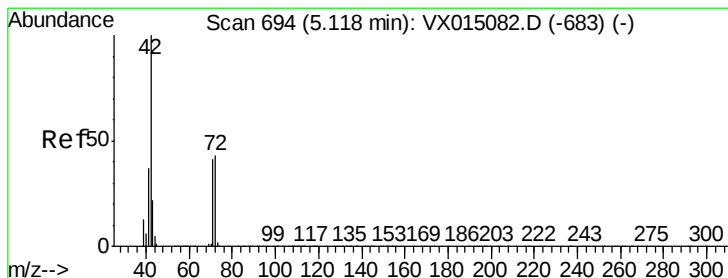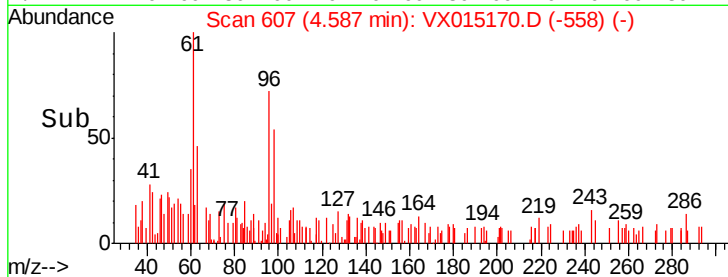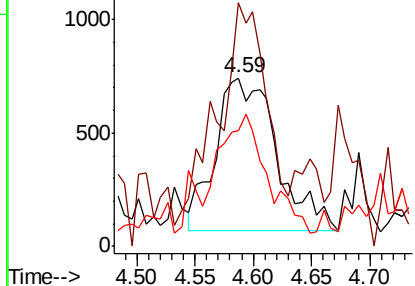



#29


Tetrahydrofuran
 Concen: 0.302 ug/l
 RT: 5.12 min Scan# 694
 Delta R.T. -0.00 min
 Lab File: VX015170.D
 Acq: 10 Mar 2020 14:56

Tgt Ion	Ratio	Lower	Upper
42	100		
72	0.0	36.4	54.6#
71	113.1	33.3	49.9#

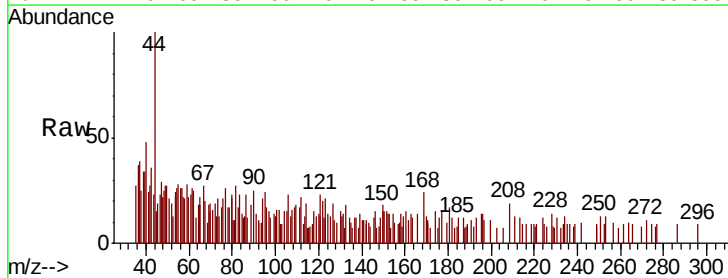

Abundance Ion 42.00 (41.70 to 42.70): VX0
 Ion 72.00 (71.70 to 72.70): VX0
 Ion 71.00 (70.70 to 71.70): VX0

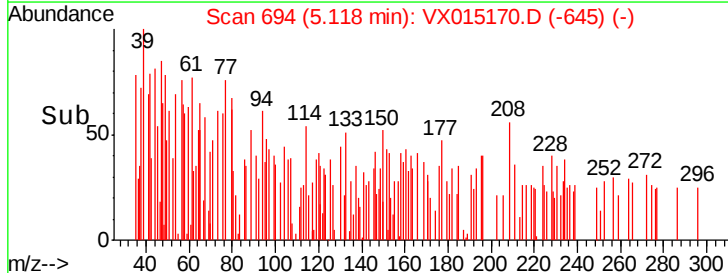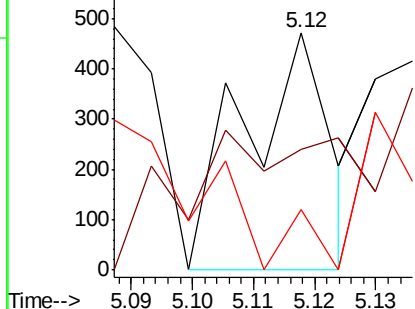

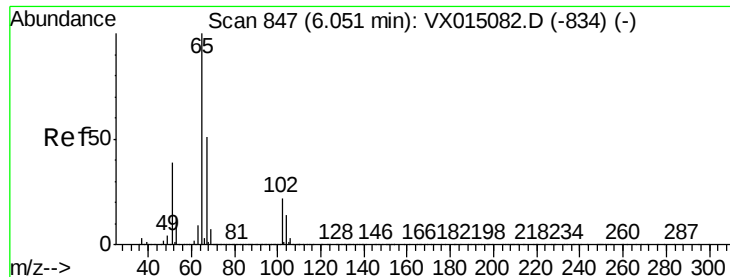

#33

1,2-Dichloroethane-d4

Concen: 52.256 ug/l

RT: 6.06 min Scan# 848

Delta R.T. 0.01 min

Lab File: VX015170.D

Acq: 10 Mar 2020 14:56

Instrument :

MSVOA_X

ClientSampleId :


RE132D4-20200305DL

Tot Ion: 65 Resp: 207480

Ion Ratio Lower Upper




65 100

67 52.9 0.0 105.6

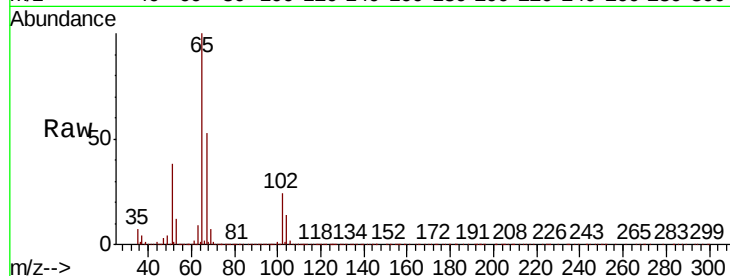

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

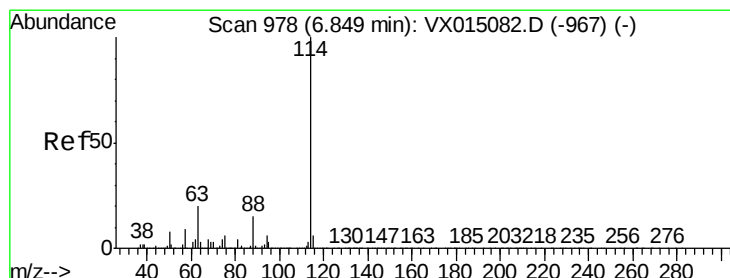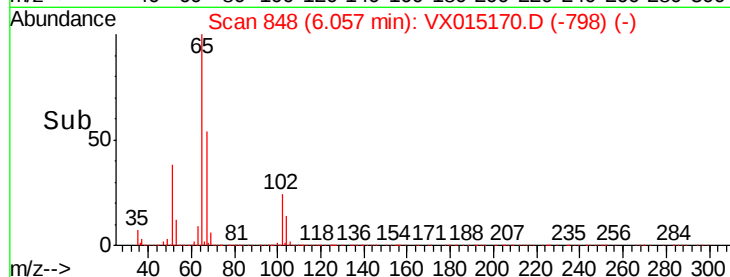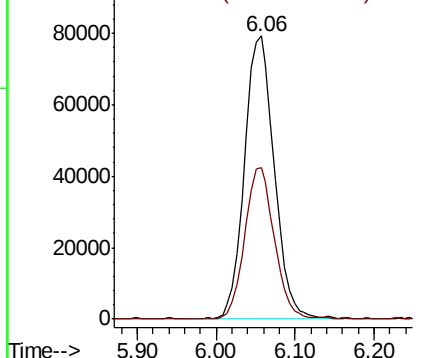

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 979

Delta R.T. 0.01 min

Lab File: VX015170.D

Acq: 10 Mar 2020 14:56


Tgt Ion: 114 Resp: 549584

Ion Ratio Lower Upper

114 100

63 20.1 0.0 40.0



88 15.1 0.0 30.6

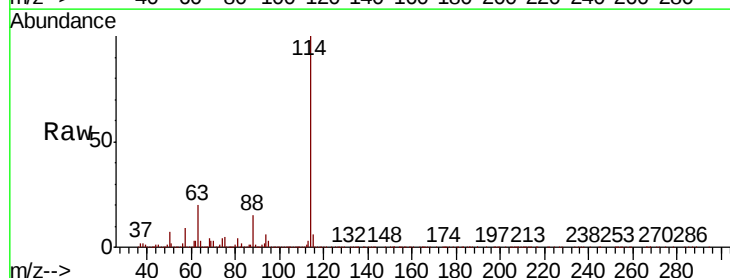


Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0



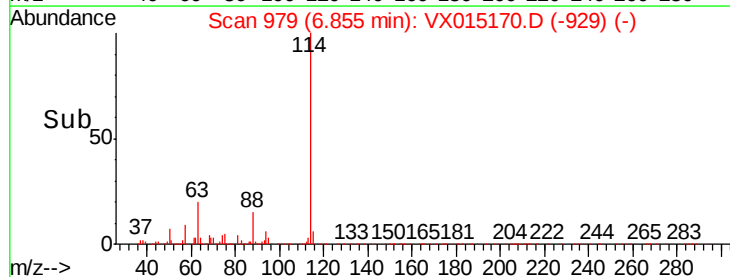
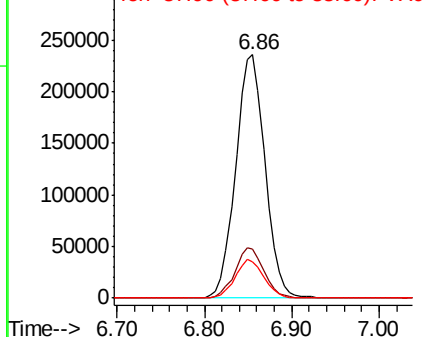




#35
 Dibromofluoromethane
 Concen: 49.945 ug/l
 RT: 5.49 min Scan# 755
 Delta R.T. -0.00 min
 Lab File: VX015170.D
 Acq: 10 Mar 2020 14:56




Instrument :
 MSVOA_X
 ClientSampleId :
 RE132D4-20200305DL


Tot Ion	Ratio	Lower	Upper
113	100		
111	103.2	82.6	123.8
192	23.4	18.6	28.0

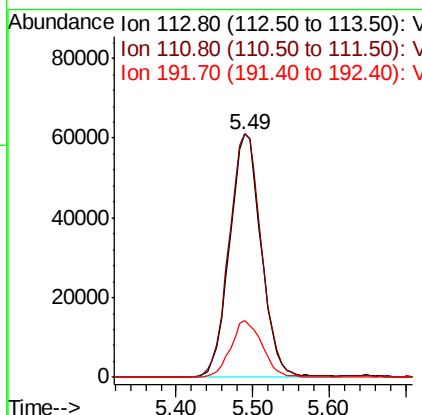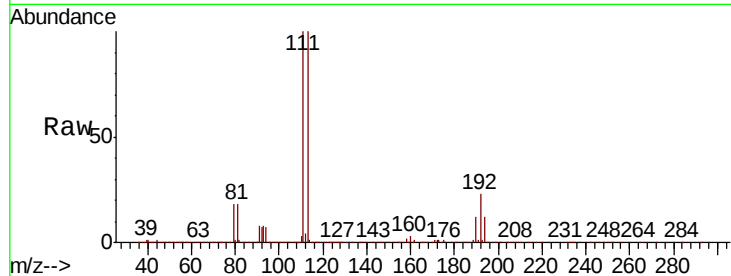

#36
 1,1-Dichloropropene
 Concen: 4.690 ug/l
 RT: 5.65 min Scan# 781
 Delta R.T. -0.15 min
 Lab File: VX015170.D
 Acq: 10 Mar 2020 14:56

Tgt Ion	Ratio	Lower	Upper
75	100		
110	11.0	17.9	53.8#
77	0.7	24.8	37.2#


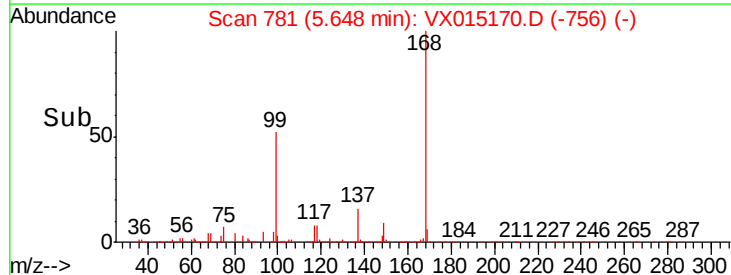
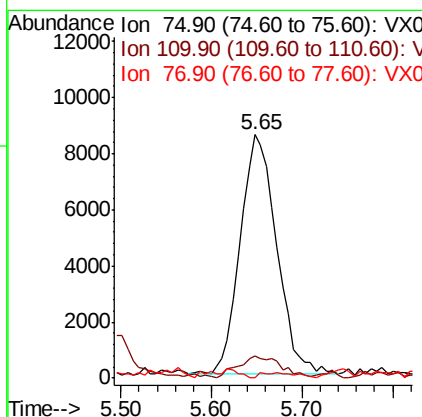



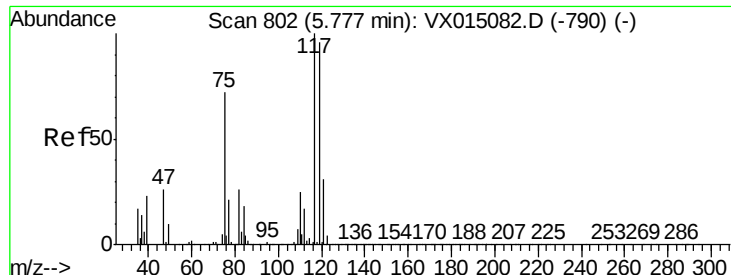

#38
Carbon Tetrachloride
Concen: 6.376 ug/l
RT: 5.65 min Scan# 782
Delta R.T. -0.12 min
Lab File: VX015170.D
Acq: 10 Mar 2020 14:56




Instrument :
MSVOA_X
ClientSampleId :
RE132D4-20200305DL


Tot Ion:117 Resp: 30577
Ion Ratio Lower Upper
117 100
119 4.8 76.9 115.3#
121 0.9 24.6 37.0#

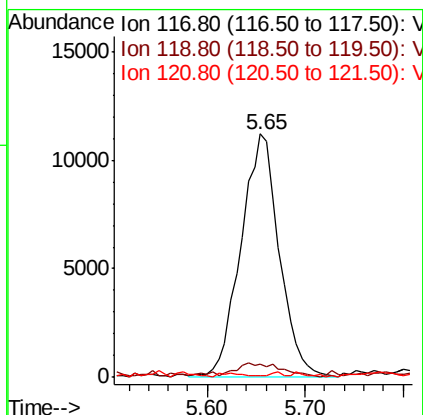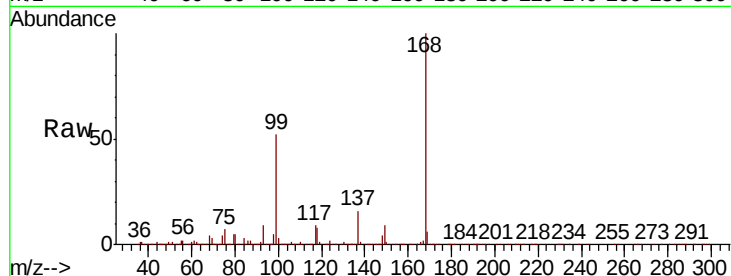

#44
Trichloroethene
Concen: 46.506 ug/l
RT: 7.21 min Scan# 1037
Delta R.T. -0.00 min
Lab File: VX015170.D
Acq: 10 Mar 2020 14:56

Tgt Ion:130 Resp: 195229
Ion Ratio Lower Upper
130 100
95 90.7 0.0 181.2


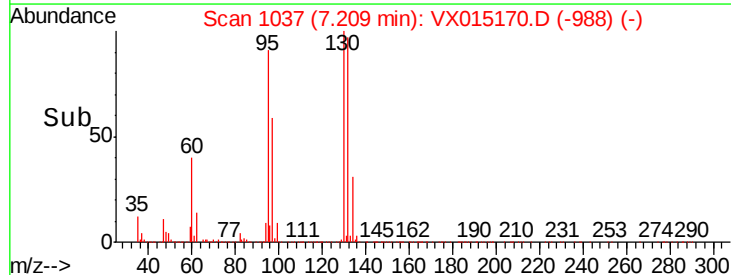
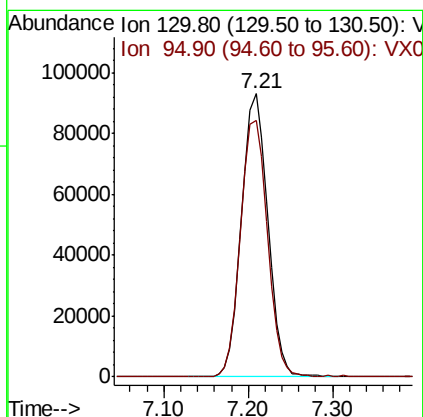



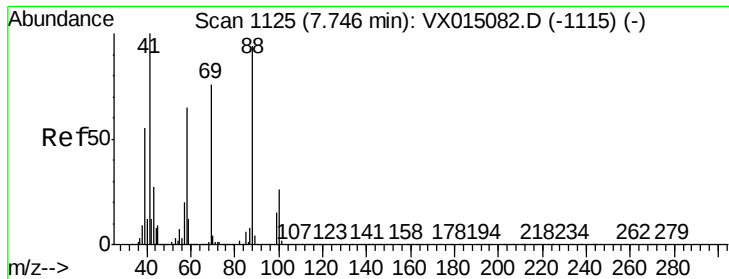

#49
1,4-Dioxane
Concen: 2.828 ug/l
RT: 7.64 min Scan# 1107
Delta R.T. -0.11 min
Lab File: VX015170.D
Acq: 10 Mar 2020 14:56




Instrument :
MSVOA_X
ClientSampleId :
RE132D4-20200305DL


Tot Ion: 88 Resp: 258
Ion Ratio Lower Upper
88 100
43 39.9 27.0 40.4
58 68.6 55.6 83.4

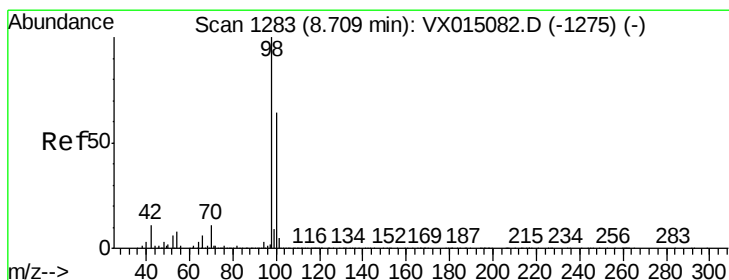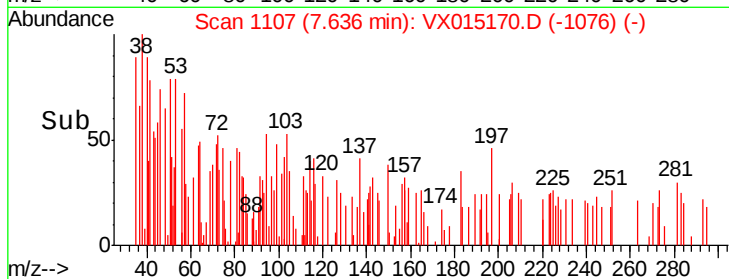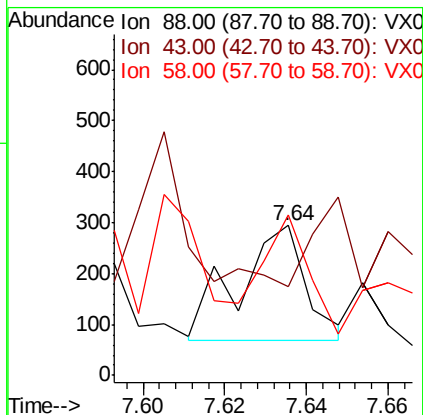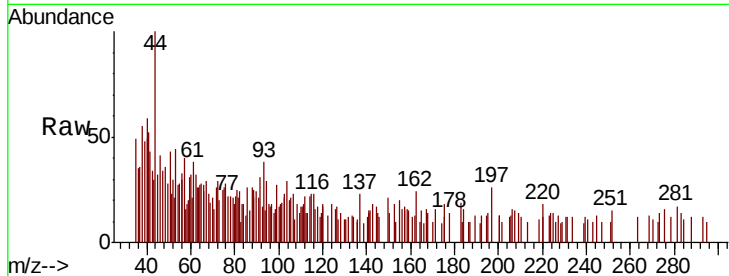

#50
Toluene-d8
Concen: 51.111 ug/l
RT: 8.71 min Scan# 1283
Delta R.T. -0.00 min
Lab File: VX015170.D
Acq: 10 Mar 2020 14:56

Tgt Ion: 98 Resp: 674078
Ion Ratio Lower Upper
98 100
100 65.0 52.4 78.6


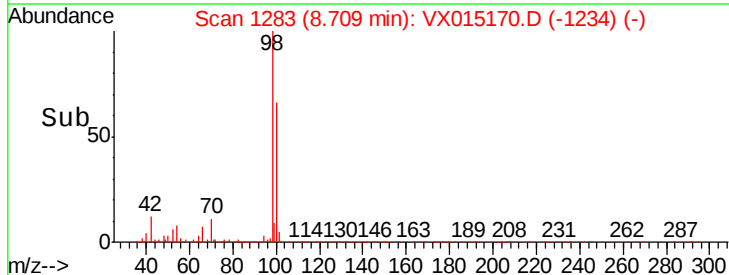
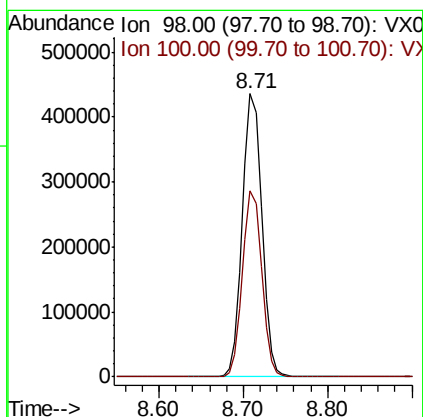
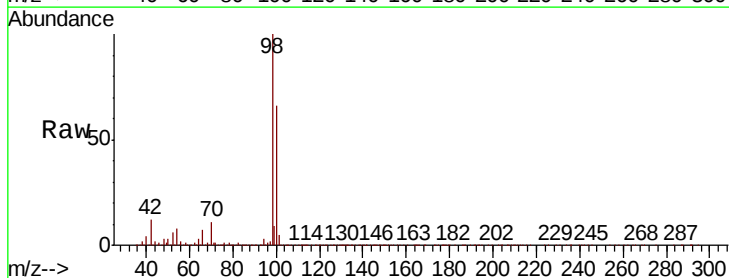




#58
2-Chloroethyl Vinyl ether
Concen: 0.218 ug/l
RT: 8.12 min Scan# 1186
Delta R.T. -0.19 min
Lab File: VX015170.D
Acq: 10 Mar 2020 14:56




Instrument :
MSVOA_X
ClientSampleId :
RE132D4-20200305DL


Tot Ion: 63 Resp: 644
Ion Ratio Lower Upper
63 100
106 29.8 22.8 34.2

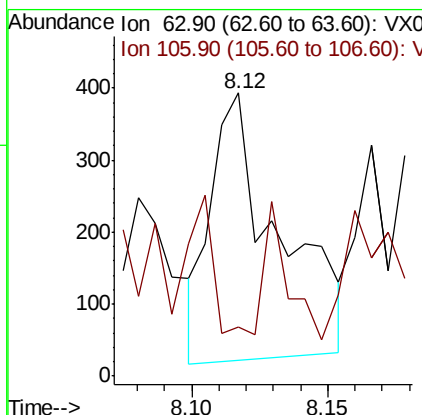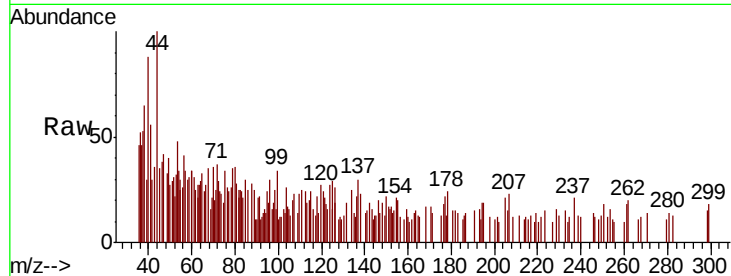

#62
4-Bromofluorobenzene
Concen: 52.107 ug/l
RT: 11.13 min Scan# 1681
Delta R.T. 0.01 min
Lab File: VX015170.D
Acq: 10 Mar 2020 14:56

Tgt Ion: 95 Resp: 245121
Ion Ratio Lower Upper
95 100
174 90.0 0.0 177.6
176 85.4 0.0 170.2



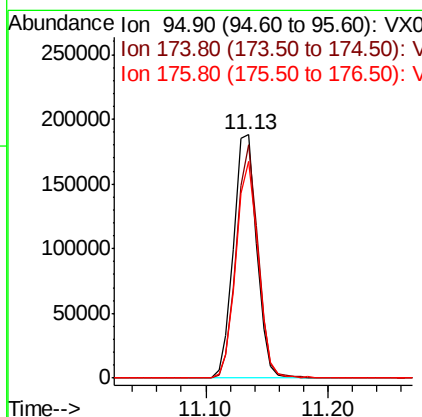
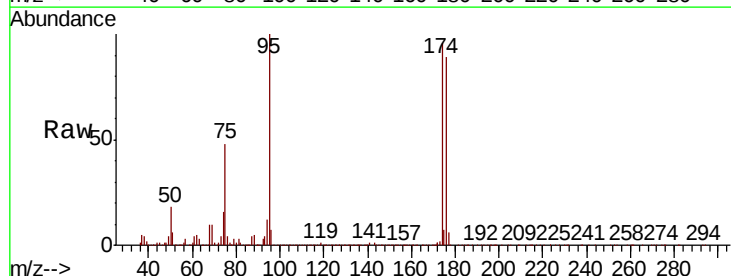




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1513
Delta R.T. -0.00 min
Lab File: VX015170.D
Acq: 10 Mar 2020 14:56




Instrument :
MSVOA_X
ClientSampleId :
RE132D4-20200305DL


Tot Ion	Ratio	Lower	Upper
117	100		
82	52.6	43.3	64.9
119	33.1	25.8	38.8

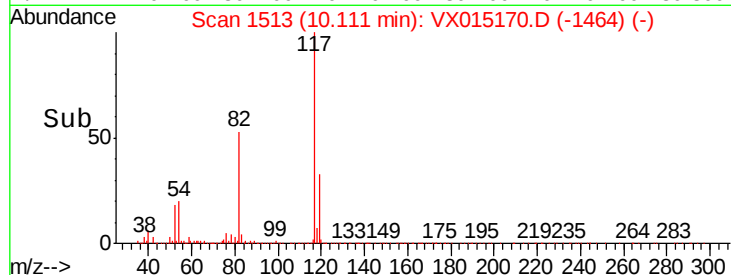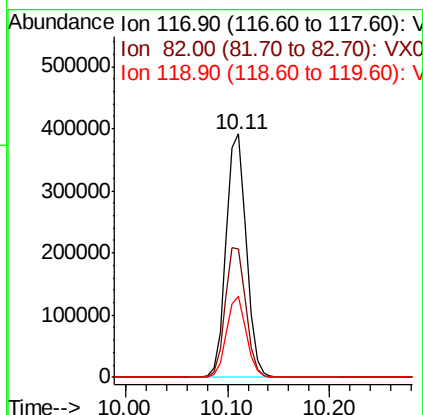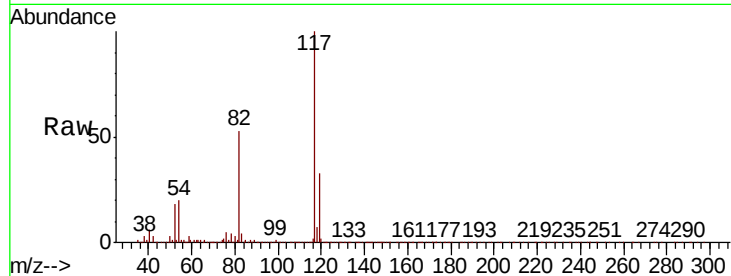

#64
Tetrachloroethene
Concen: 1.040 ug/l
RT: 9.33 min Scan# 1385
Delta R.T. -0.00 min
Lab File: VX015170.D
Acq: 10 Mar 2020 14:56

Tgt Ion	Ratio	Lower	Upper
164	100		
166	112.1	101.1	151.7
129	79.4	69.4	104.0
131	71.2	69.8	104.8

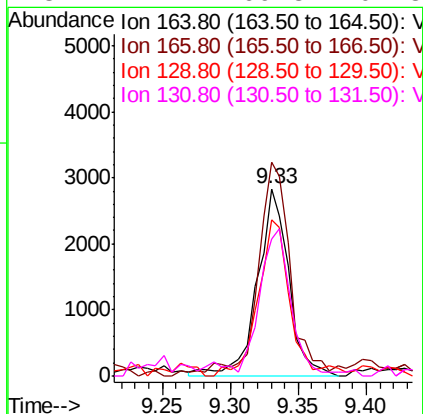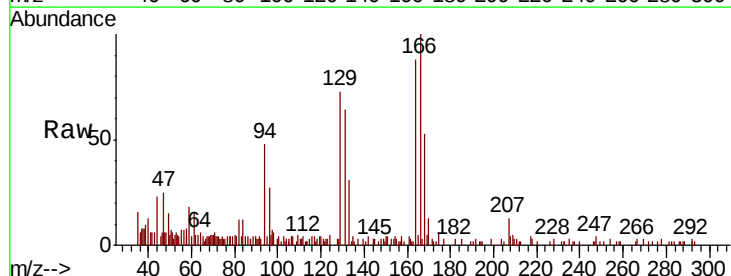



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.07 min Scan# 1835

Delta R.T. -0.00 min

Lab File: VX015170.D

Acq: 10 Mar 2020 14:56

Instrument :

MSVOA_X

ClientSampleId :

RE132D4-20200305DL


Tot Ion:152 Resp: 273299

Ion Ratio Lower Upper

152 100

115 54.7 38.2 114.6




150 155.3 0.0 343.8

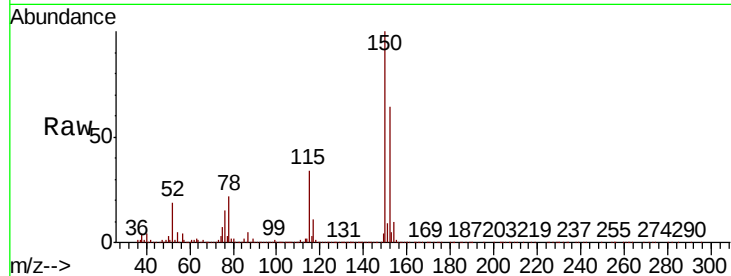

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

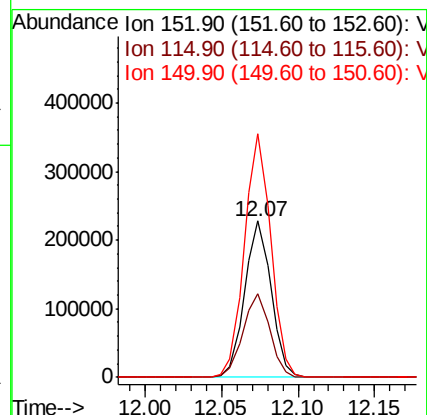

#76

1,2,3-Trichloropropane

Concen: 22.136 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.16 min

Lab File: VX015170.D


Acq: 10 Mar 2020 14:56

Tgt Ion: 75 Resp: 120672

Ion Ratio Lower Upper



75 100


77 1.3 22.6 67.8#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

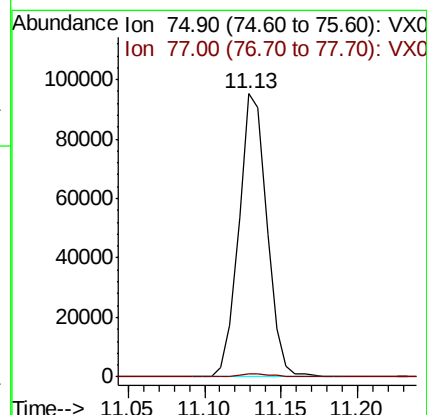

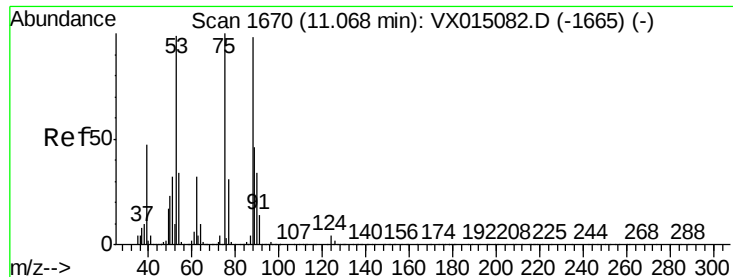

#81

trans-1,4-Dichloro-2-butene

Concen: 62.821 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. 0.06 min

Lab File: VX015170.D

Acq: 10 Mar 2020 14:56

Instrument :

MSVOA_X

ClientSampleId :

RE132D4-20200305DL


Tot Ion: 75 Resp: 120672

Ion Ratio Lower Upper

75 100

53 0.5 77.9 116.9#




89 0.2 36.2 54.2#

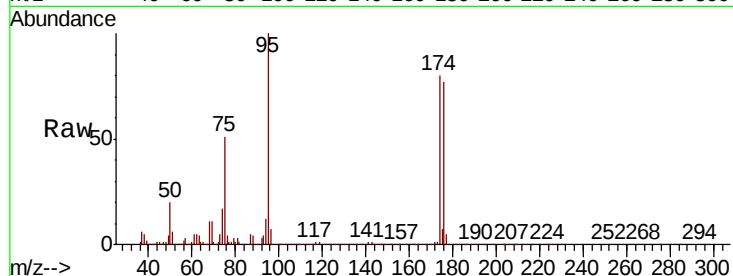

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

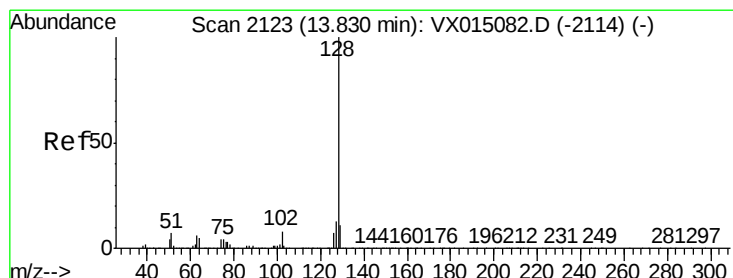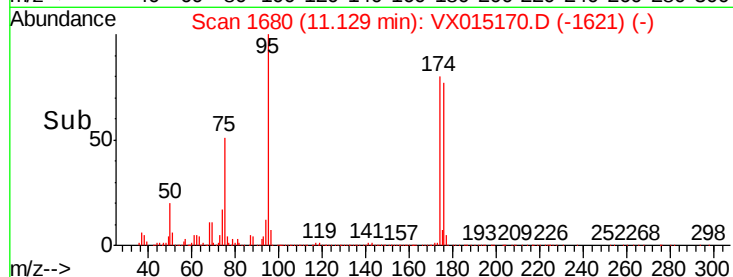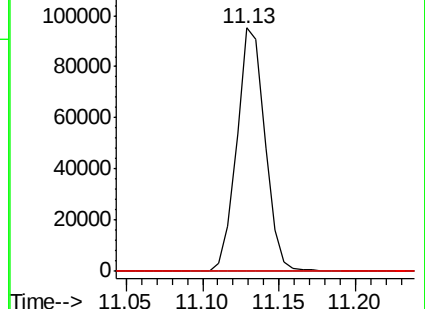

#95

Naphthalene

Concen: 1.450 ug/l

RT: 13.82 min Scan# 2122

Delta R.T. -0.01 min

Lab File: VX015170.D

Acq: 10 Mar 2020 14:56


Tgt Ion: 128 Resp: 554

Ion Ratio Lower Upper

128 100

127 0.0 10.3 15.5#

129 0.0 8.6 13.0#

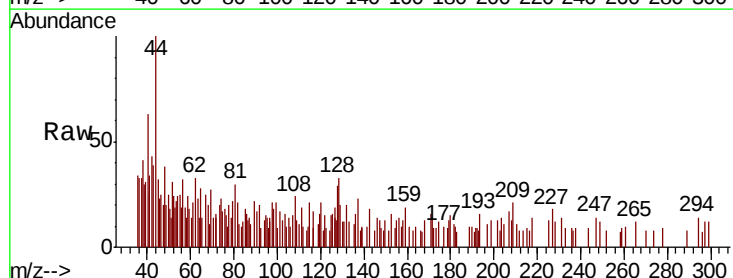

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

