

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031021\  
Data File : VX021132.D  
Acq On : 10 Mar 2021 13:31  
Operator : JC/MD  
Sample : M1596-23  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FB01-20210305

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X022421W.M

Title : SW846 8260

Signal : TIC: VX021132.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.470       | 731           | 745         | 760          | rBV      | 132664         | 376623        | 31.09%          | 6.045%        |
| 2         | 5.629       | 761           | 772         | 790          | rVV      | 208673         | 580658        | 47.94%          | 9.320%        |
| 3         | 6.035       | 830           | 841         | 858          | rBV      | 144275         | 375401        | 30.99%          | 6.025%        |
| 4         | 6.835       | 964           | 977         | 1000         | rBV      | 349148         | 842615        | 69.57%          | 13.524%       |
| 5         | 8.694       | 1286          | 1293        | 1317         | rBV      | 758921         | 1211253       | 100.00%         | 19.441%       |
| 6         | 10.094      | 1525          | 1531        | 1551         | rVB      | 818282         | 1082826       | 89.40%          | 17.380%       |
| 7         | 11.118      | 1699          | 1705        | 1717         | rBV      | 638761         | 811461        | 66.99%          | 13.024%       |
| 8         | 12.059      | 1860          | 1865        | 1874         | rBV      | 757340         | 949468        | 78.39%          | 15.240%       |




Sum of corrected areas: 6230305

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031021\  
Data File : VX021132.D  
Acq On : 10 Mar 2021 13:31  
Operator : JC/MD  
Sample : M1596-23  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FB01-20210305

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X022421W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

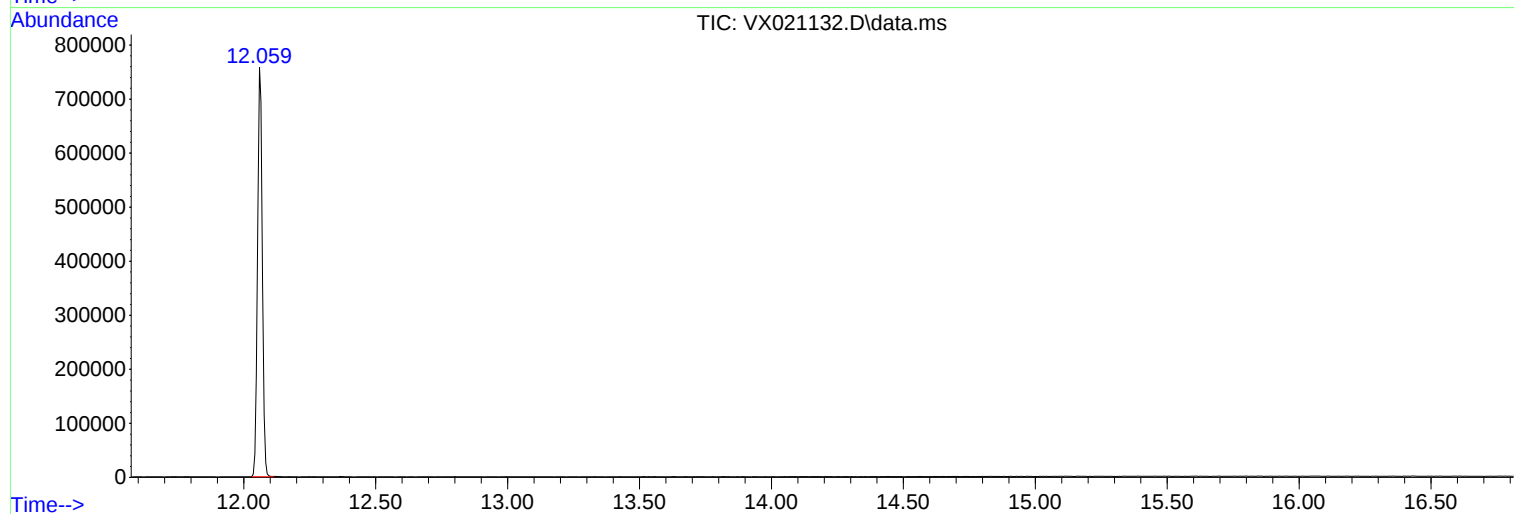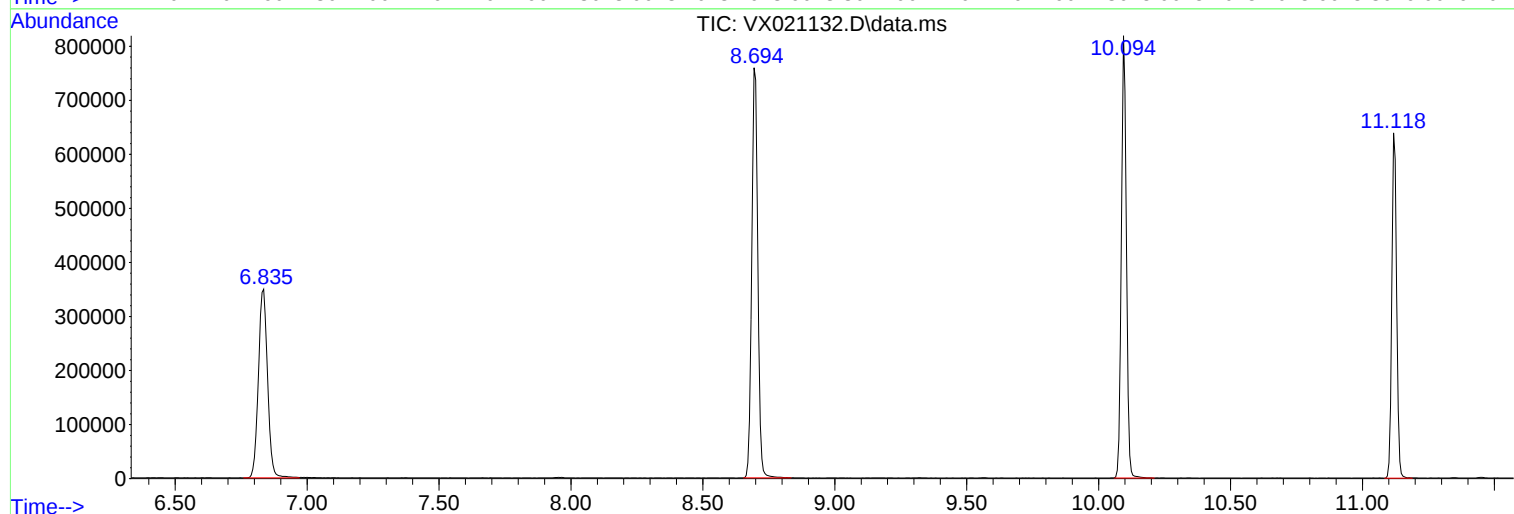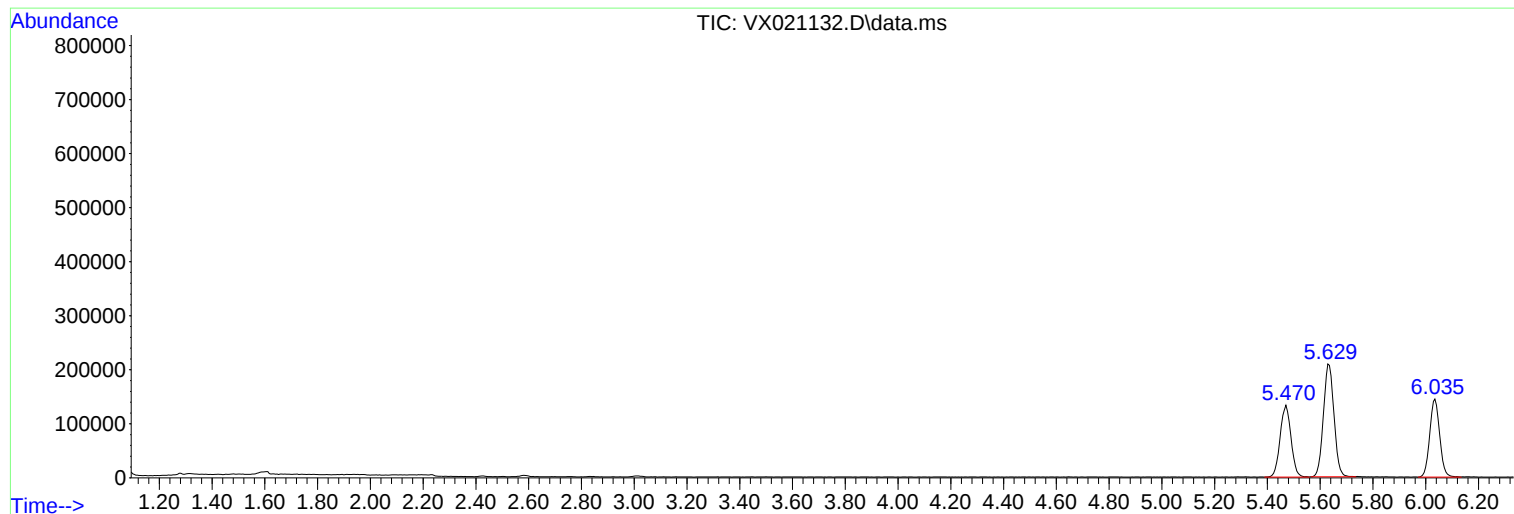

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031021\  
Data File : VX021132.D  
Acq On : 10 Mar 2021 13:31  
Operator : JC/MD  
Sample : M1596-23  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FB01-20210305

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X022421W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031021\  
Data File : VX021132.D  
Acq On : 10 Mar 2021 13:31  
Operator : JC/MD  
Sample : M1596-23  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FB01-20210305

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X022421W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|