


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031021\
Data File : VX021124.D
Acq On : 10 Mar 2021 09:18
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Title : SW846 8260
Last Update : Wed Feb 24 13:50:55 2021

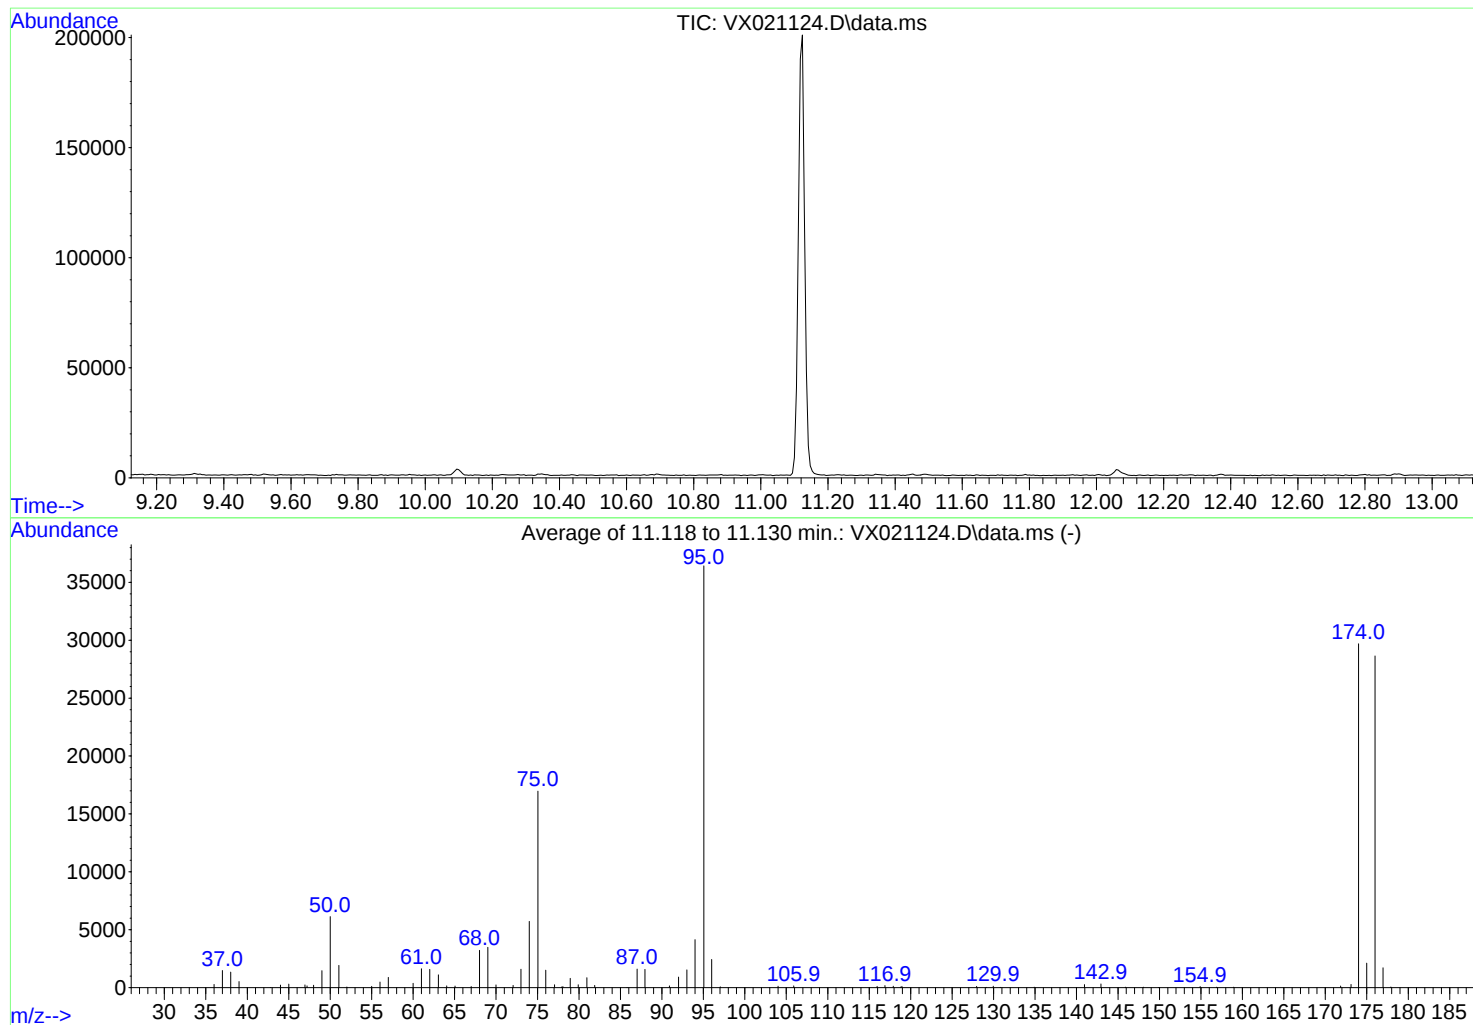

AutoFind: Scans 1705, 1706, 1707; Background Corrected with Scan 1698

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.8	6128	PASS
75	95	30	60	46.6	16961	PASS
95	95	100	100	100.0	36421	PASS
96	95	5	9	6.7	2430	PASS
173	174	0.00	2	0.9	270	PASS
174	95	50	100	81.5	29685	PASS
175	174	5	9	7.1	2119	PASS
176	174	95	101	96.5	28643	PASS
177	176	5	9	6.0	1714	PASS