

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031022\
Data File : VX027384.D
Acq On : 10 Mar 2022 18:16
Operator : JC/MD
Sample : N1889-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-01-031022

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M

Title : SW846 8260

Signal : TIC: VX027384.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.257	23	28	33	rBV2	11473	25763	1.42%	0.263%
2	2.538	230	238	247	rBV	16541	32137	1.77%	0.327%
3	5.391	693	706	721	rBV	218078	632225	34.86%	6.442%
4	5.555	722	733	752	rVB	376483	1057406	58.31%	10.775%
5	5.958	788	799	814	rBV	210827	555539	30.64%	5.661%
6	6.763	921	931	946	rBV	556401	1325524	73.10%	13.507%
7	8.652	1234	1241	1250	rBV	1156073	1813373	100.00%	18.478%
8	10.055	1465	1471	1486	rBV	1194456	1590469	87.71%	16.207%
9	11.085	1634	1640	1650	rBV	970783	1229767	67.82%	12.531%
10	12.024	1788	1794	1808	rBV	1242548	1528804	84.31%	15.579%
11	14.603	2210	2217	2220	rBV2	13403	22529	1.24%	0.230%




Sum of corrected areas: 9813536

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031022\
Data File : VX027384.D
Acq On : 10 Mar 2022 18:16
Operator : JC/MD
Sample : N1889-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-01-031022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

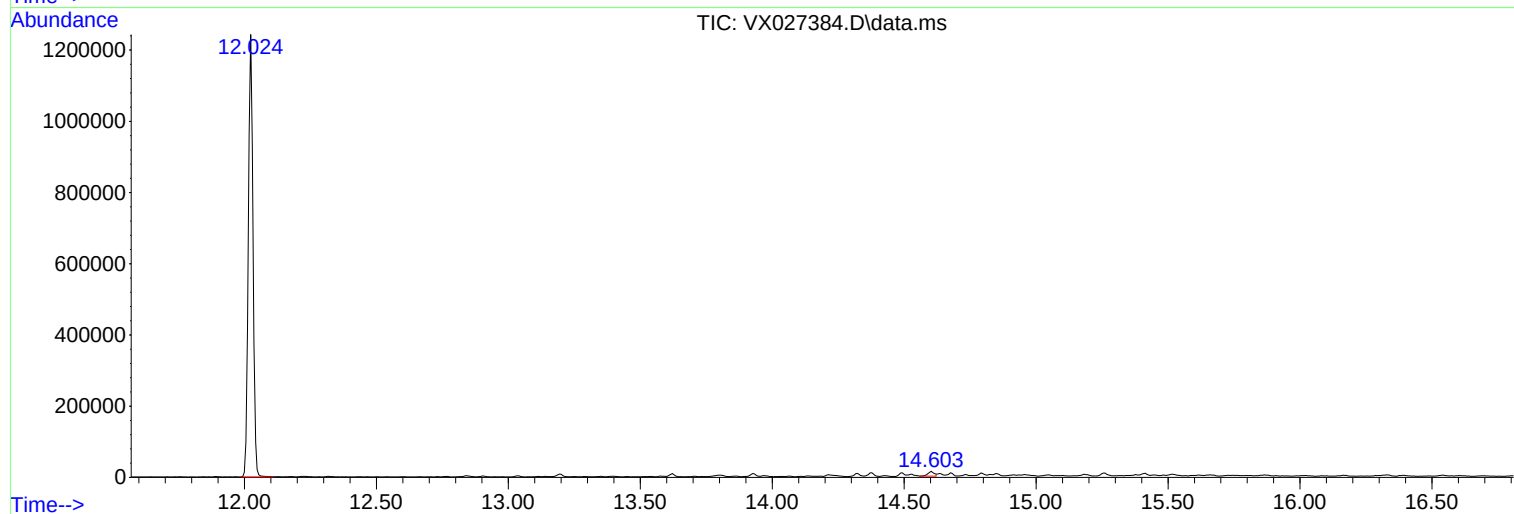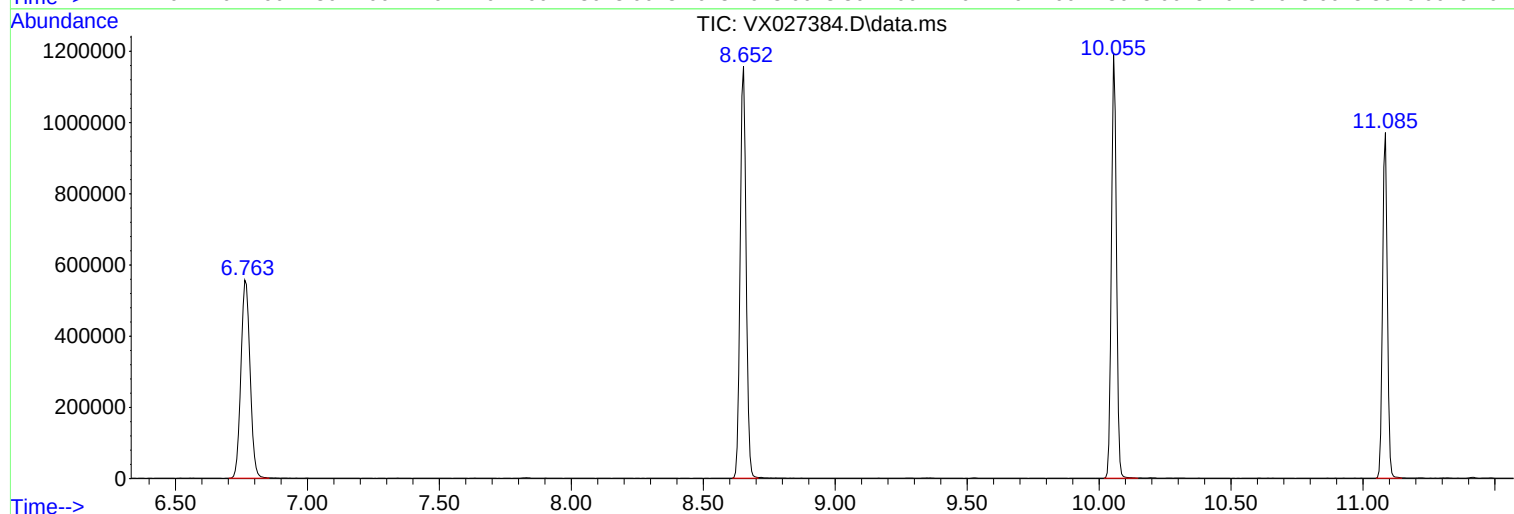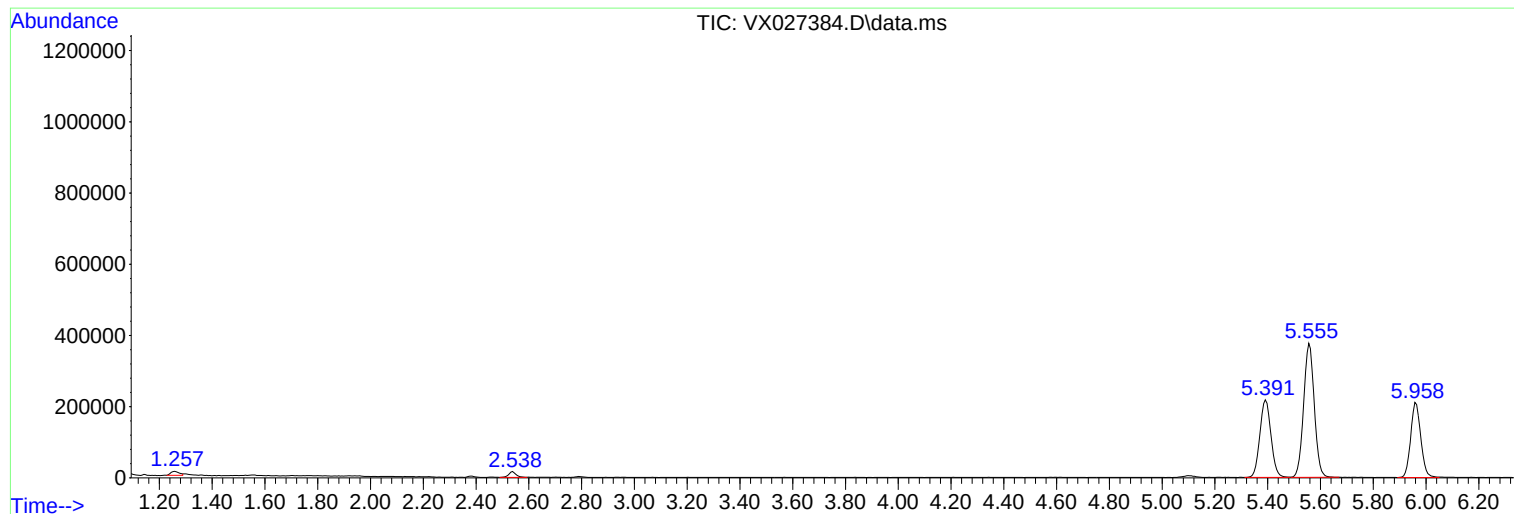

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031022\
Data File : VX027384.D
Acq On : 10 Mar 2022 18:16
Operator : JC/MD
Sample : N1889-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-01-031022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031022\
Data File : VX027384.D
Acq On : 10 Mar 2022 18:16
Operator : JC/MD
Sample : N1889-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-01-031022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------