
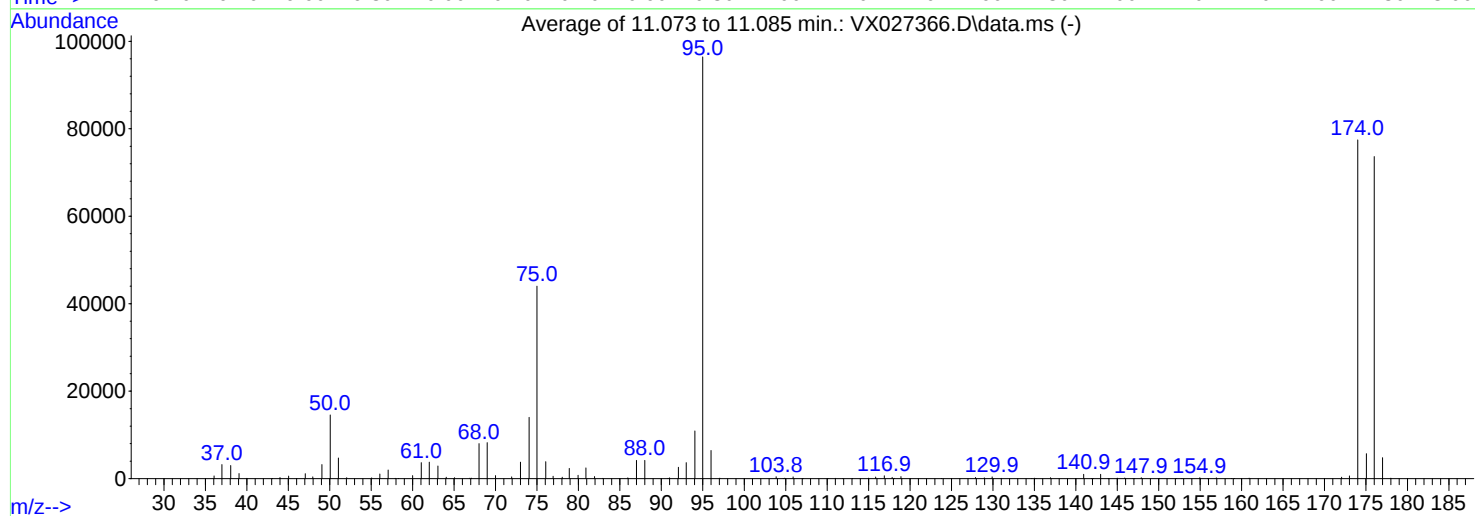


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031022\
 Data File : VX027366.D
 Acq On : 10 Mar 2022 10:16
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
 Title : SW846 8260
 Last Update : Tue Mar 08 15:54:34 2022

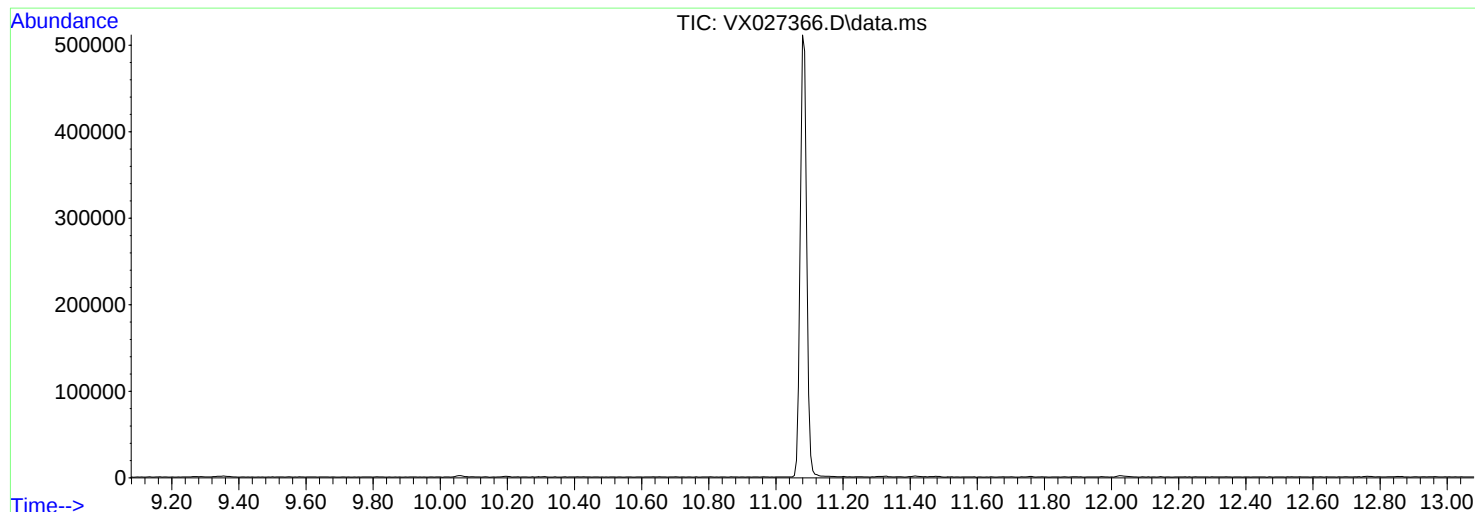

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	14575	PASS
75	95	30	60	45.7	44029	PASS
95	95	100	100	100.0	96448	PASS
96	95	5	9	6.7	6427	PASS
173	174	0.00	2	0.8	632	PASS
174	95	50	100	80.3	77464	PASS
175	174	5	9	7.4	5707	PASS
176	174	95	101	95.1	73667	PASS
177	176	5	9	6.5	4812	PASS