
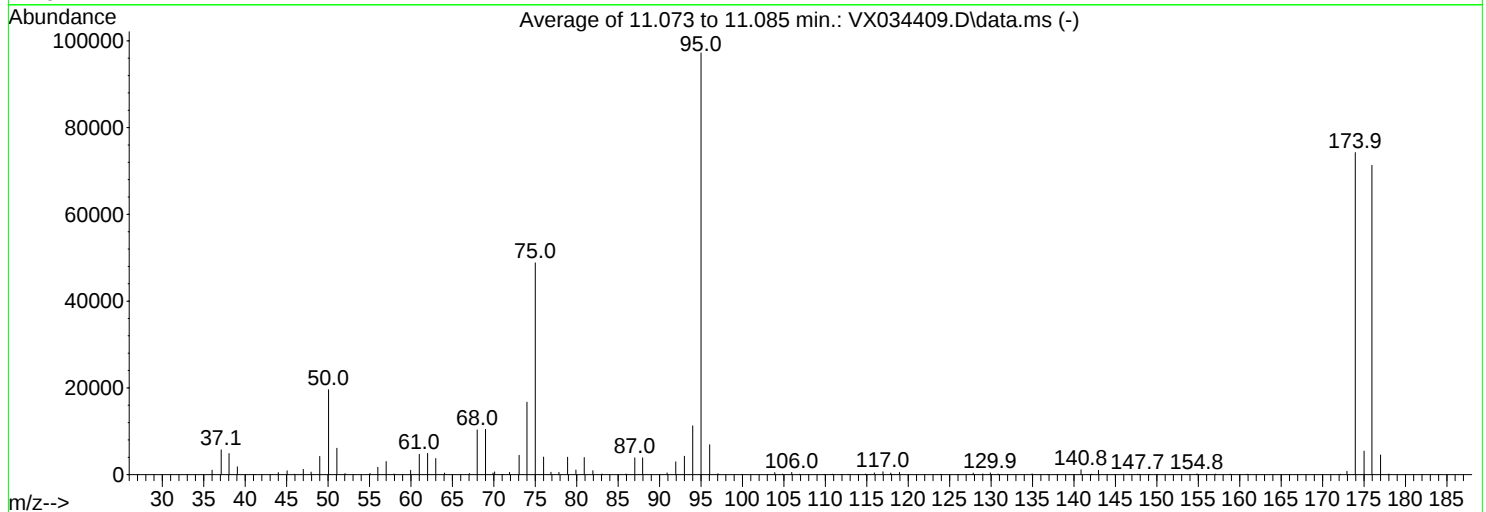


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031023\
Data File : VX034409.D
Acq On : 10 Mar 2023 09:36
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Title : SW846 8260
Last Update : Mon Mar 13 10:29:32 2023

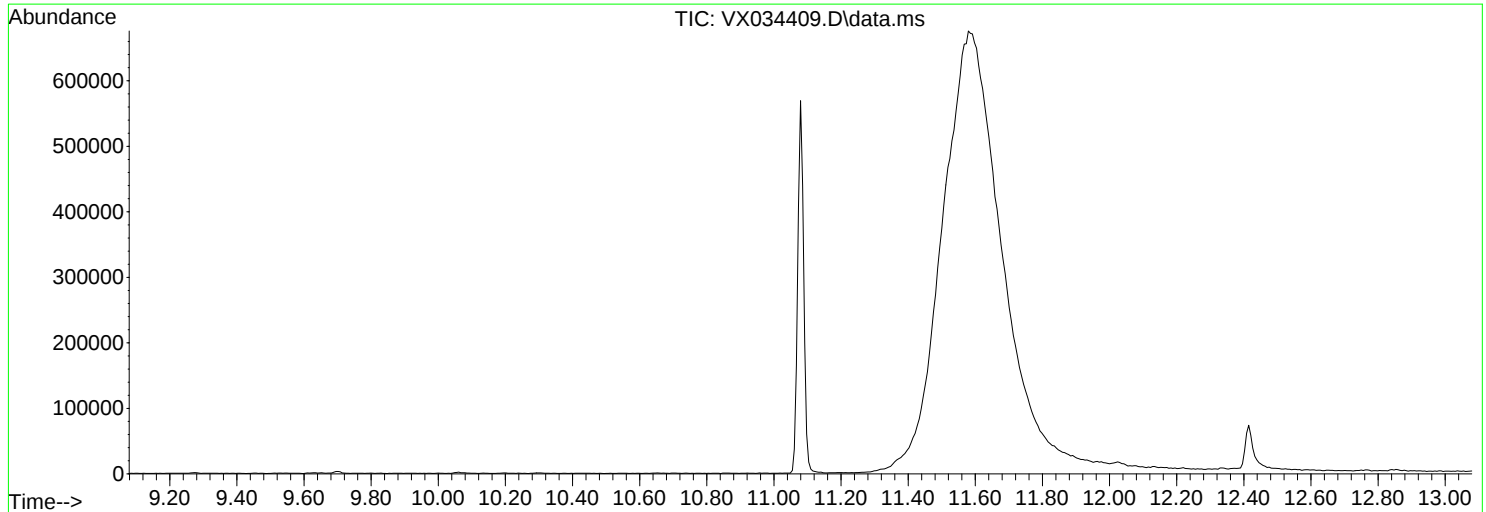

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.2	19595	PASS
75	95	30	60	50.2	48835	PASS
95	95	100	100	100.0	97235	PASS
96	95	5	9	7.1	6913	PASS
173	174	0.00	2	1.1	782	PASS
174	95	50	100	76.3	74235	PASS
175	174	5	9	7.3	5420	PASS
176	174	95	101	96.0	71301	PASS
177	176	5	9	6.4	4552	PASS