

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031025\
 Data File : VX045185.D
 Acq On : 10 Mar 2025 10:57
 Operator : JC/MD
 Sample : VX0310WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0310WBL01

Quant Time: Mar 11 03:51:06 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	76457	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	152674	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	139915	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	59432	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	64489	53.027	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 106.060%	
35) Dibromofluoromethane	5.379	113	52216	51.147	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 102.300%	
50) Toluene-d8	8.647	98	187192	50.578	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 101.160%	
62) 4-Bromofluorobenzene	11.079	95	65631	53.514	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 107.020%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031025\
Data File : VX045185.D
Acq On : 10 Mar 2025 10:57
Operator : JC/MD
Sample : VX0310WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0310WBL01

Quant Time: Mar 11 03:51:06 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration




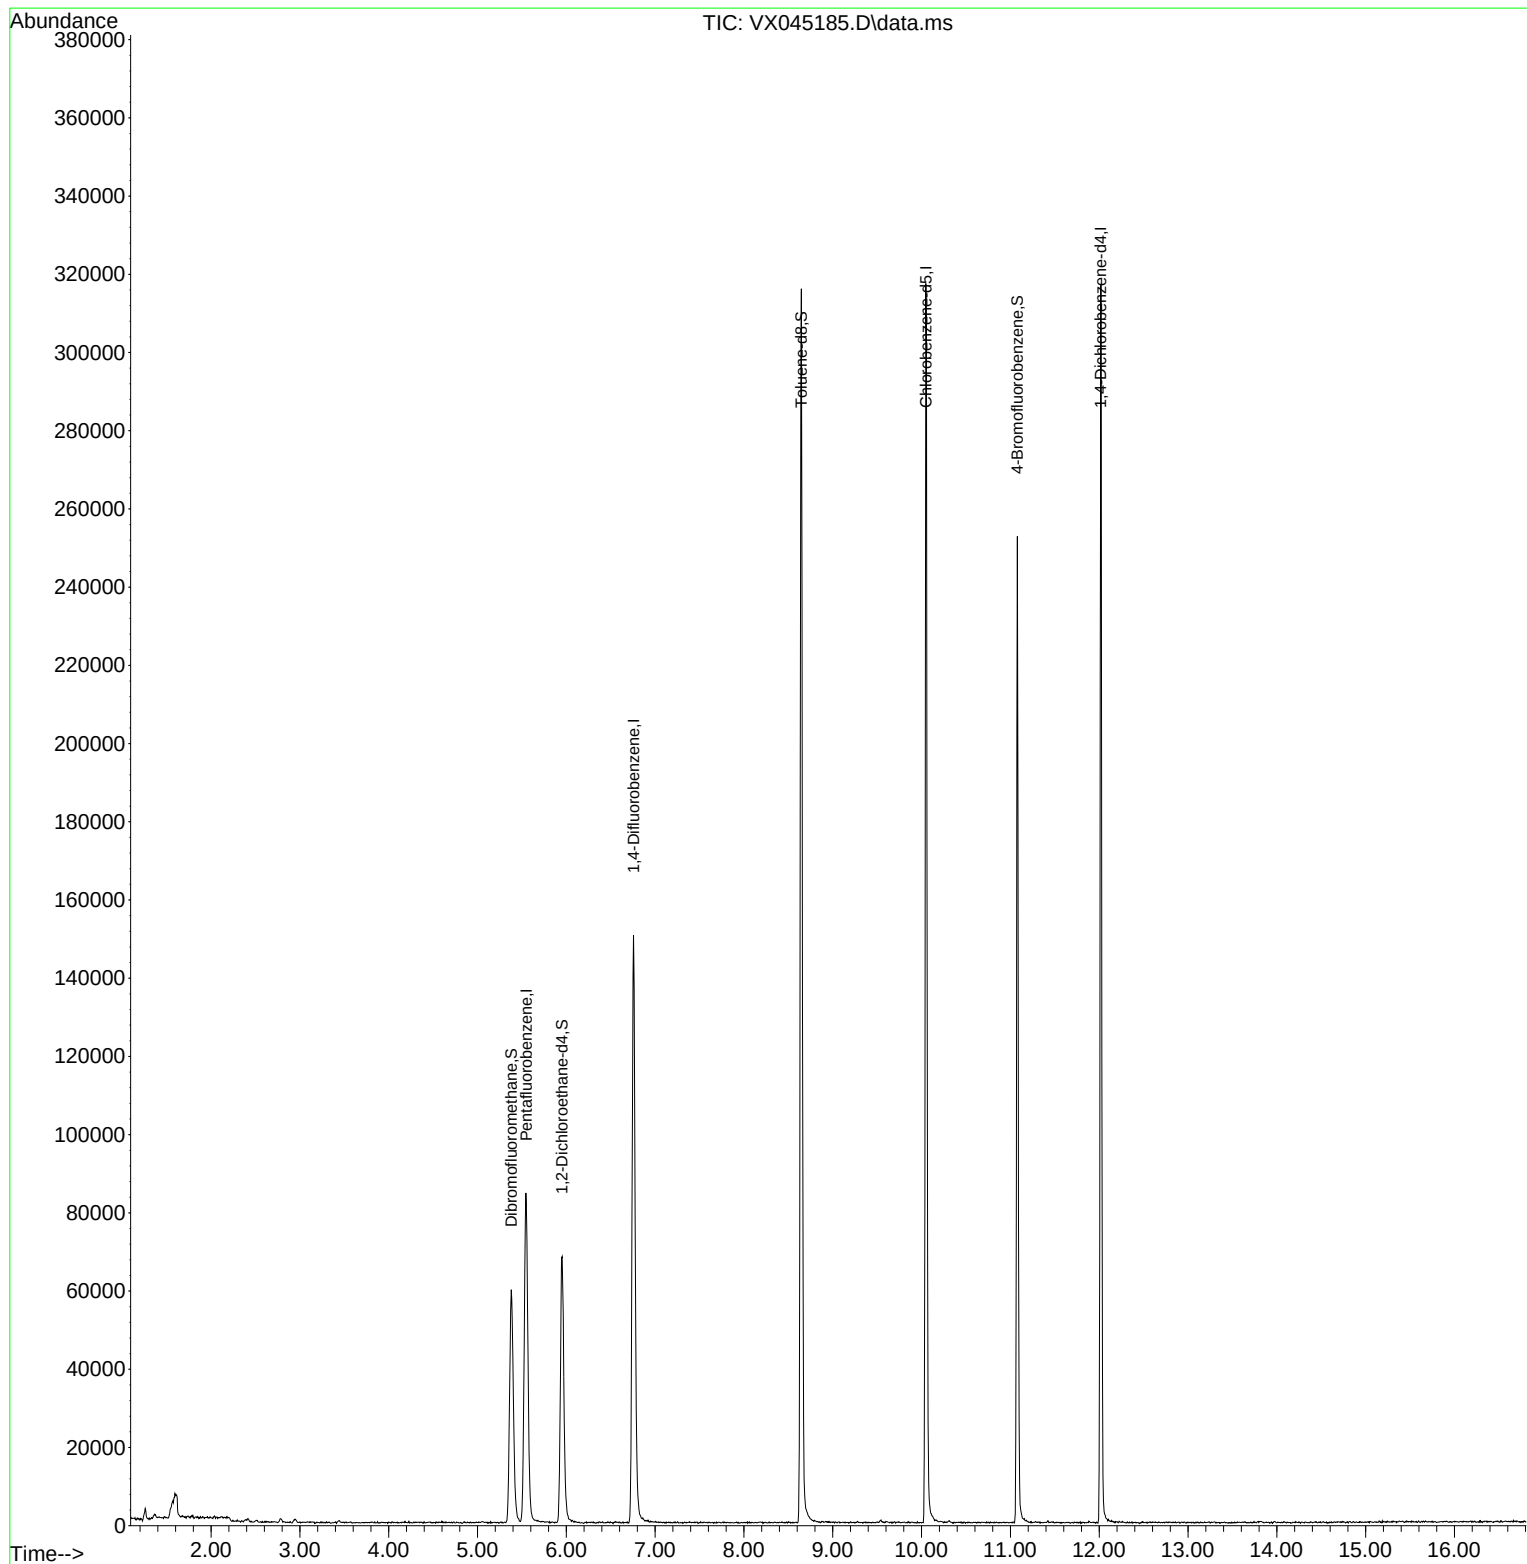


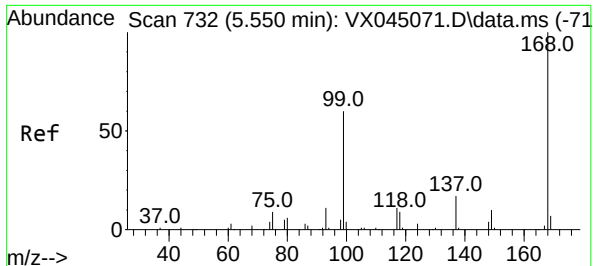

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX045185.D
Acq: 10 Mar 2025 10:57




Instrument :
MSVOA_X
ClientSampleId :
VX0310WBL01


Tgt Ion:168 Resp: 76457
Ion Ratio Lower Upper
168 100
99 62.5 48.2 72.4

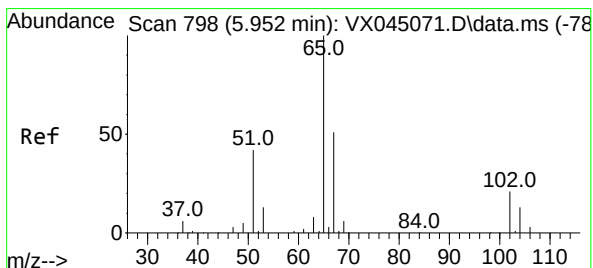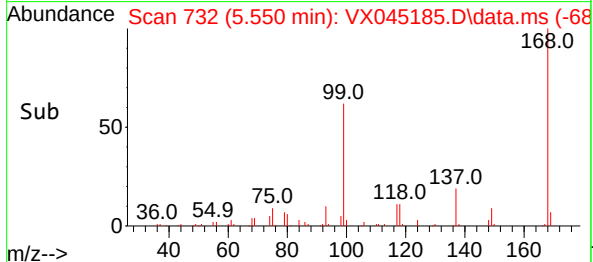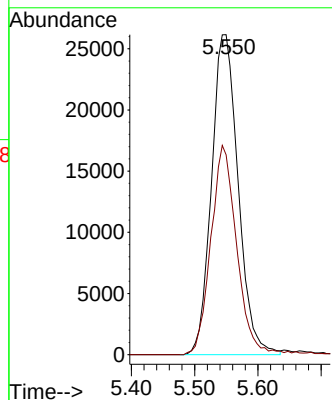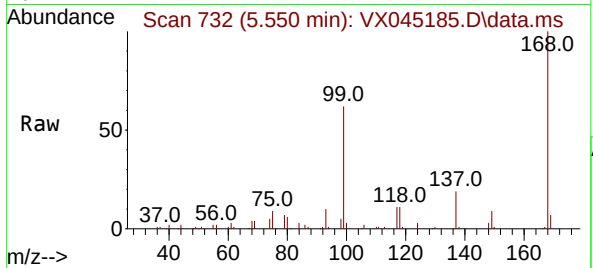

#33
1,2-Dichloroethane-d4
Concen: 53.027 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX045185.D
Acq: 10 Mar 2025 10:57

Tgt Ion: 65 Resp: 64489
Ion Ratio Lower Upper
65 100
67 52.9 0.0 106.2


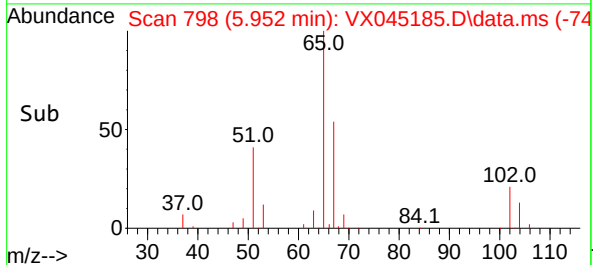
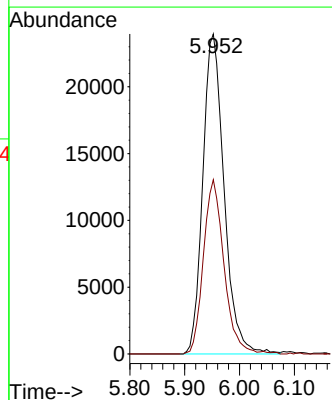
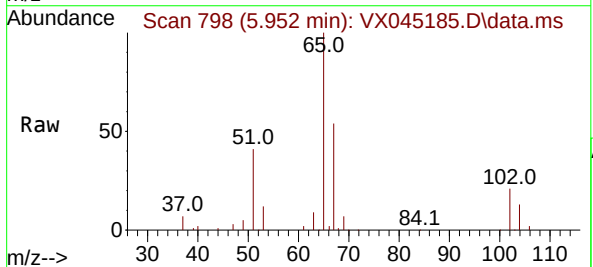


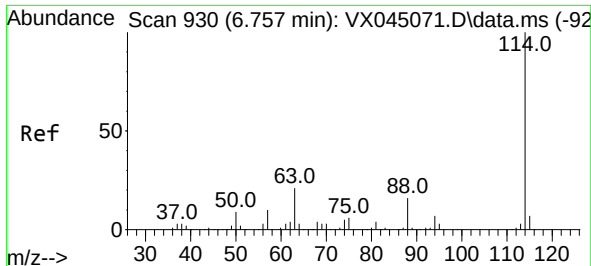

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX045185.D
Acq: 10 Mar 2025 10:57




Instrument :
MSVOA_X
ClientSampleId :
VX0310WBL01


Tgt Ion:114 Resp: 152674
Ion Ratio Lower Upper
114 100
63 22.3 0.0 41.8
88 15.7 0.0 32.8

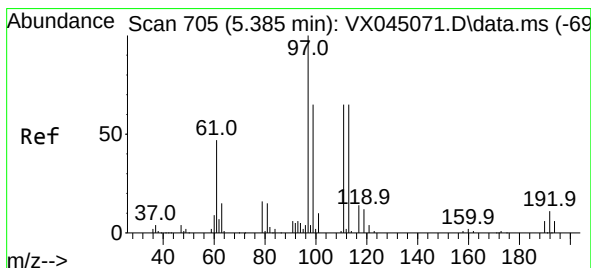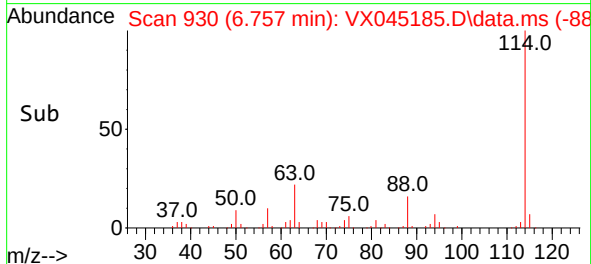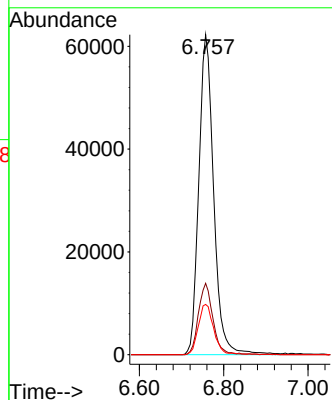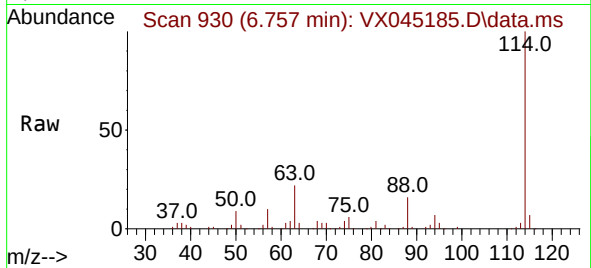

#35
Dibromofluoromethane
Concen: 51.147 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.006 min
Lab File: VX045185.D
Acq: 10 Mar 2025 10:57

Tgt Ion:113 Resp: 52216
Ion Ratio Lower Upper
113 100
111 104.5 81.8 122.6
192 17.9 14.3 21.5


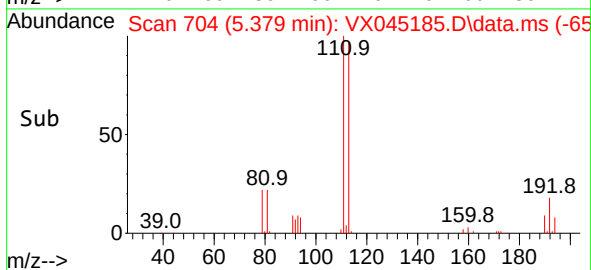
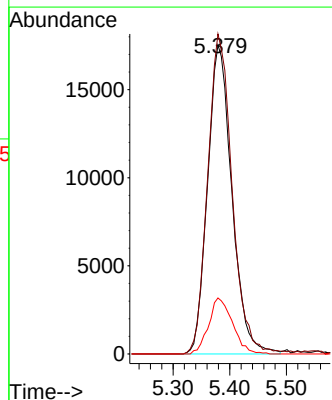
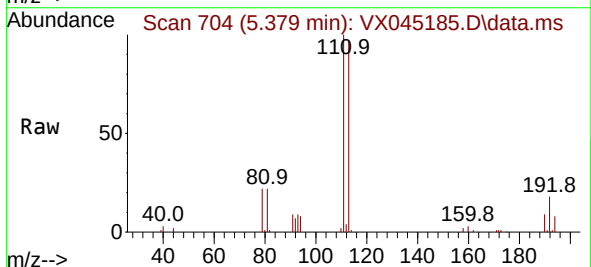


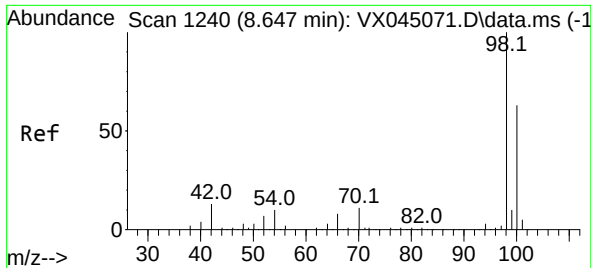

#50
Toluene-d8
Concen: 50.578 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX045185.D
Acq: 10 Mar 2025 10:57




Instrument :
MSVOA_X
ClientSampleId :
VX0310WBL01


Tgt Ion: 98 Resp: 187192
Ion Ratio Lower Upper
98 100
100 65.7 52.0 78.0

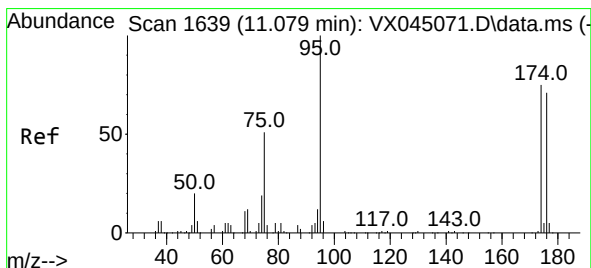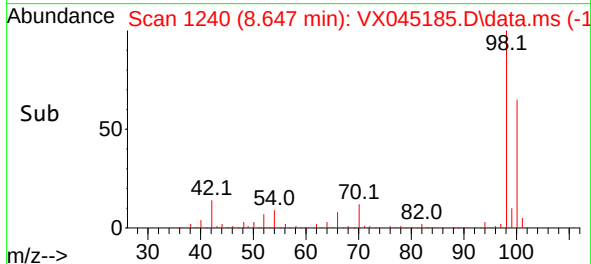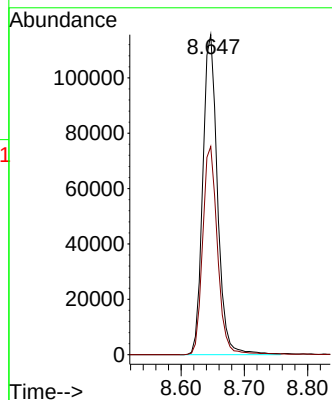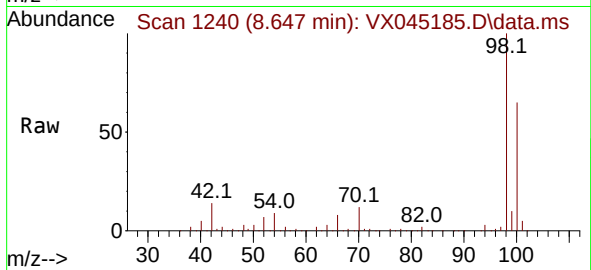

#62
4-Bromofluorobenzene
Concen: 53.514 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045185.D
Acq: 10 Mar 2025 10:57

Tgt Ion: 95 Resp: 65631
Ion Ratio Lower Upper
95 100
174 72.5 0.0 148.2
176 69.9 0.0 141.4


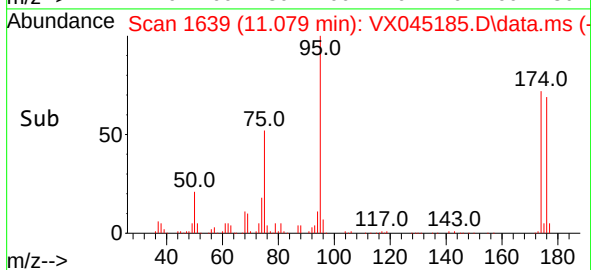
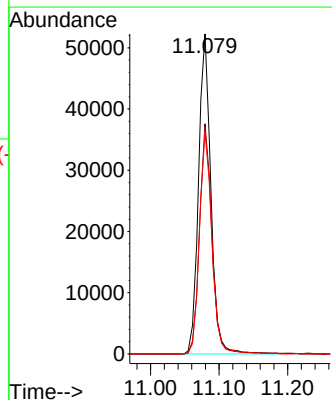
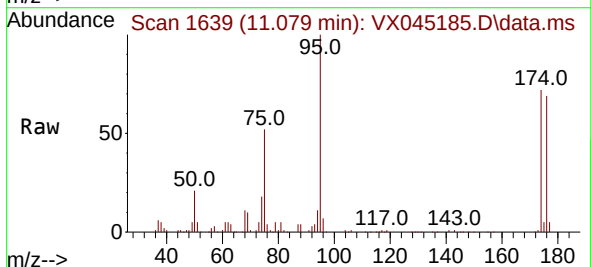


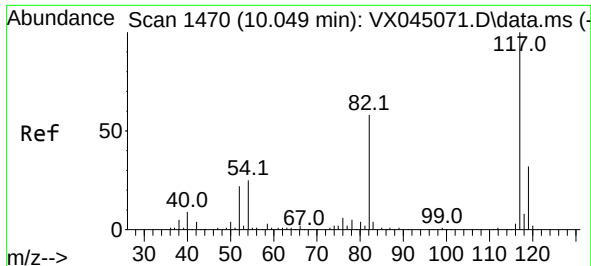

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX045185.D
Acq: 10 Mar 2025 10:57

Instrument :
MSVOA_X
ClientSampleId :
VX0310WBL01

Tgt Ion:117 Resp: 139915
Ion Ratio Lower Upper
117 100
82 59.4 46.3 69.5
119 31.8 25.7 38.5

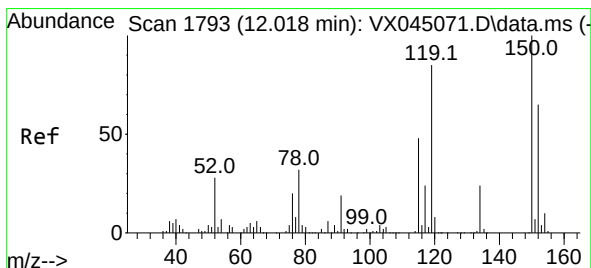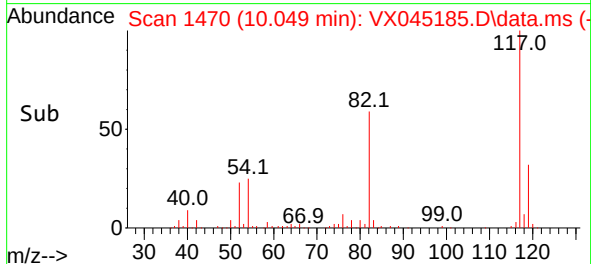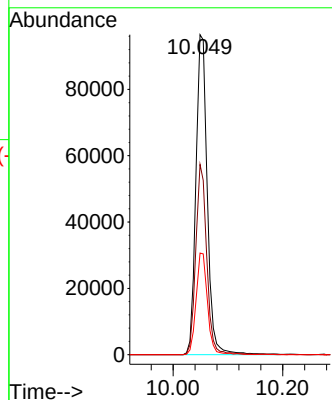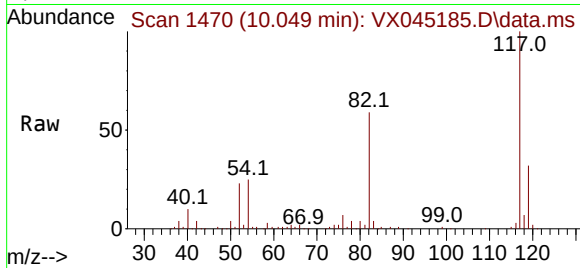

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX045185.D
Acq: 10 Mar 2025 10:57

Tgt Ion:152 Resp: 59432
Ion Ratio Lower Upper
152 100
115 61.9 44.2 132.6
150 160.1 0.0 349.0

