

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031025\  
Data File : VX045201.D  
Acq On : 10 Mar 2025 17:12  
Operator : JC/MD  
Sample : Q1531-11  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RE103D2-20250306

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X022825W.M

Title : SW846 8260

Signal : TIC: VX045201.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.385       | 692           | 705         | 720          | rBV      | 54039          | 160499        | 7.90%           | 3.669%        |
| 2         | 5.550       | 721           | 732         | 746          | rVV2     | 74255          | 217095        | 10.69%          | 4.963%        |
| 3         | 5.952       | 789           | 798         | 811          | rBV2     | 61094          | 164714        | 8.11%           | 3.766%        |
| 4         | 6.757       | 922           | 930         | 941          | rBV      | 138129         | 326835        | 16.09%          | 7.472%        |
| 5         | 7.122       | 981           | 990         | 1016         | rBV      | 905575         | 2031753       | 100.00%         | 46.451%       |
| 6         | 8.647       | 1232          | 1240        | 1255         | rBV      | 289945         | 463910        | 22.83%          | 10.606%       |
| 7         | 10.049      | 1465          | 1470        | 1486         | rBV      | 282962         | 402422        | 19.81%          | 9.200%        |
| 8         | 11.079      | 1634          | 1639        | 1652         | rBV      | 219467         | 279436        | 13.75%          | 6.389%        |
| 9         | 12.018      | 1788          | 1793        | 1805         | rBV      | 257959         | 327299        | 16.11%          | 7.483%        |




Sum of corrected areas: 4373963

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031025\  
Data File : VX045201.D  
Acq On : 10 Mar 2025 17:12  
Operator : JC/MD  
Sample : Q1531-11  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RE103D2-20250306

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X022825W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

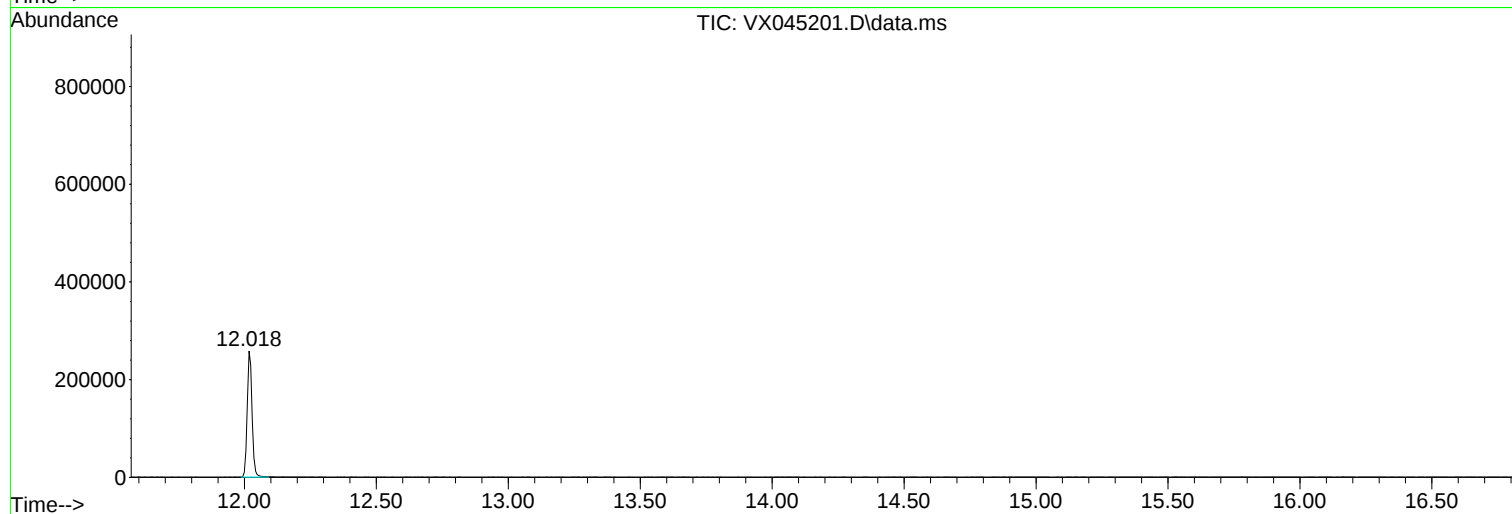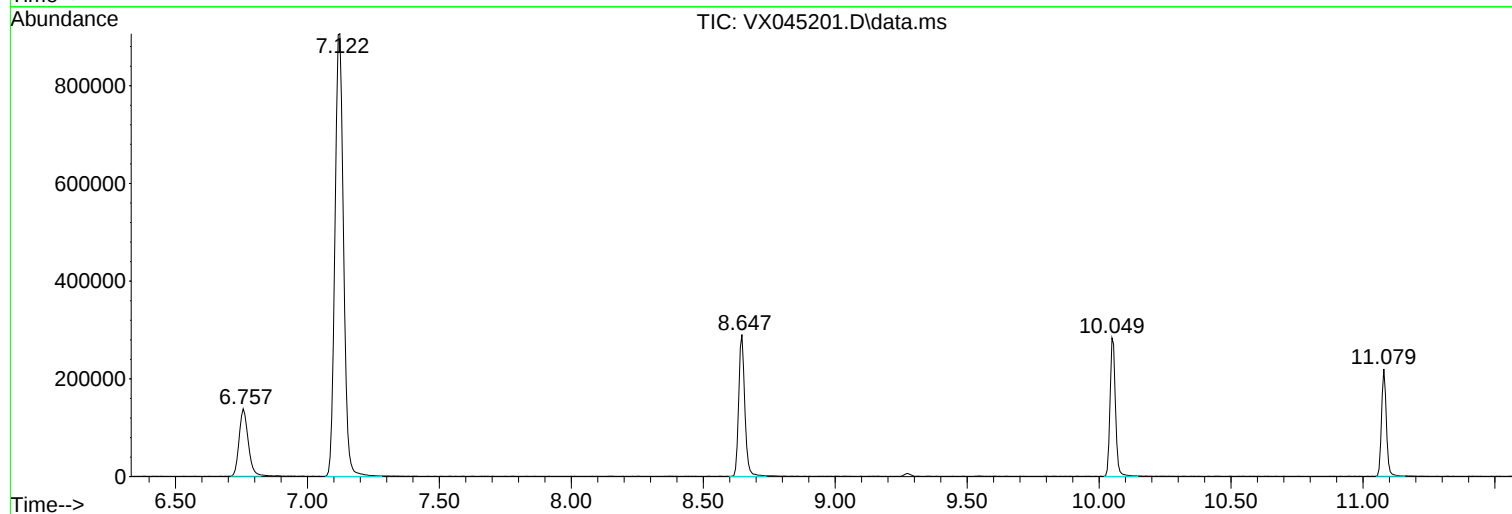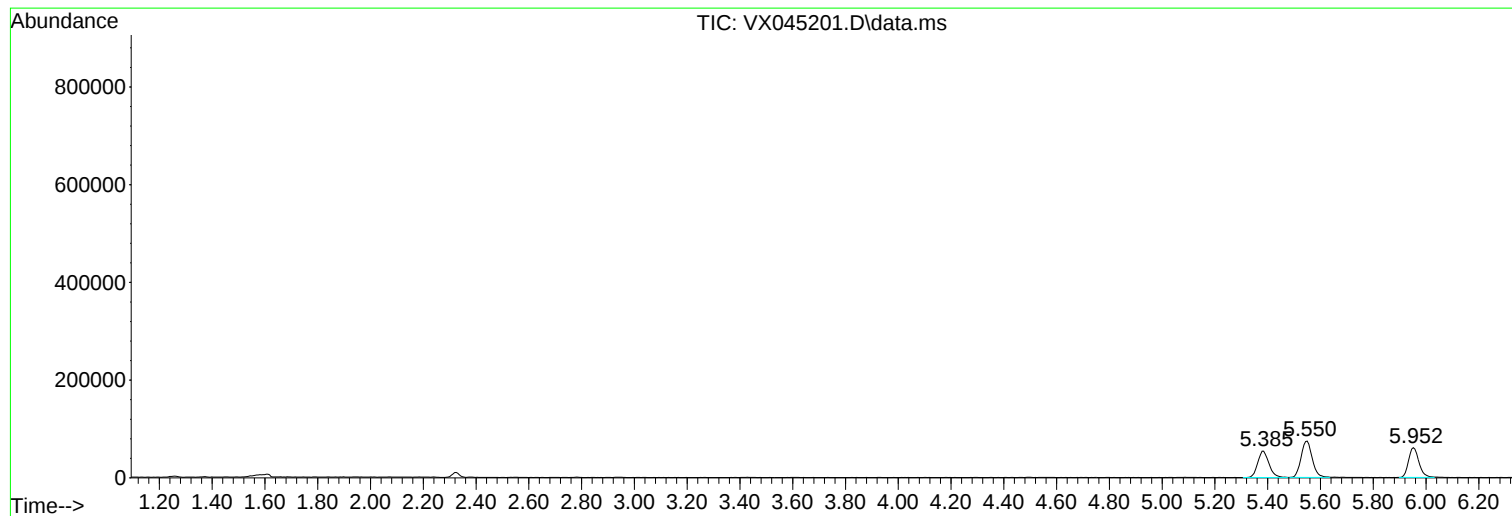

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031025\  
Data File : VX045201.D  
Acq On : 10 Mar 2025 17:12  
Operator : JC/MD  
Sample : Q1531-11  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RE103D2-20250306

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X022825W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031025\  
Data File : VX045201.D  
Acq On : 10 Mar 2025 17:12  
Operator : JC/MD  
Sample : Q1531-11  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RE103D2-20250306

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X022825W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |