


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031119\
Data File : VX007959.D
Acq On : 11 Mar 2019 09:06
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X030819W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Mar 08 12:01:36 2019

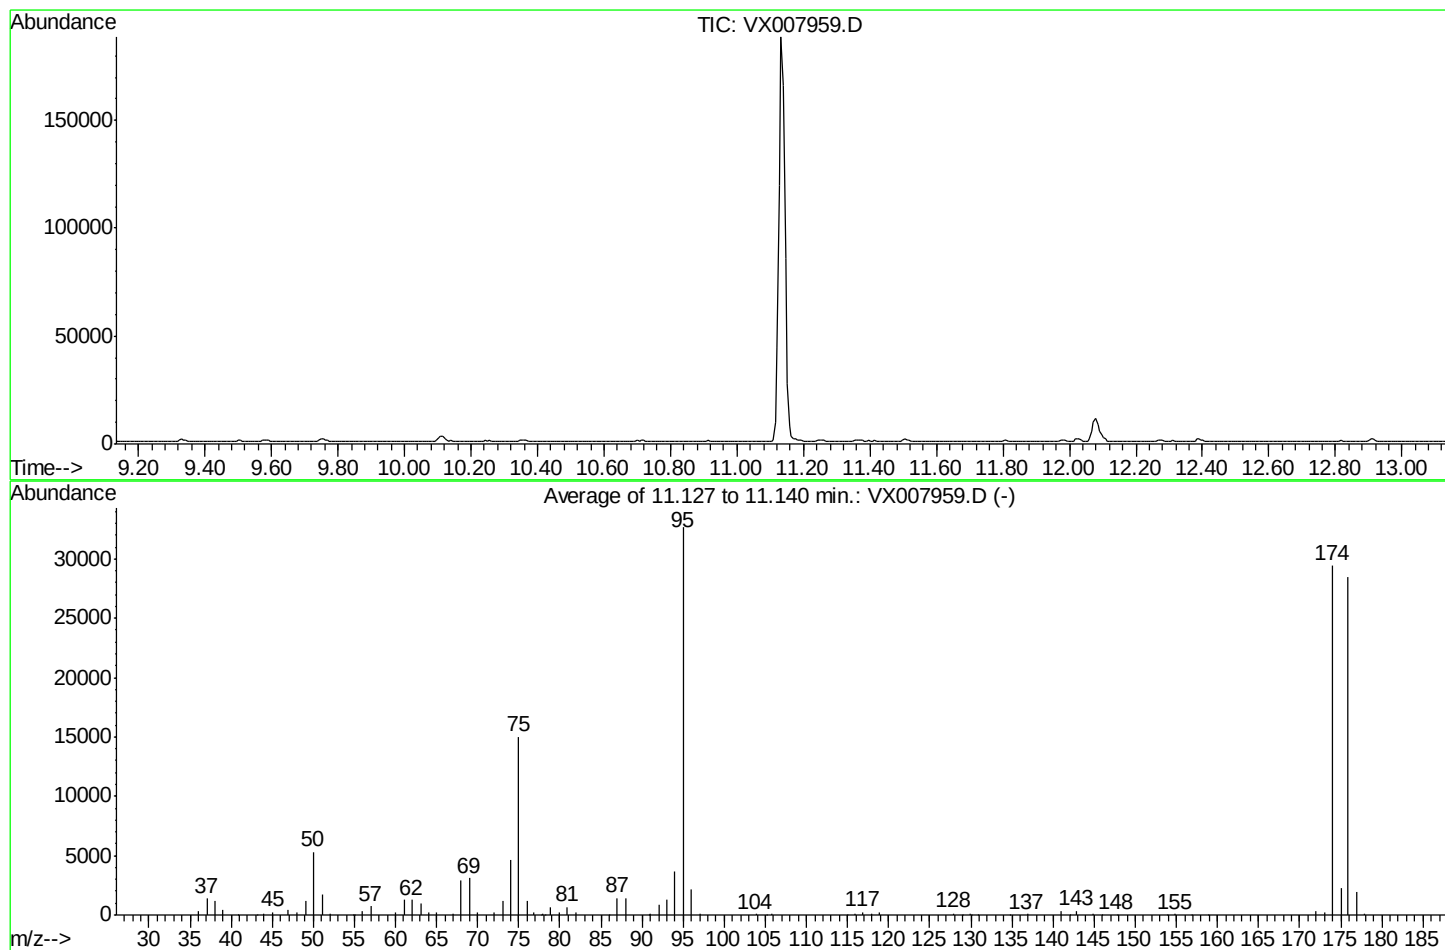

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	5304	PASS
75	95	30	60	45.9	14994	PASS
95	95	100	100	100.0	32658	PASS
96	95	5	9	6.6	2169	PASS
173	174	0.00	2	0.7	208	PASS
174	95	50	100	90.1	29424	PASS
175	174	5	9	7.6	2230	PASS
176	174	95	101	96.9	28512	PASS
177	176	5	9	6.8	1933	PASS