


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031119\
 Data File : VX007968.D
 Acq On : 11 Mar 2019 14:05
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X030619W.M
 Title : SW846 8260
 Last Update : Thu Mar 07 07:33:26 2019

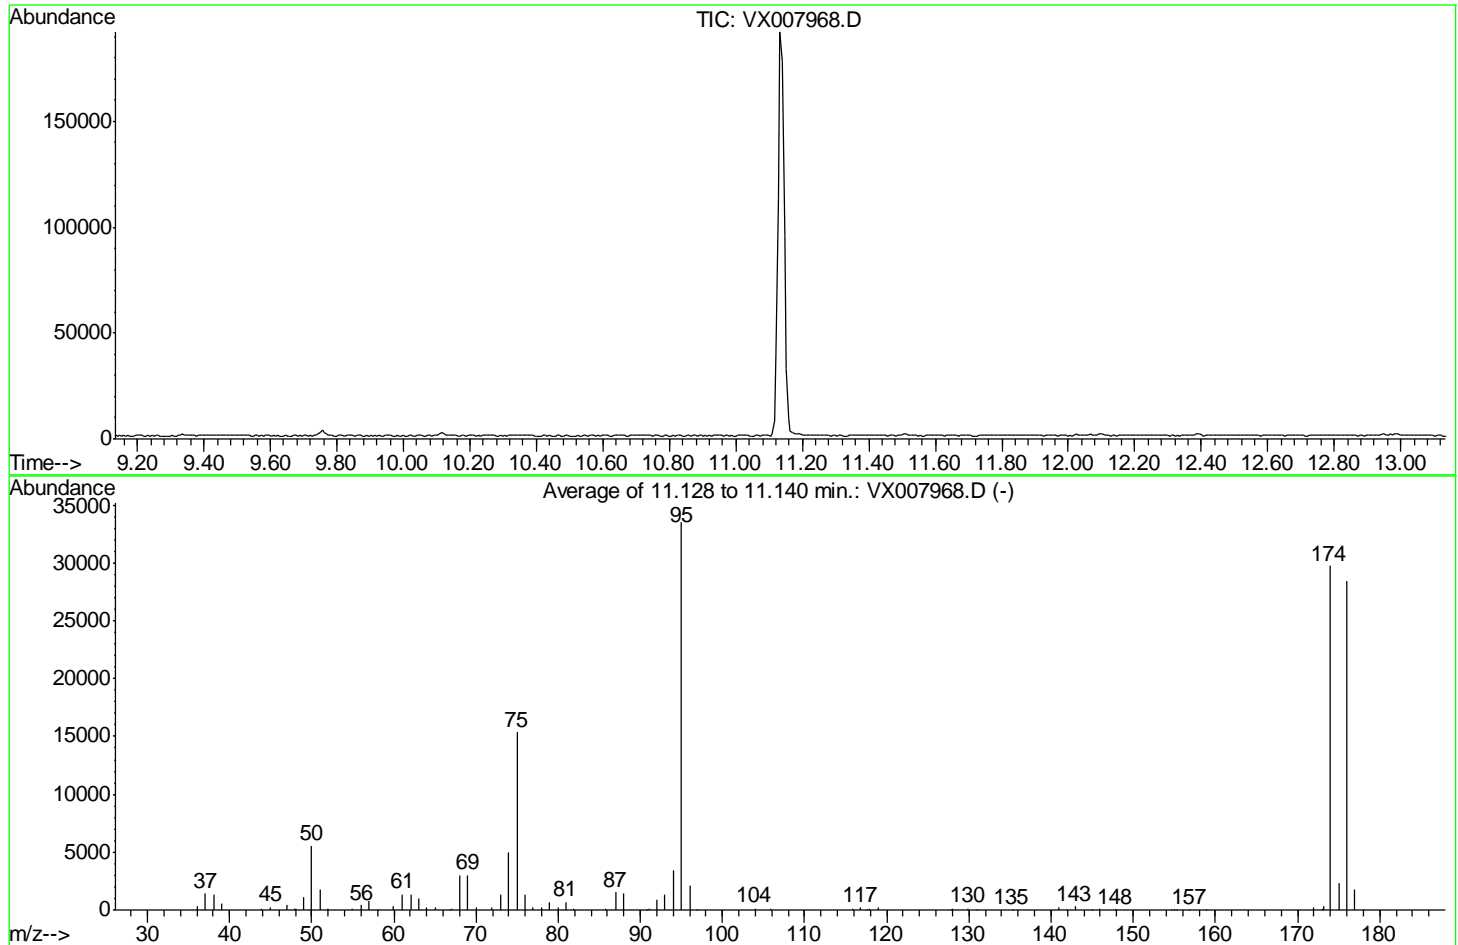

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	5559	PASS
75	95	30	60	45.9	15373	PASS
95	95	100	100	100.0	33506	PASS
96	95	5	9	6.4	2154	PASS
173	174	0.00	2	1.0	298	PASS
174	95	50	100	88.7	29709	PASS
175	174	5	9	7.7	2294	PASS
176	174	95	101	95.8	28450	PASS
177	176	5	9	6.4	1829	PASS