


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX031119\
 Data File : VX007991.D
 Acq On : 12 Mar 2019 01:09
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X030819W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Mar 08 12:01:36 2019

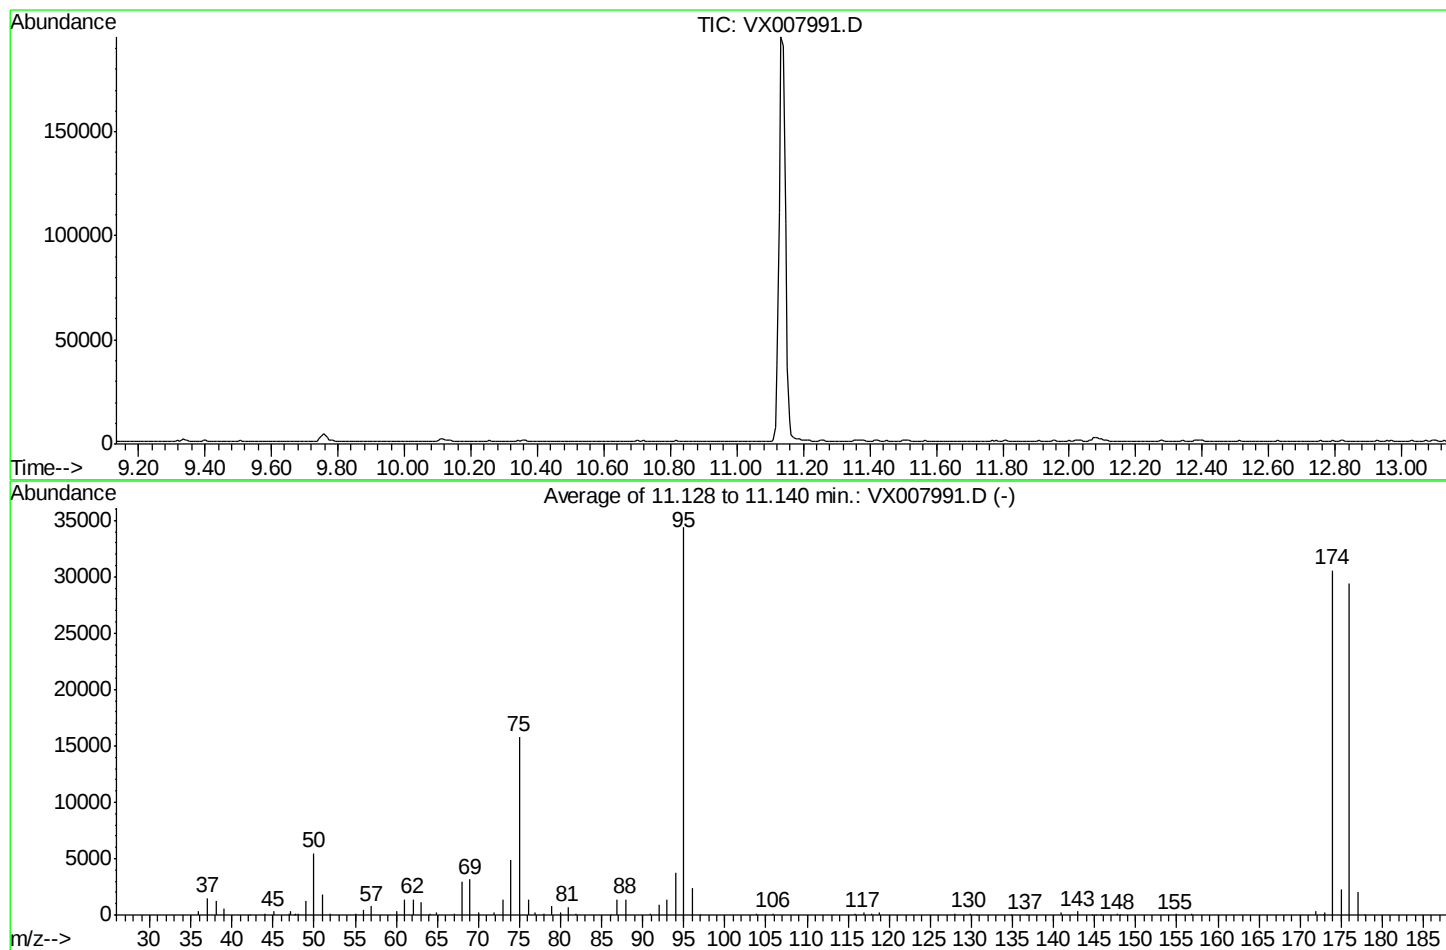

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	5508	PASS
75	95	30	60	46.0	15820	PASS
95	95	100	100	100.0	34386	PASS
96	95	5	9	6.9	2365	PASS
173	174	0.00	2	0.8	252	PASS
174	95	50	100	88.9	30568	PASS
175	174	5	9	7.6	2309	PASS
176	174	95	101	96.1	29386	PASS
177	176	5	9	7.0	2060	PASS