


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031120\
 Data File : VX015184.D
 Acq On : 11 Mar 2020 08:21
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X030420W.M
 Title : SW846 8260
 Last Update : Wed Mar 04 14:19:10 2020

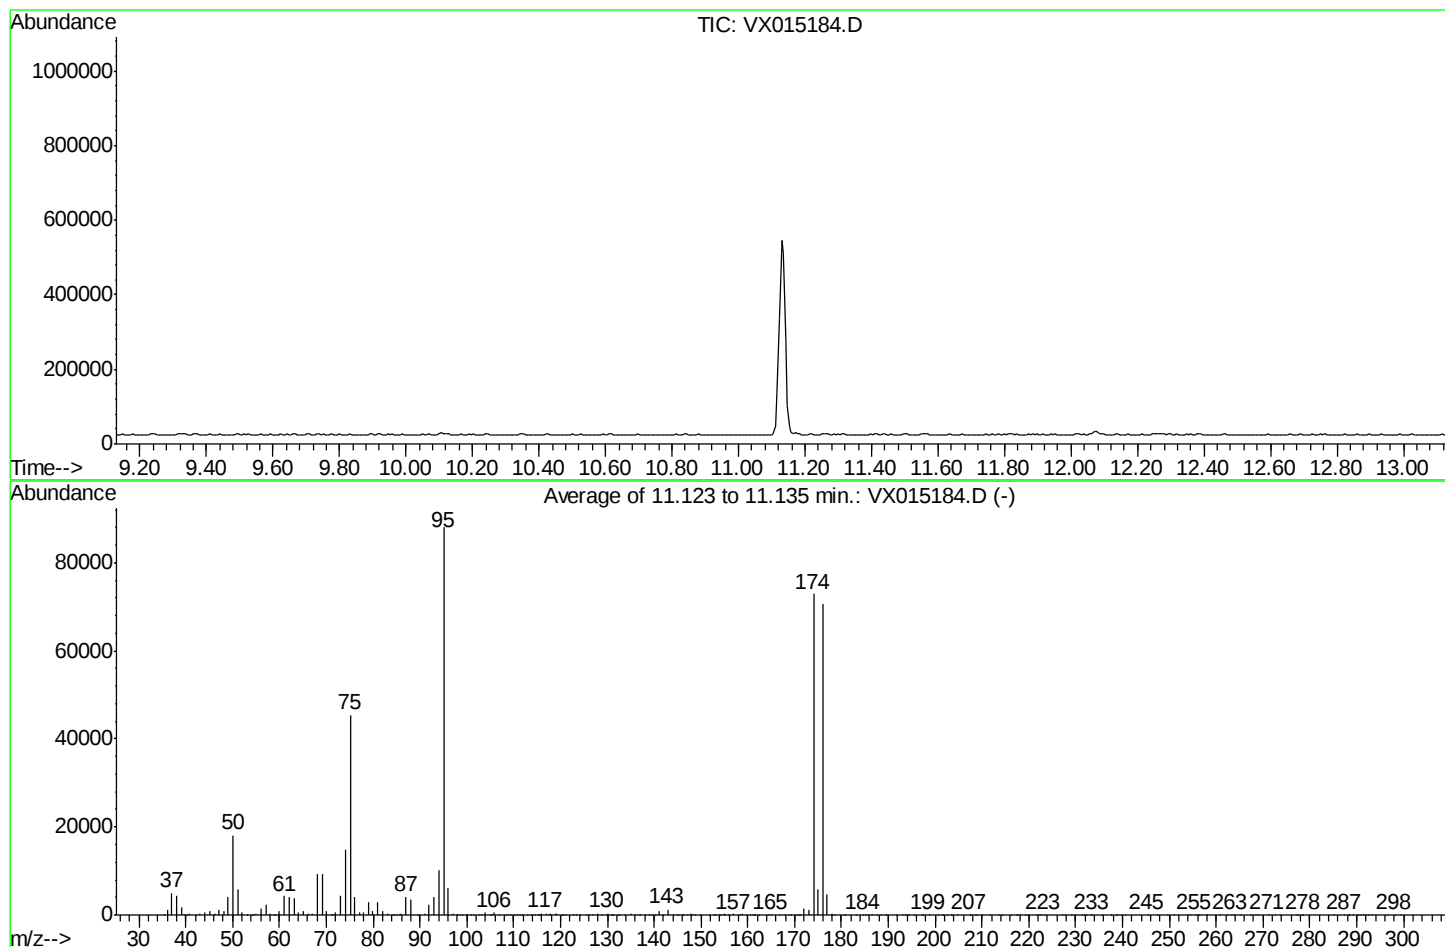

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1670

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	18112	PASS
75	95	30	60	51.6	45461	PASS
95	95	100	100	100.0	88042	PASS
96	95	5	9	6.9	6080	PASS
173	174	0.00	2	1.6	1199	PASS
174	95	50	100	82.9	72965	PASS
175	174	5	9	7.9	5742	PASS
176	174	95	101	96.7	70535	PASS
177	176	5	9	6.4	4521	PASS