

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031121\
 Data File : VX021156.D
 Acq On : 11 Mar 2021 15:18
 Operator : JC/MD
 Sample : M1605-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Mar 12 02:20:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 24 13:50:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.629	168	213666	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.829	114	395420	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.094	117	373910	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.059	152	183339	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.029	65	140002	48.51	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	97.02%		
35) Dibromofluoromethane	5.464	113	122692	51.07	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	102.14%		
50) Toluene-d8	8.694	98	495503	52.90	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	105.80%		
62) 4-Bromofluorobenzene	11.118	95	192032	55.44	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	110.88%		
Target Compounds						Qvalue
5) Bromomethane	1.646	94	560	Below Cal		97
11) Tert butyl alcohol	3.023	59	2849	4.43 ug/l #		90
13) Acrolein	2.276	56	245	0.62 ug/l #		14
16) Acetone	2.423	43	67618	56.86 ug/l		98
18) Methyl Acetate	2.752	43	768	0.27 ug/l		99
20) Methylene Chloride	2.834	84	616	0.22 ug/l #		79
25) 2-Butanone	4.641	43	21547	11.93 ug/l		99
29) Tetrahydrofuran	5.111	42	408	0.35 ug/l #		43
36) 1,1-Dichloropropene	5.629	75	16978	4.52 ug/l #		48
37) Ethyl Acetate	4.799	43	1522	0.43 ug/l #		86
38) Carbon Tetrachloride	5.623	117	20161	5.54 ug/l #		16
40) Benzene	6.111	78	6924	0.61 ug/l		99
51) 4-Methyl-2-Pentanone	8.618	43	2369	0.67 ug/l		97
52) Toluene	8.765	92	51572	7.35 ug/l		98
59) 2-Hexanone	9.471	43	3144	1.18 ug/l		95
67) Ethyl Benzene	10.235	91	71144	4.98 ug/l		99
68) m/p-Xylenes	10.341	106	143359	27.29 ug/l		96
69) o-Xylene	10.682	106	92184	17.98 ug/l		98
70) Styrene	10.682	104	7776	0.88 ug/l #		1
73) Isopropylbenzene	11.000	105	14445	1.00 ug/l		98
76) 1,2,3-Trichloropropane	11.418	75	3734	0.95 ug/l #		1
78) n-propylbenzene	11.341	91	77224	4.68 ug/l		98
79) 2-Chlorotoluene	11.418	91	50456	5.04 ug/l #		41
80) 1,3,5-Trimethylbenzene	11.488	105	158083	13.12 ug/l		98
81) trans-1,4-Dichloro-2-b...	11.118	75	91721	51.49 ug/l #		12
82) 4-Chlorotoluene	11.488	91	15796	1.37 ug/l #		45
83) tert-Butylbenzene	11.789	119	85412	7.29 ug/l #		64
84) 1,2,4-Trimethylbenzene	11.789	105	700642	57.28 ug/l		98
85) sec-Butylbenzene	11.789	105	700642	50.72 ug/l #		57
86) p-Isopropyltoluene	12.006	119	18763	1.48 ug/l		97
89) n-Butylbenzene	12.359	91	37836	3.35 ug/l #		16
90) Hexachloroethane	12.571	117	9371	3.88 ug/l #		9
92) 1,2-Dibromo-3-Chloropr...	12.959	75	935	0.87 ug/l #		1
95) Naphthalene	13.818	128	628043	46.71 ug/l		100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031121\
Data File : VX021156.D
Acq On : 11 Mar 2021 15:18
Operator : JC/MD
Sample : M1605-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Mar 12 02:20:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 24 13:50:55 2021
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Quant Time: Mar 12 02:20:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 24 13:50:55 2021
Response via : Initial Calibration




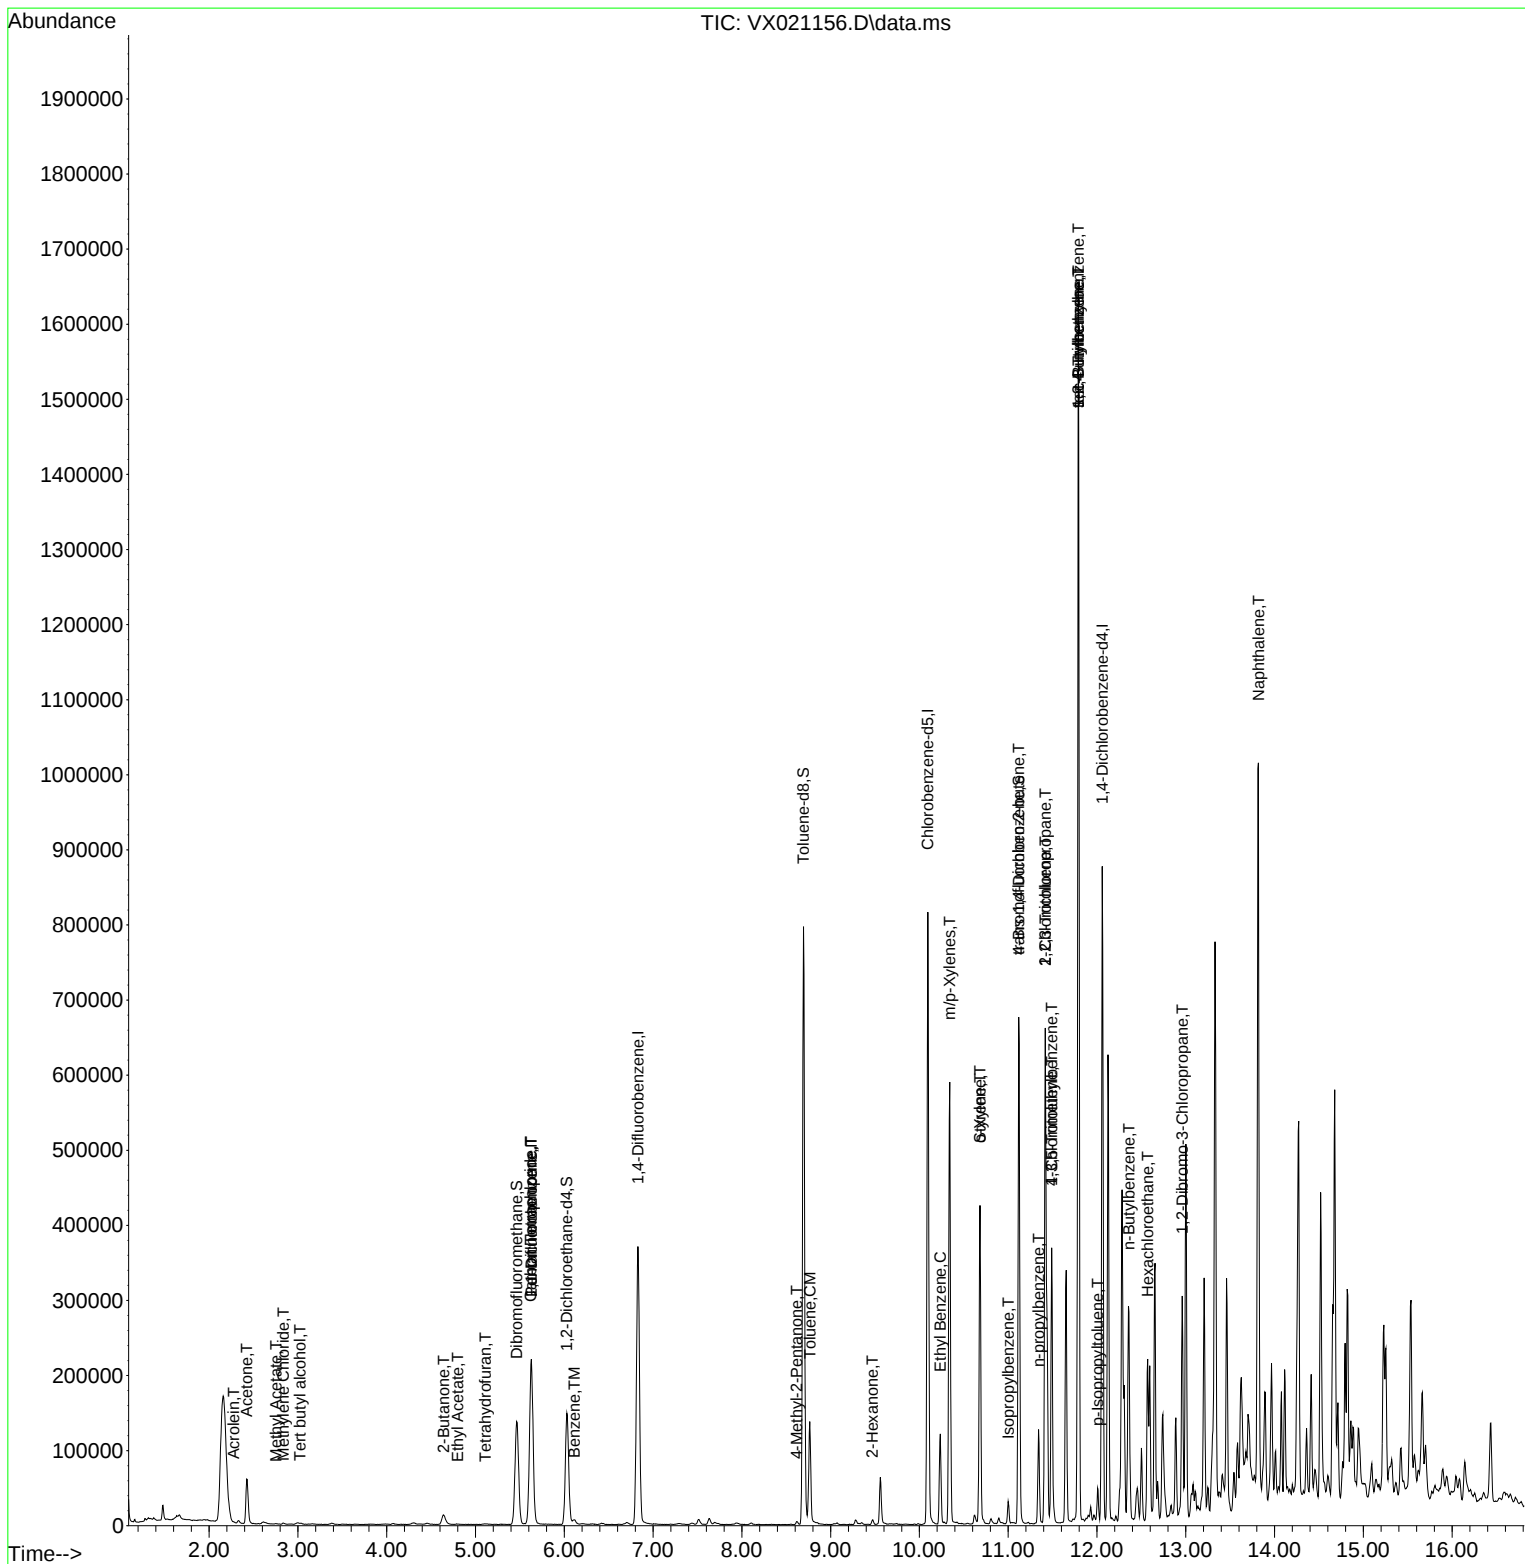




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 772
Delta R.T. 0.006 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 213666
Ion Ratio Lower Upper
168 100
99 55.8 45.8 68.6

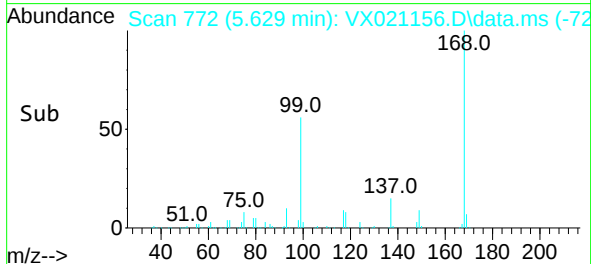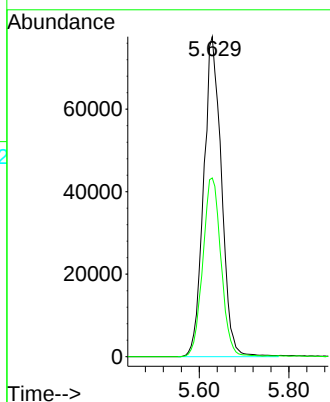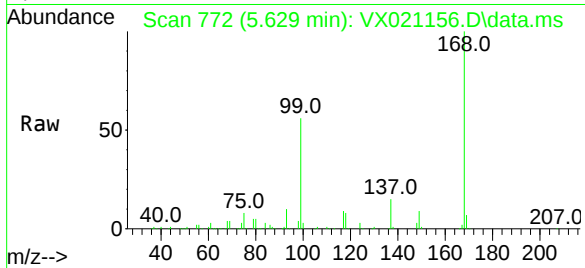

#5
Bromomethane
Concen: Below Cal
RT: 1.646 min Scan# 95
Delta R.T. 0.023 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18


Tgt Ion: 94 Resp: 560
Ion Ratio Lower Upper
94 100
96 98.4 76.4 114.6

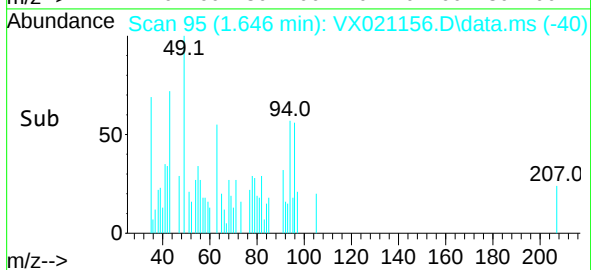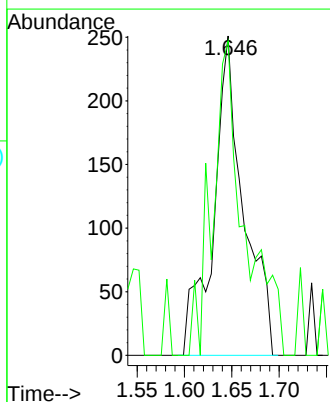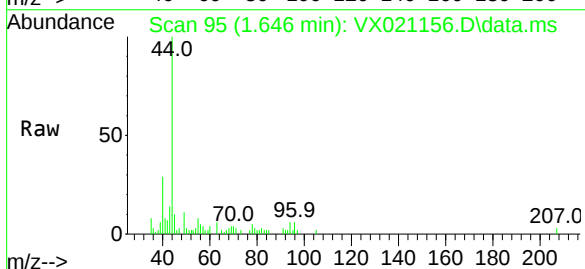






#11
Tert butyl alcohol
Concen: 4.43 ug/l
RT: 3.023 min Scan# 329
Delta R.T. 0.006 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Instrument :
MSVOA_X
ClientSampled :







Tgt Ion: 59 Resp: 2849
Ion Ratio Lower Upper
59 100
57 6.1 7.8 11.8#



#13
Acrolein
Concen: 0.62 ug/l
RT: 2.276 min Scan# 202
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Tgt Ion: 56 Resp: 245
Ion Ratio Lower Upper
56 100
55 0.0 56.4 84.6#


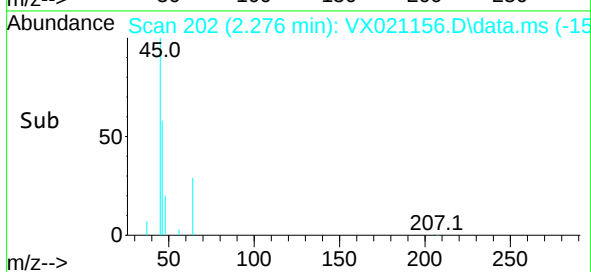

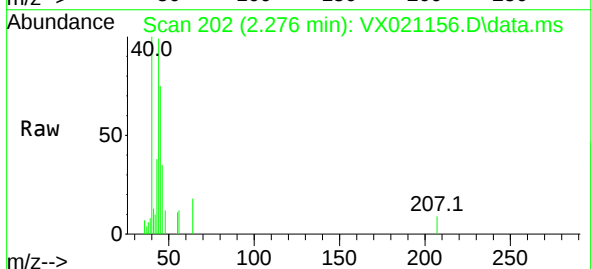




#16
Acetone
Concen: 56.86 ug/l
RT: 2.423 min Scan# 227
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 67618
Ion Ratio Lower Upper
43 100
58 33.4 27.8 41.8

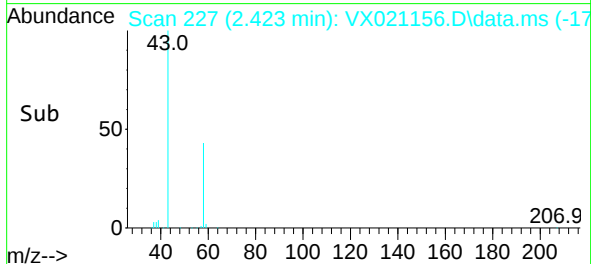

#18
Methyl Acetate
Concen: 0.27 ug/l
RT: 2.752 min Scan# 283
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18


Tgt Ion: 43 Resp: 768
Ion Ratio Lower Upper
43 100
74 28.1 21.9 32.9

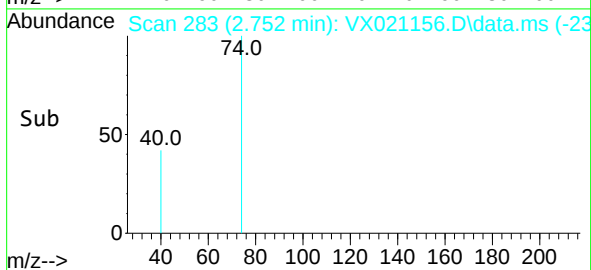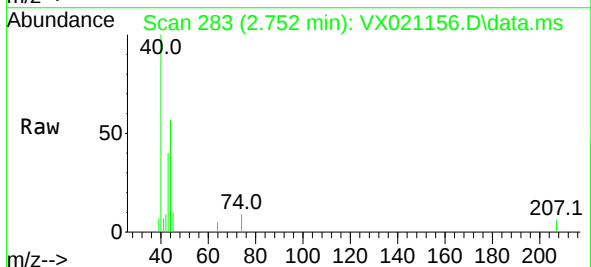



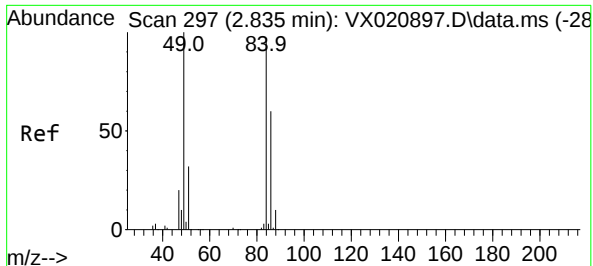


#20
Methylene Chloride
Concen: 0.22 ug/l
RT: 2.834 min Scan# 297
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Instrument :
MSVOA_X
ClientSampleId :



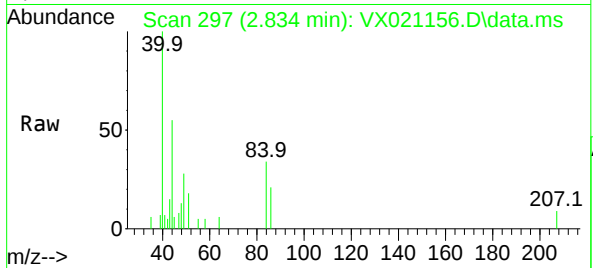



Tgt Ion:	84	Resp:	616
Ion	Ratio	Lower	Upper
84	100		
49	81.6	88.6	132.8#
51	52.3	27.0	40.6#
86	60.7	50.3	75.5

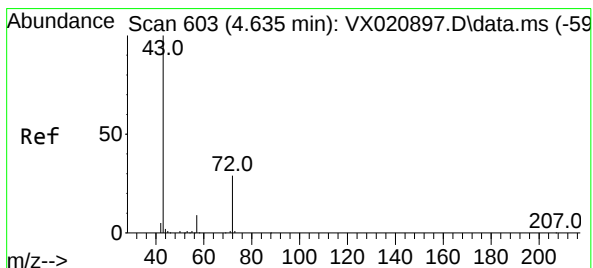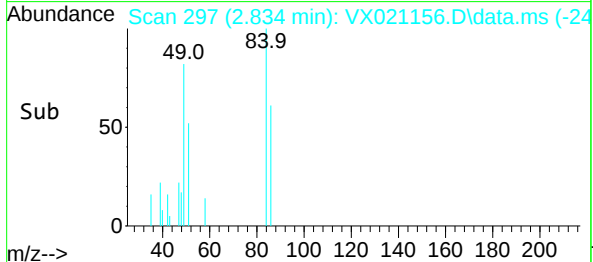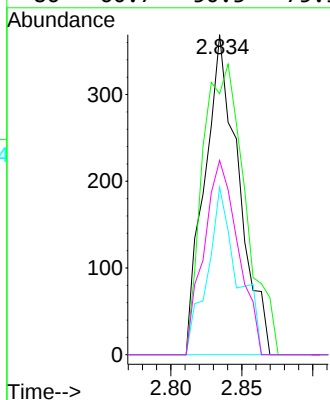

#25
2-Butanone
Concen: 11.93 ug/l
RT: 4.641 min Scan# 604
Delta R.T. 0.006 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Tgt Ion:	43	Resp:	21547
Ion	Ratio	Lower	Upper
43	100		
72	30.1	23.7	35.5

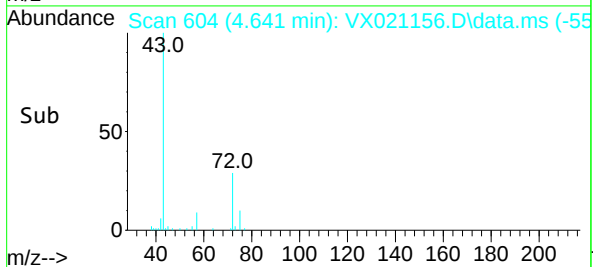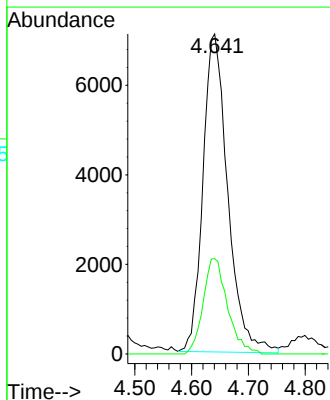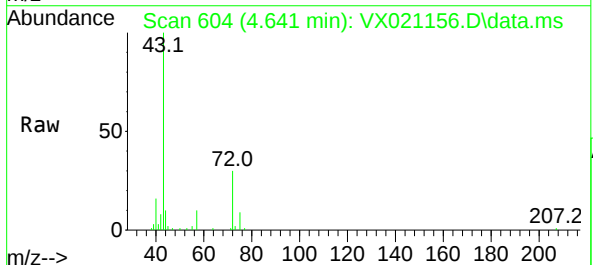



#29

Tetrahydrofuran

Concen: 0.35 ug/l

RT: 5.111 min Scan# 684

Delta R.T. 0.023 min

Lab File: VX021156.D

Acq: 11 Mar 2021 15:18

Tgt Ion: 42 Resp: 408

Ion Ratio Lower Upper

42 100





72 5.6 41.7 62.5#

71 16.2 38.4 57.6#

Instrument :

MSVOA_X

ClientSampled :

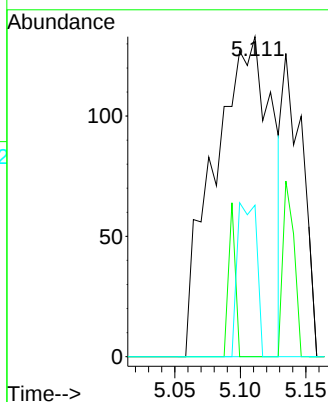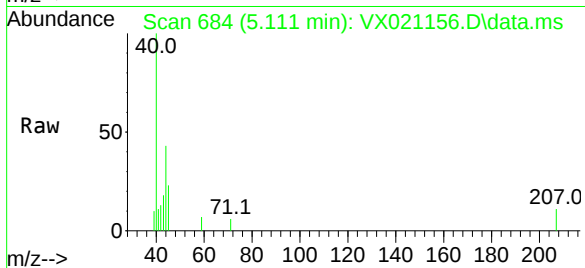

#33

1,2-Dichloroethane-d4

Concen: 48.51 ug/l

RT: 6.029 min Scan# 840

Delta R.T. -0.000 min

Lab File: VX021156.D




Acq: 11 Mar 2021 15:18


Tgt Ion: 65 Resp: 140002

Ion Ratio Lower Upper

65 100


67 52.9 0.0 105.4

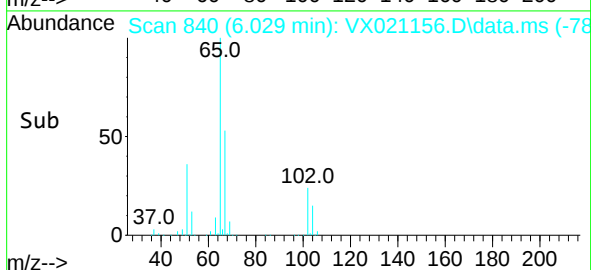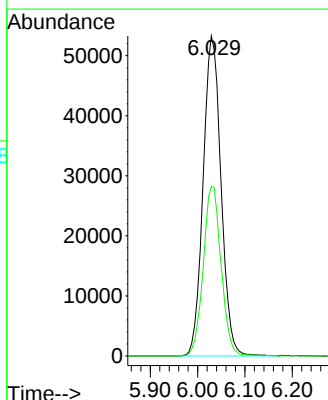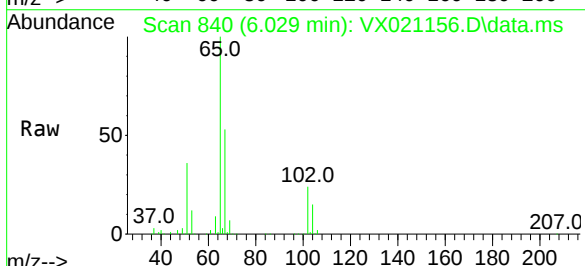






#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.829 min Scan# 976
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Instrument :
MSVOA_X
ClientSampled :







Tgt Ion:114 Resp: 395420
Ion Ratio Lower Upper
114 100
63 20.2 0.0 40.8
88 15.7 0.0 32.8

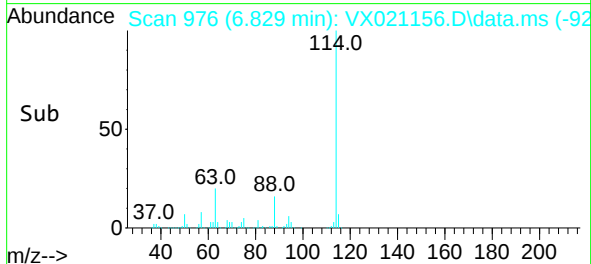

#35
Dibromofluoromethane
Concen: 51.07 ug/l
RT: 5.464 min Scan# 744
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18


Tgt Ion:113 Resp: 122692
Ion Ratio Lower Upper
113 100
111 102.2 81.9 122.9
192 19.9 16.7 25.1

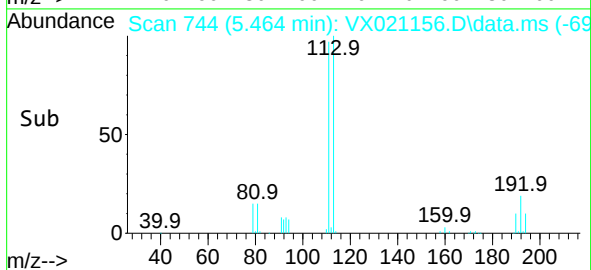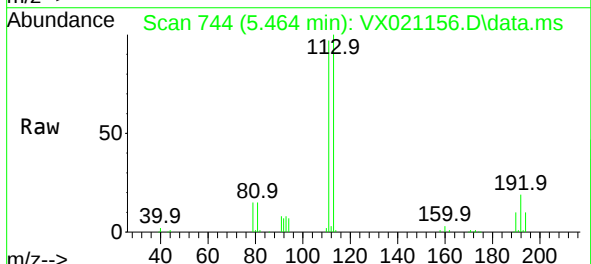






#36
1,1-Dichloropropene
Concen: 4.52 ug/l
RT: 5.629 min Scan# 772
Delta R.T. -0.141 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18


Instrument :
MSVOA_X
ClientSampled :

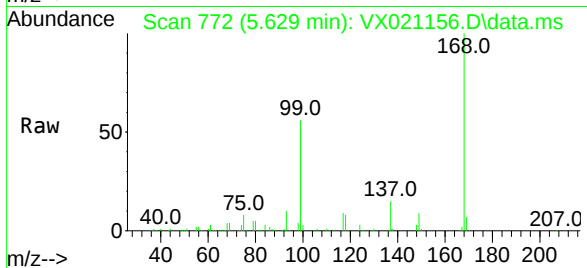



Tgt Ion: 75 Resp: 16978
Ion Ratio Lower Upper
75 100
110 7.9 18.1 54.4#
77 0.0 25.3 37.9#




#37
Ethyl Acetate
Concen: 0.43 ug/l
RT: 4.799 min Scan# 631
Delta R.T. 0.006 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

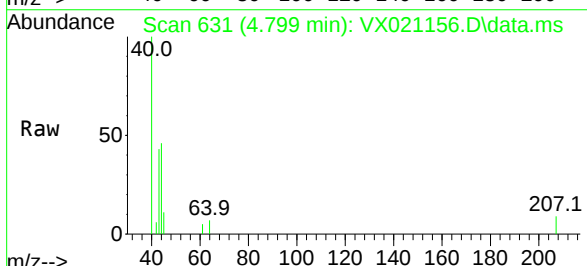


Tgt Ion: 43 Resp: 1522
Ion Ratio Lower Upper
43 100
61 14.3 12.8 19.2
70 3.0 10.5 15.7#

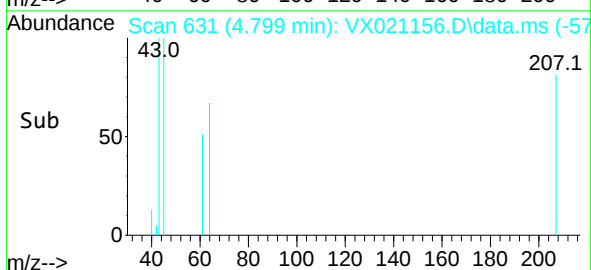






#38
Carbon Tetrachloride
Concen: 5.54 ug/l
RT: 5.623 min Scan# 771
Delta R.T. -0.130 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Instrument :
MSVOA_X
ClientSampled :



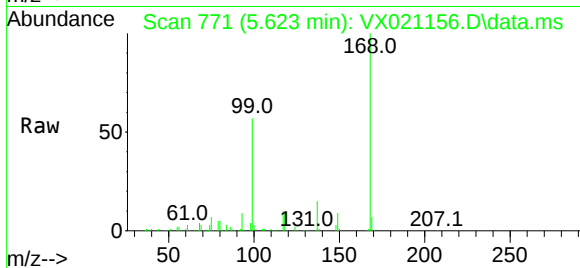



Tgt Ion: 117 Resp: 20161
Ion Ratio Lower Upper
117 100
119 4.5 76.2 114.2#
121 0.0 24.8 37.2#



#40
Benzene
Concen: 0.61 ug/l
RT: 6.111 min Scan# 854
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Tgt Ion: 78 Resp: 6924
Ion Ratio Lower Upper
78 100
77 24.0 18.9 28.3


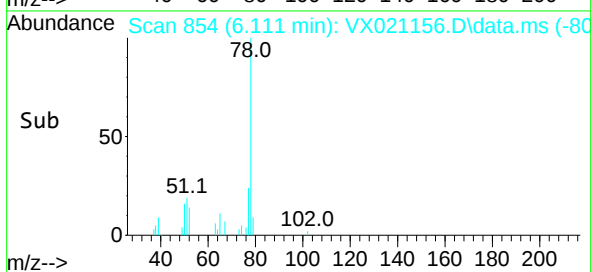

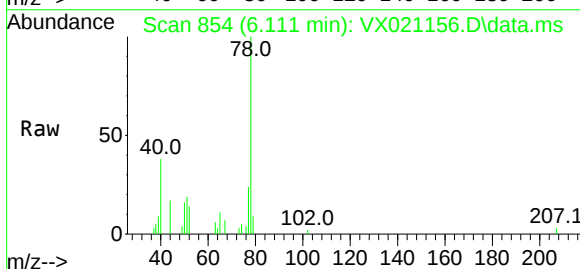




#50
Toluene-d8
Concen: 52.90 ug/l
RT: 8.694 min Scan# 1293
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 98 Resp: 495503
Ion Ratio Lower Upper
98 100
100 66.4 51.9 77.9

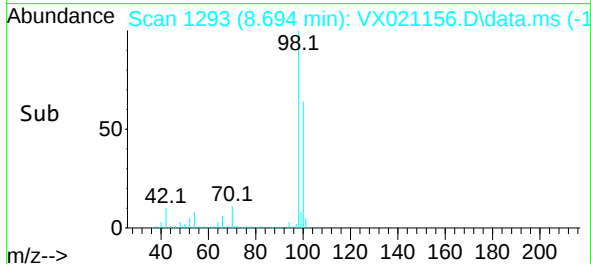

#51
4-Methyl-2-Pentanone
Concen: 0.67 ug/l
RT: 8.618 min Scan# 1280
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Tgt Ion: 43 Resp: 2369
Ion Ratio Lower Upper
43 100
58 45.8 35.4 53.0


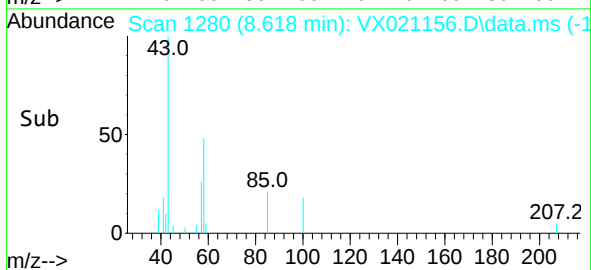

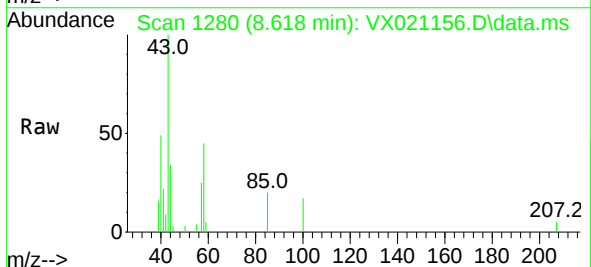


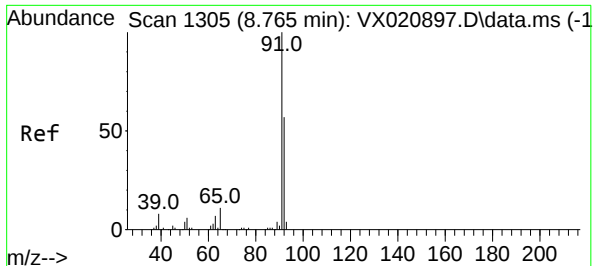

#52
Toluene
Concen: 7.35 ug/l
RT: 8.765 min Scan# 1305
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 92 Resp: 51572
Ion Ratio Lower Upper
92 100
91 168.9 137.1 205.7

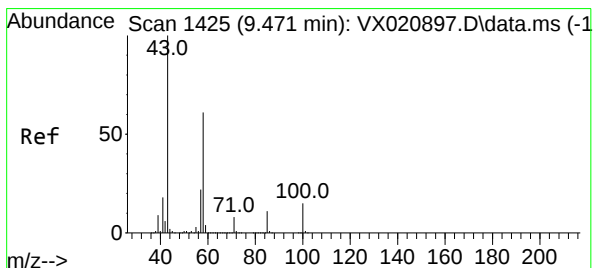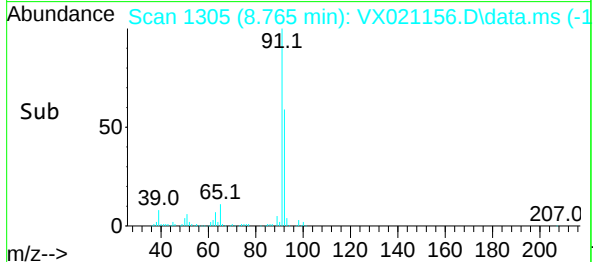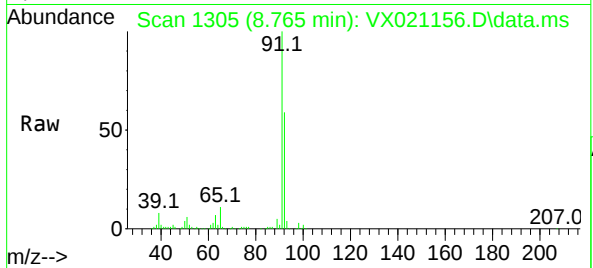

#59
2-Hexanone
Concen: 1.18 ug/l
RT: 9.471 min Scan# 1425
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Tgt Ion: 43 Resp: 3144
Ion Ratio Lower Upper
43 100
58 65.6 30.9 92.8


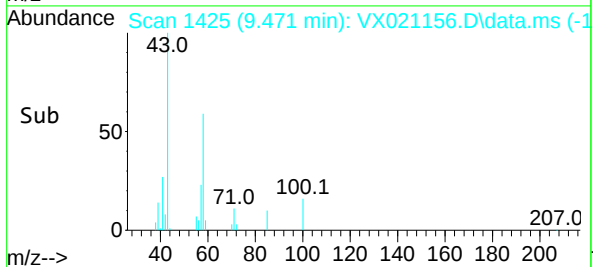

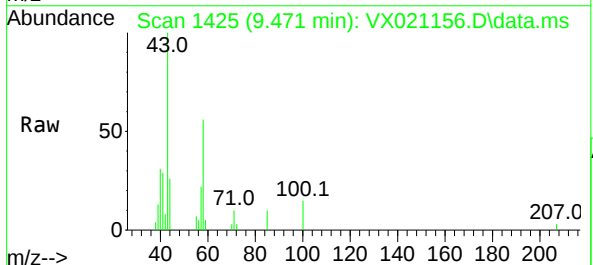


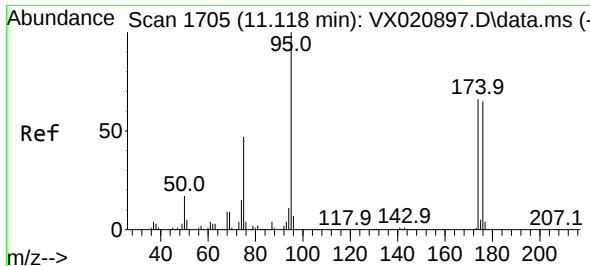

#62
4-Bromofluorobenzene
Concen: 55.44 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 192032
Ion Ratio Lower Upper
95 100
174 75.7 0.0 154.6
176 72.9 0.0 155.8

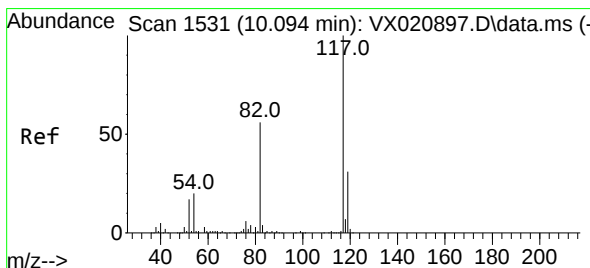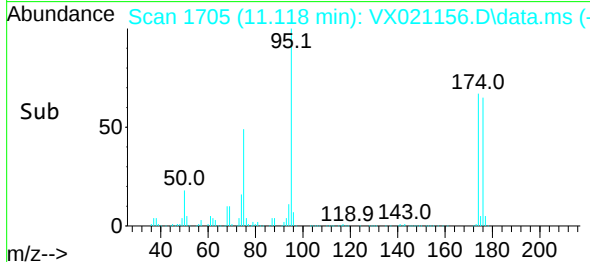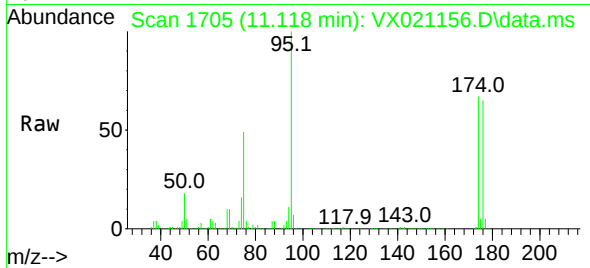

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.094 min Scan# 1531
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Tgt Ion: 117 Resp: 373910
Ion Ratio Lower Upper
117 100
82 60.3 47.4 71.2
119 33.7 26.6 39.8


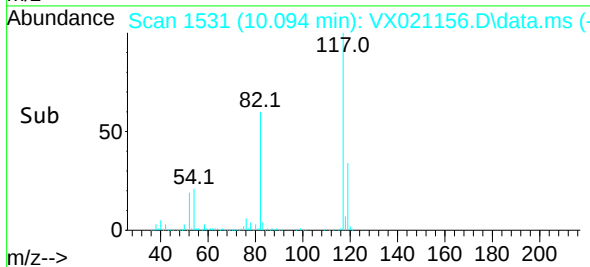

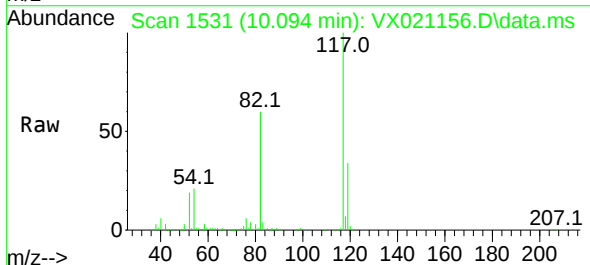


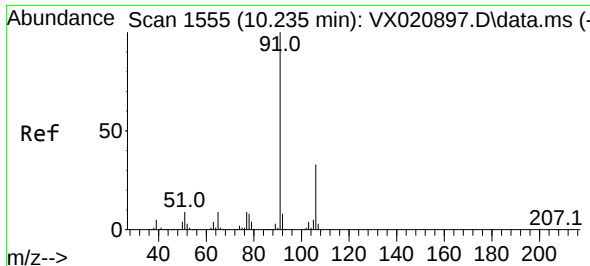

#67
Ethyl Benzene
Concen: 4.98 ug/l
RT: 10.235 min Scan# 1555
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 91 Resp: 71144
Ion Ratio Lower Upper
91 100
106 30.4 24.6 37.0

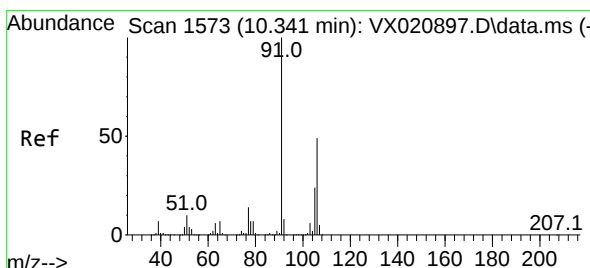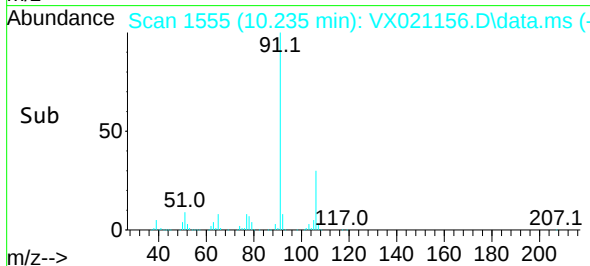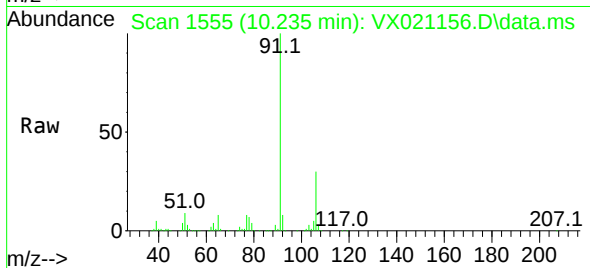

#68
m/p-Xylenes
Concen: 27.29 ug/l
RT: 10.341 min Scan# 1573
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Tgt Ion:106 Resp: 143359
Ion Ratio Lower Upper
106 100
91 197.9 162.8 244.2


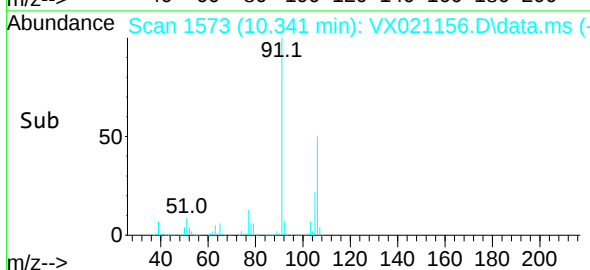

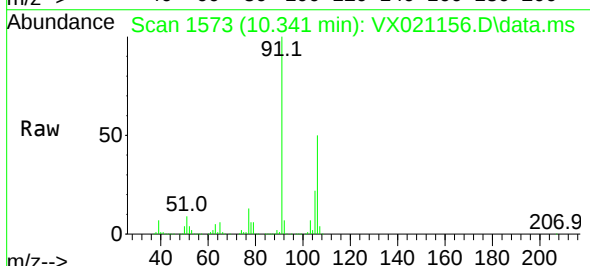




#69
o-Xylene
Concen: 17.98 ug/l
RT: 10.682 min Scan# 1631
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:106 Resp: 92184
Ion Ratio Lower Upper
106 100
91 212.6 108.1 324.2

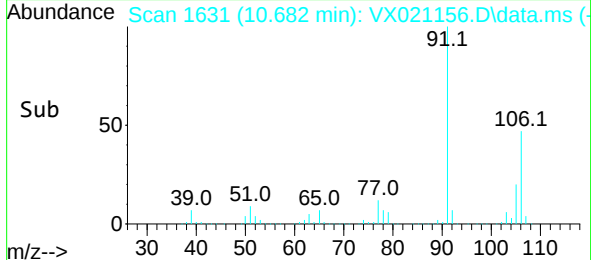

#70
Styrene
Concen: 0.88 ug/l
RT: 10.682 min Scan# 1631
Delta R.T. -0.012 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Tgt Ion:104 Resp: 7776
Ion Ratio Lower Upper
104 100
78 181.6 40.0 60.0#
103 176.7 43.4 65.0#


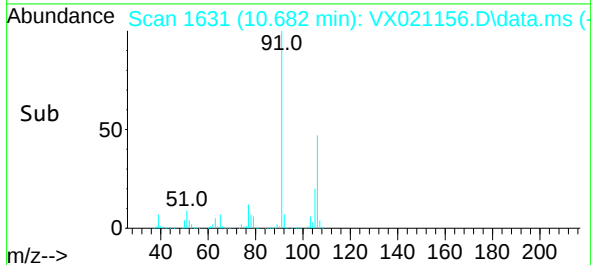

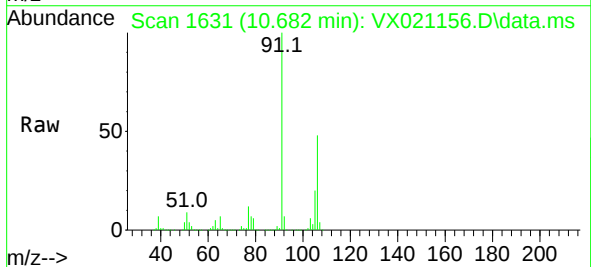




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.059 min Scan# 1865
Delta R.T. -0.006 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:152 Resp: 183339
Ion Ratio Lower Upper
152 100
115 58.5 41.1 123.3
150 153.6 0.0 349.0

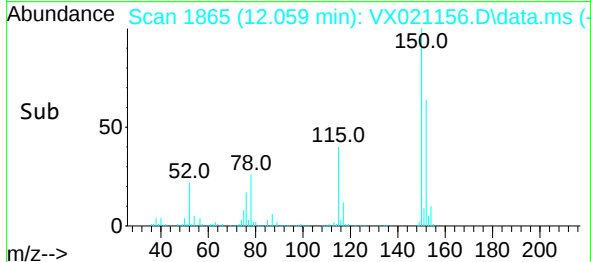

#73
Isopropylbenzene
Concen: 1.00 ug/l
RT: 11.000 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Tgt Ion:105 Resp: 14445
Ion Ratio Lower Upper
105 100
120 27.4 13.2 39.6


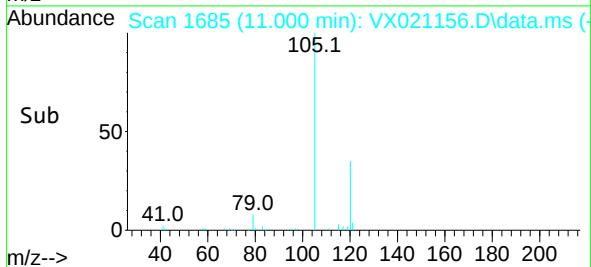

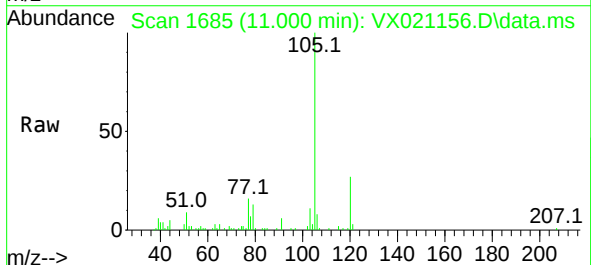


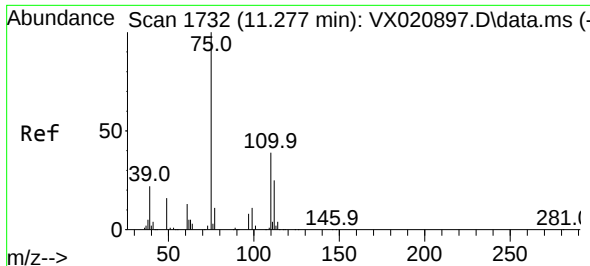

#76
1,2,3-Trichloropropane
Concen: 0.95 ug/l
RT: 11.418 min Scan# 1756
Delta R.T. 0.141 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 75 Resp: 3734
Ion Ratio Lower Upper
75 100
77 1339.8 19.1 57.5#

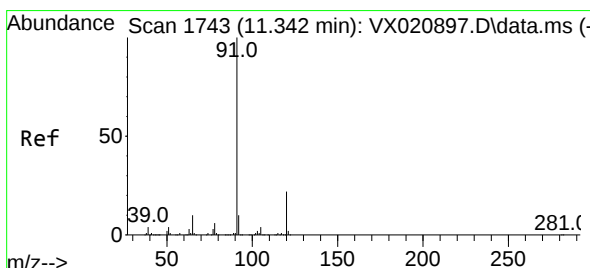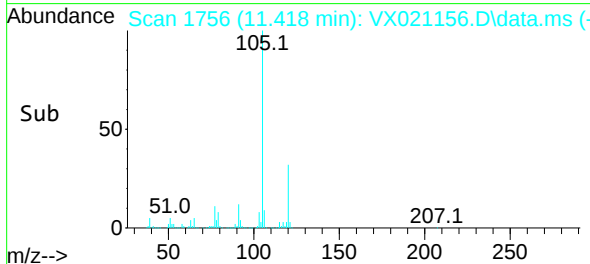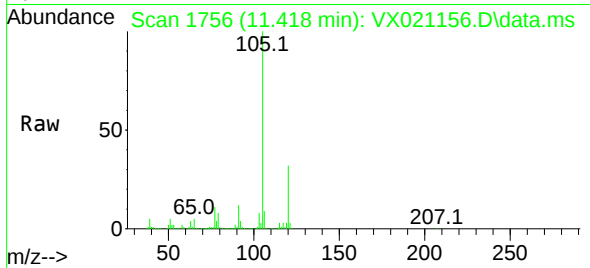

#78
n-propylbenzene
Concen: 4.68 ug/l
RT: 11.341 min Scan# 1743
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Tgt Ion: 91 Resp: 77224
Ion Ratio Lower Upper
91 100
120 22.1 11.5 34.5


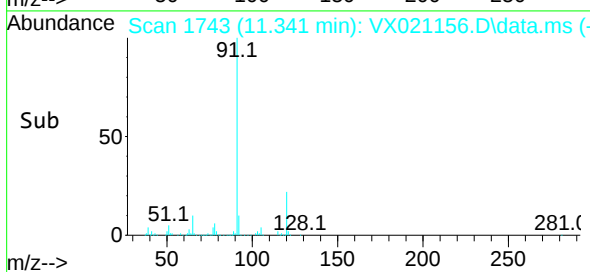

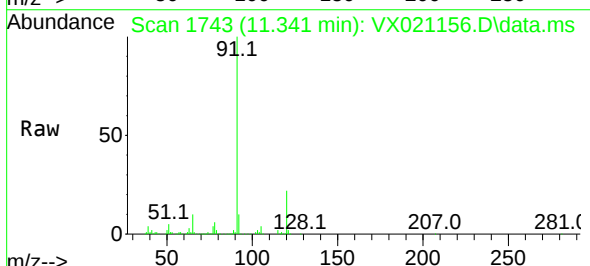




#79
2-Chlorotoluene
Concen: 5.04 ug/l
RT: 11.418 min Scan# 1756
Delta R.T. 0.018 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 91 Resp: 50456
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#

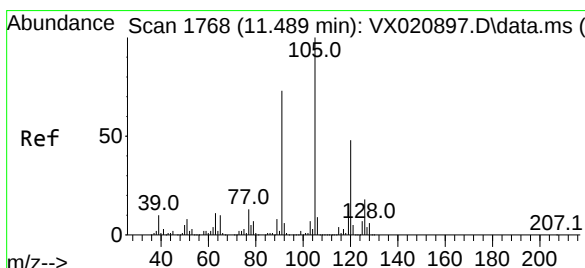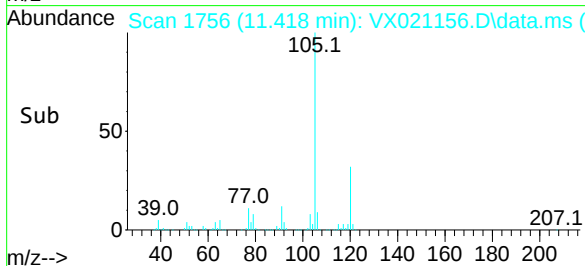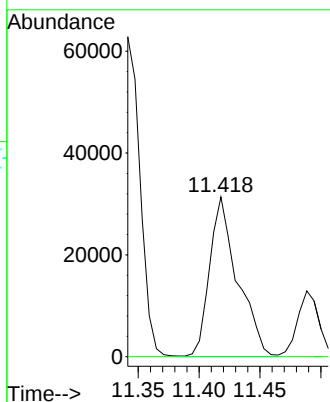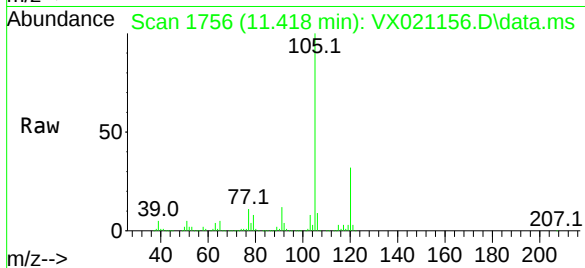

#80
1,3,5-Trimethylbenzene
Concen: 13.12 ug/l
RT: 11.488 min Scan# 1768
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Tgt Ion: 105 Resp: 158083
Ion Ratio Lower Upper
105 100
120 49.0 23.8 71.5


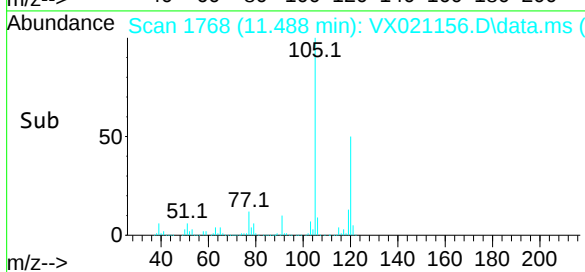
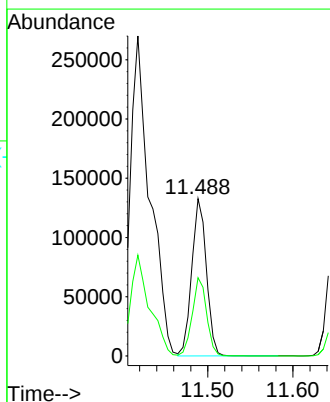
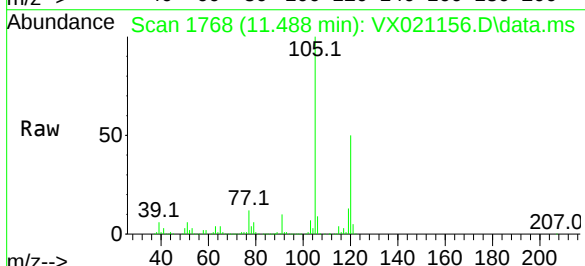




#81
trans-1,4-Dichloro-2-butene
Concen: 51.49 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. 0.059 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 91721
Ion Ratio Lower Upper
75 100
53 0.1 74.5 111.7#
89 0.0 37.9 56.9#

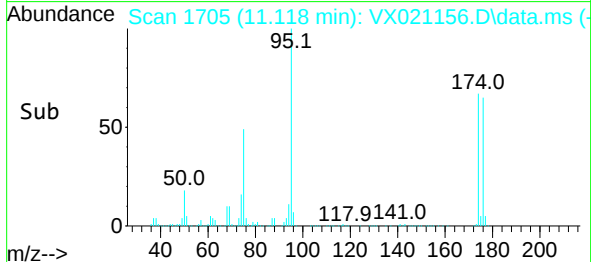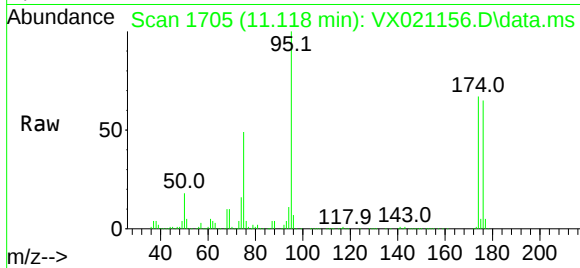

#82
4-Chlorotoluene
Concen: 1.37 ug/l
RT: 11.488 min Scan# 1768
Delta R.T. -0.006 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Tgt Ion: 91 Resp: 15796
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#


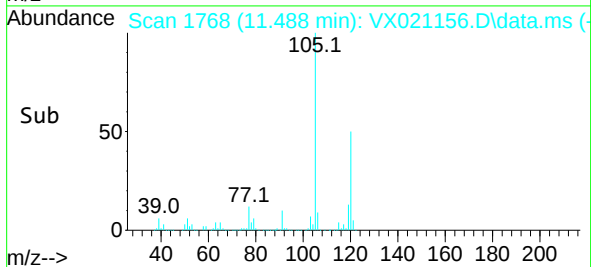

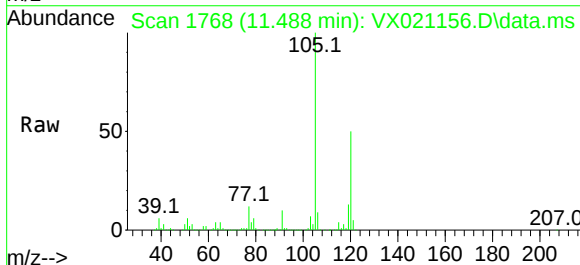




#83
 tert-Butylbenzene
 Concen: 7.29 ug/l
 RT: 11.789 min Scan# 1819
 Delta R.T. 0.035 min
 Lab File: VX021156.D
 Acq: 11 Mar 2021 15:18




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion:119 Resp: 85412
 Ion Ratio Lower Upper
 119 100
 91 78.8 27.9 83.7
 134 0.0 11.3 33.9#

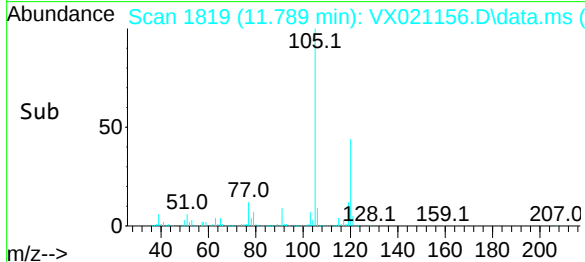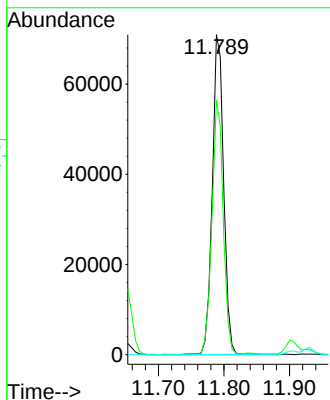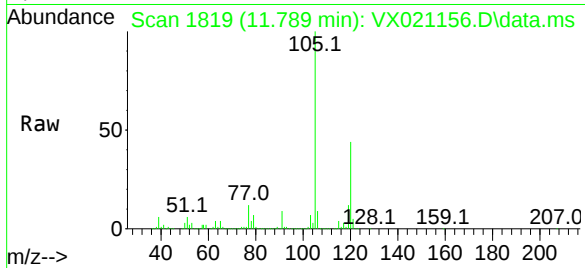

#84
 1,2,4-Trimethylbenzene
 Concen: 57.28 ug/l
 RT: 11.789 min Scan# 1819
 Delta R.T. -0.000 min
 Lab File: VX021156.D
 Acq: 11 Mar 2021 15:18

Tgt Ion:105 Resp: 700642
 Ion Ratio Lower Upper
 105 100
 120 46.0 22.4 67.3


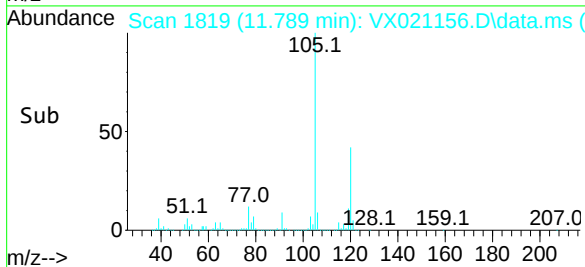
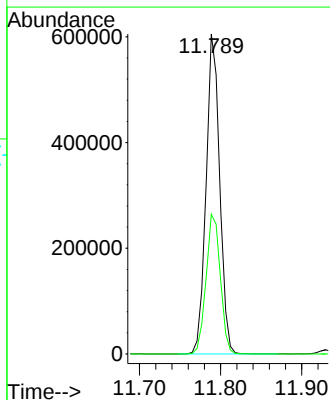
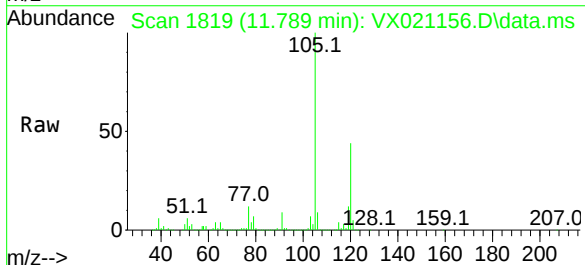


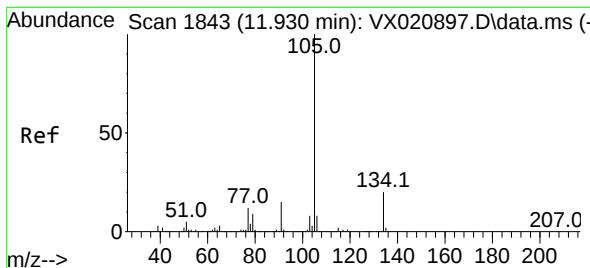

#85
 sec-Butylbenzene
 Concen: 50.72 ug/l
 RT: 11.789 min Scan# 1819
 Delta R.T. -0.141 min
 Lab File: VX021156.D
 Acq: 11 Mar 2021 15:18




Instrument :
 MSVOA_X
 ClientSampled :


Tgt Ion:105 Resp: 700642
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.0 29.8#

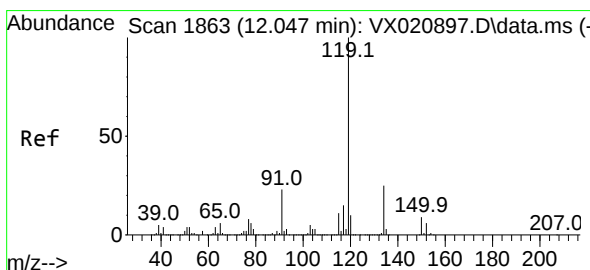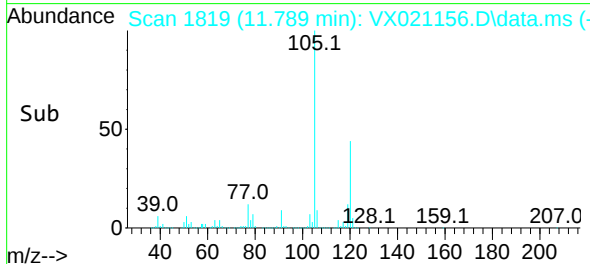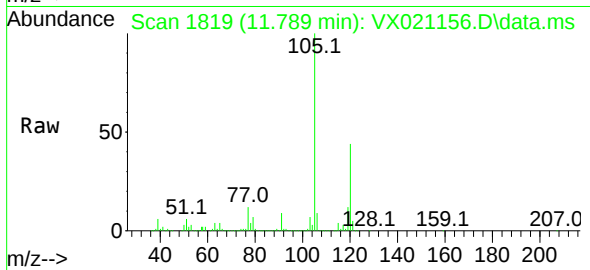

#86
 p-Isopropyltoluene
 Concen: 1.48 ug/l
 RT: 12.006 min Scan# 1856
 Delta R.T. -0.041 min
 Lab File: VX021156.D
 Acq: 11 Mar 2021 15:18

Tgt Ion:119 Resp: 18763
 Ion Ratio Lower Upper
 119 100
 134 28.1 12.9 38.7
 91 22.9 11.7 35.0


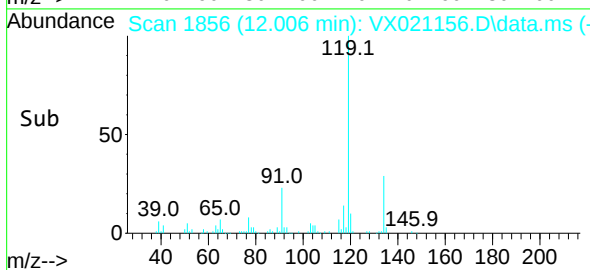

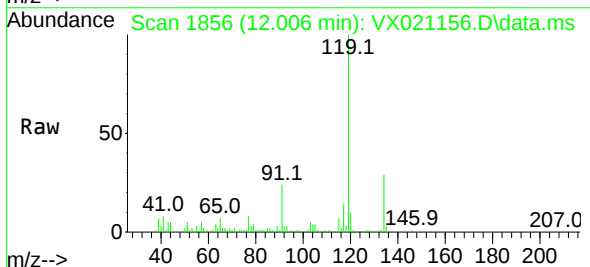




#89
n-Butylbenzene
Concen: 3.35 ug/l
RT: 12.359 min Scan# 1916
Delta R.T. -0.012 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 91 Resp: 37836
Ion Ratio Lower Upper
91 100
92 30.4 27.4 82.0
134 122.2 13.2 39.5#

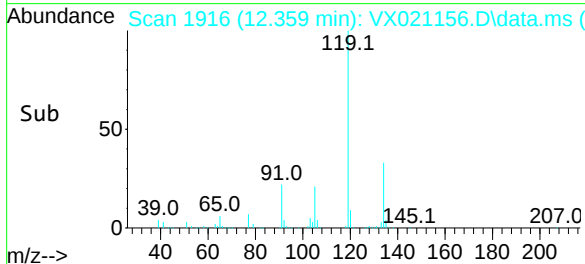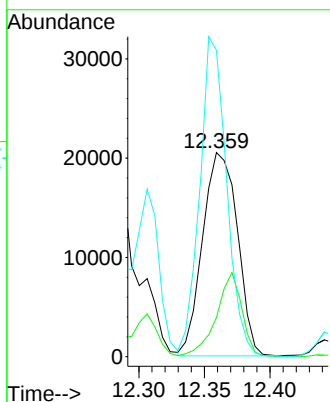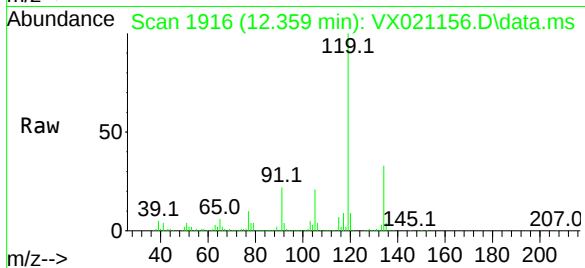

#90
Hexachloroethane
Concen: 3.88 ug/l
RT: 12.571 min Scan# 1952
Delta R.T. -0.006 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Tgt Ion: 117 Resp: 9371
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#


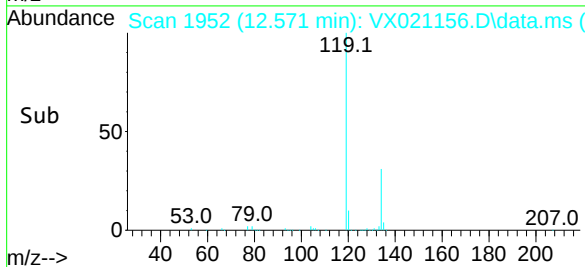
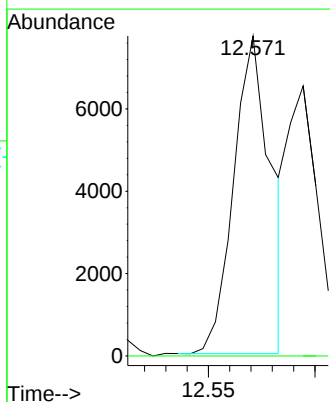
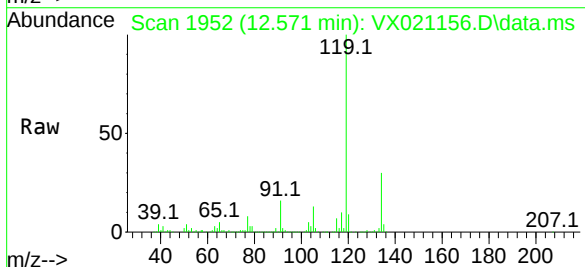




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.87 ug/l
RT: 12.959 min Scan# 2018
Delta R.T. -0.024 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 75 Resp: 935
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#

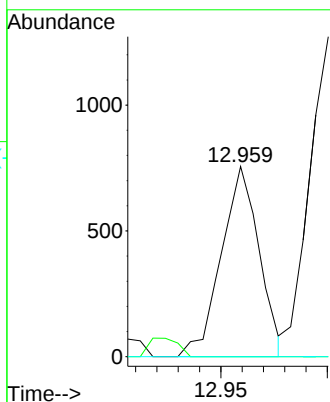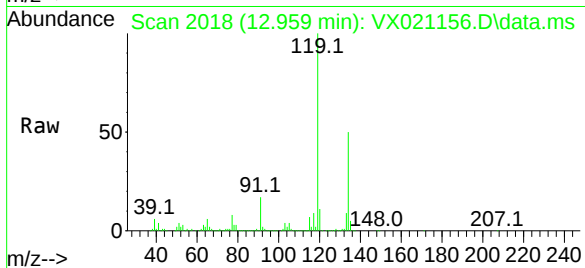

#95
Naphthalene
Concen: 46.71 ug/l
RT: 13.818 min Scan# 2164
Delta R.T. -0.000 min
Lab File: VX021156.D
Acq: 11 Mar 2021 15:18

Tgt Ion:128 Resp: 628043
Ion Ratio Lower Upper
128 100
127 12.8 10.3 15.5
129 11.3 8.8 13.2

