

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031121\
 Data File : VX021164.D
 Acq On : 11 Mar 2021 18:22
 Operator : JC/MD
 Sample : M1647-21 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP5-30811:15

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M

Title : SW846 8260

Signal : TIC: VX021164.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.476	62	66	77	rBV	377261	425059	36.35%	6.260%
2	2.993	315	324	332	rBV	5705	13393	1.15%	0.197%
3	5.464	732	744	759	rBV	127804	366193	31.31%	5.393%
4	5.629	760	772	787	rVB2	199531	564586	48.28%	8.315%
5	6.029	829	840	849	rBV	137973	361904	30.95%	5.330%
6	6.111	849	854	867	rVB2	10673	30002	2.57%	0.442%
7	6.829	966	976	991	rBV	339703	804321	68.78%	11.845%
8	8.694	1286	1293	1301	rBV	748390	1169389	100.00%	17.222%
9	8.765	1301	1305	1318	rVB	27791	46752	4.00%	0.689%
10	10.094	1525	1531	1545	rBV	775811	1050411	89.83%	15.470%
11	10.341	1568	1573	1578	rBV	19319	27163	2.32%	0.400%
12	10.683	1626	1631	1638	rBV2	19938	29521	2.52%	0.435%
13	11.118	1699	1705	1719	rBV	639959	822686	70.35%	12.116%
14	12.059	1857	1865	1873	rBV	824419	1004479	85.90%	14.793%
15	12.453	1927	1932	1938	rVB	11017	14085	1.20%	0.207%
16	13.818	2159	2164	2170	rBV	48936	60186	5.15%	0.886%




Sum of corrected areas: 6790130

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031121\
Data File : VX021164.D
Acq On : 11 Mar 2021 18:22
Operator : JC/MD
Sample : M1647-21 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP5-30811:15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

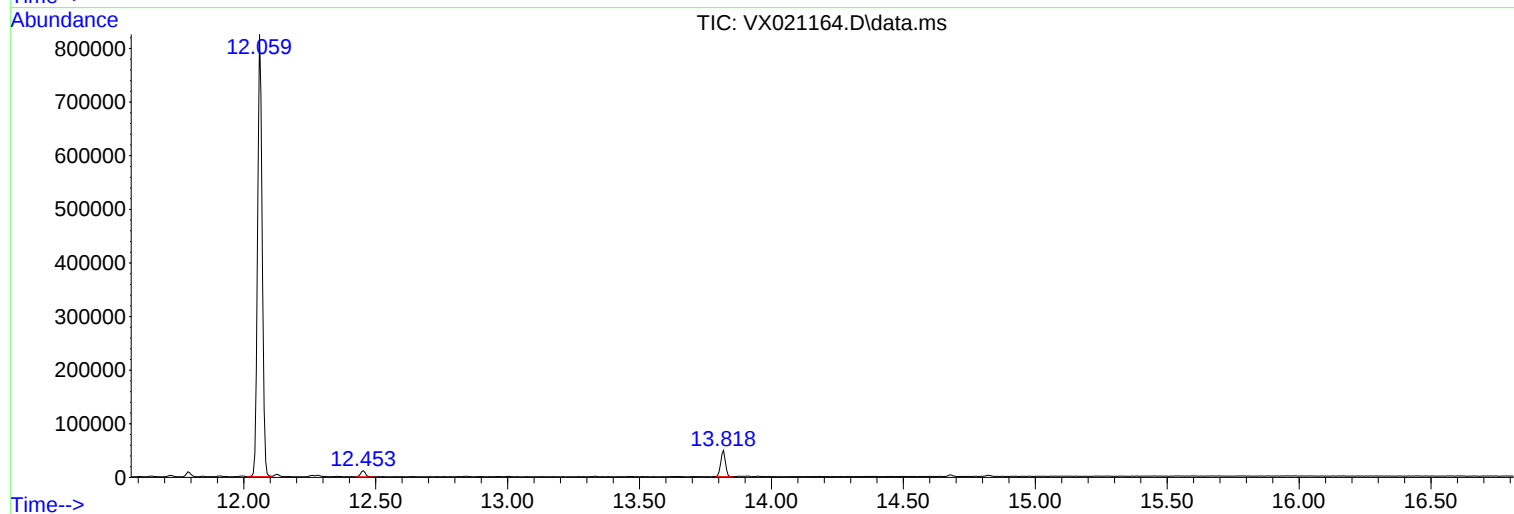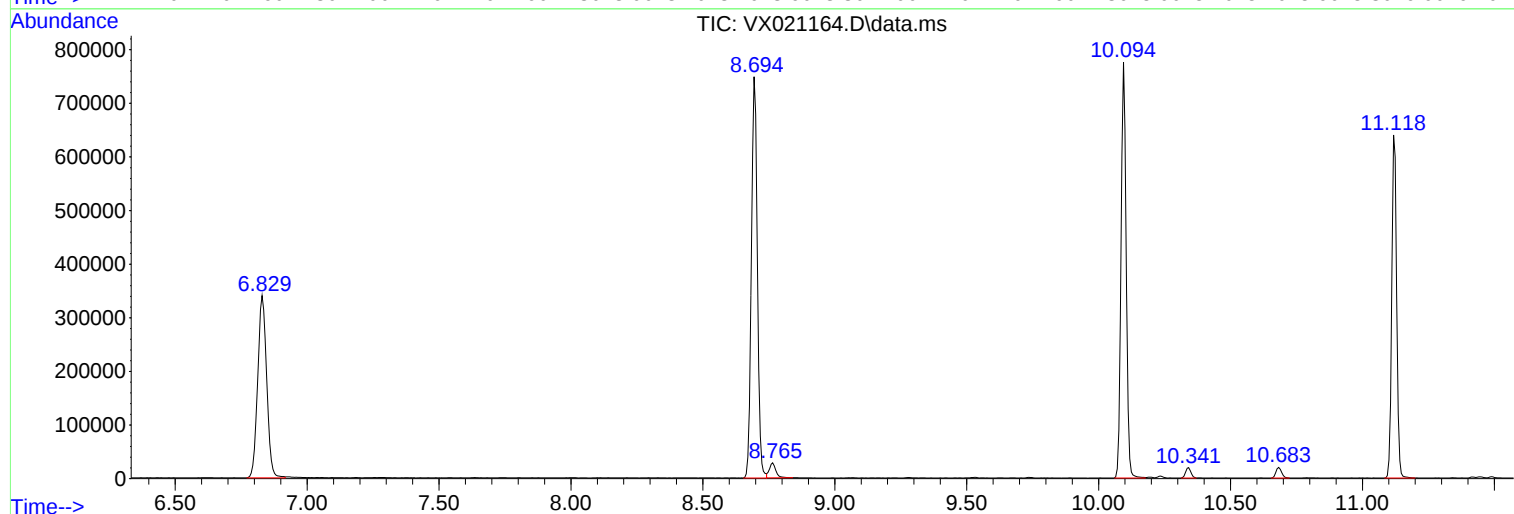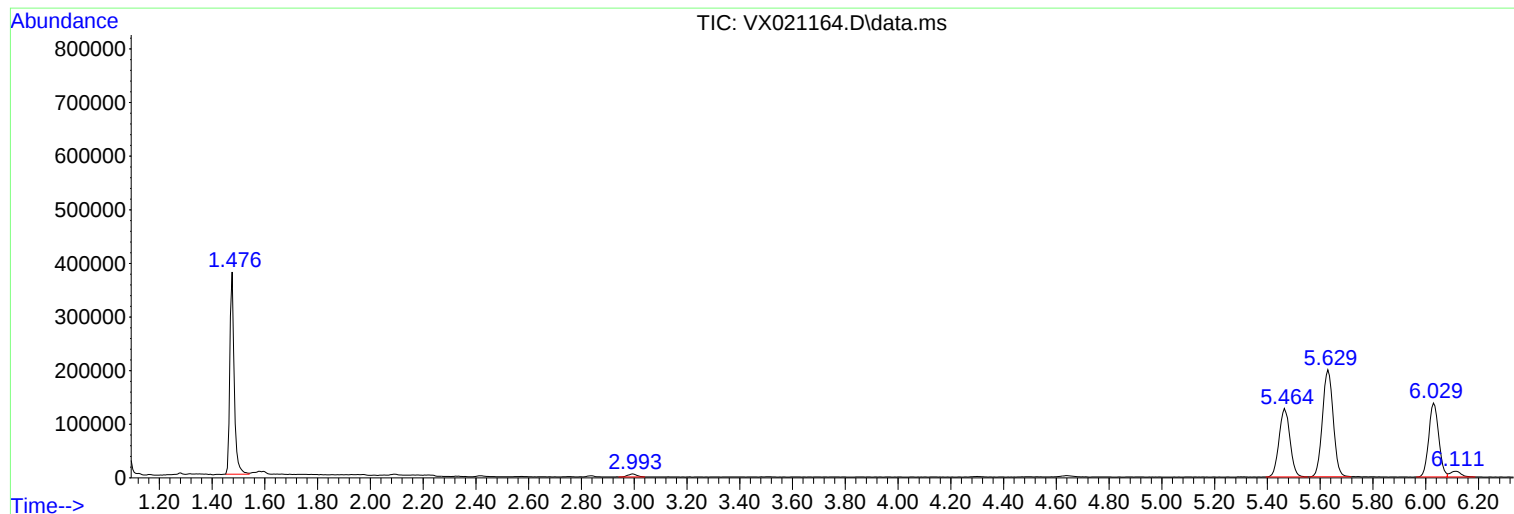

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031121\
Data File : VX021164.D
Acq On : 11 Mar 2021 18:22
Operator : JC/MD
Sample : M1647-21 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP5-30811:15










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Acetaldehyde Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.476	37.64 ug/l	425059	Pentafluorobenzene	5.629

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Acetaldehyde	44	C2H4O	000075-07-0	74
2			Propane	44	C3H8	000074-98-6	5
3			Ethylene oxide	44	C2H4O	000075-21-8	5
4			Alanine	89	C3H7NO2	000056-41-7	4
5			1,2-Propanediamine	74	C3H10N2	000078-90-0	4

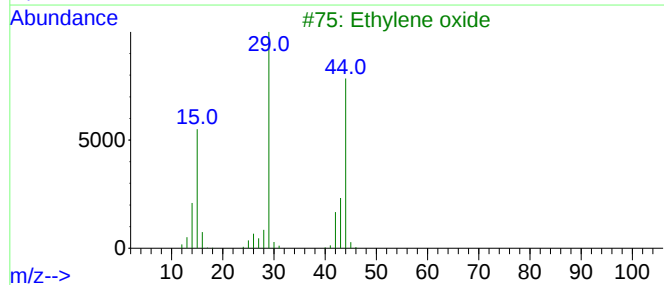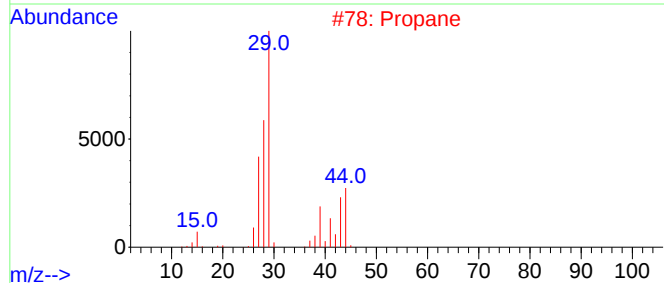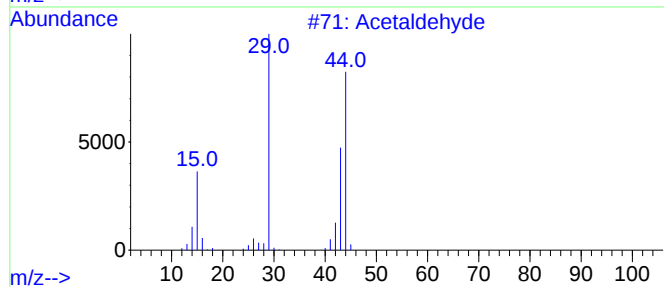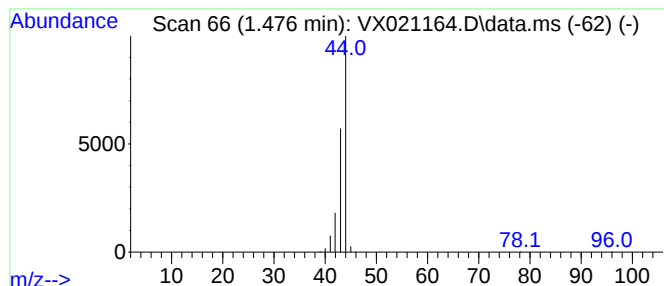

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031121\
Data File : VX021164.D
Acq On : 11 Mar 2021 18:22
Operator : JC/MD
Sample : M1647-21 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP5-30811:15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Acetaldehyde	1.476	37.6	ug/l	425059	1	5.629	564586	50.0