

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031121\
 Data File : VX021166.D
 Acq On : 11 Mar 2021 19:08
 Operator : JC/MD
 Sample : M1648-07 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP1-41727:28

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M

Title : SW846 8260

Signal : TIC: VX021166.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	78	87	90	rVB4	5539	13726	1.16%	0.216%
2	2.993	315	324	333	rVB	5101	11981	1.02%	0.189%
3	5.464	731	744	759	rBV	131640	374002	31.70%	5.895%
4	5.629	759	772	786	rBV2	207405	578742	49.05%	9.122%
5	6.029	828	840	856	rBV	139949	367832	31.18%	5.798%
6	6.829	965	976	991	rBV	347834	823579	69.80%	12.981%
7	8.694	1286	1293	1300	rBV	775569	1179865	100.00%	18.597%
8	8.765	1300	1305	1317	rVB	51783	86811	7.36%	1.368%
9	10.094	1525	1531	1548	rBV	804326	1064196	90.20%	16.774%
10	11.118	1699	1705	1718	rBV	636615	829250	70.28%	13.070%
11	12.059	1859	1865	1874	rBV	816353	1014468	85.98%	15.990%




Sum of corrected areas: 6344452

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031121\
Data File : VX021166.D
Acq On : 11 Mar 2021 19:08
Operator : JC/MD
Sample : M1648-07 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

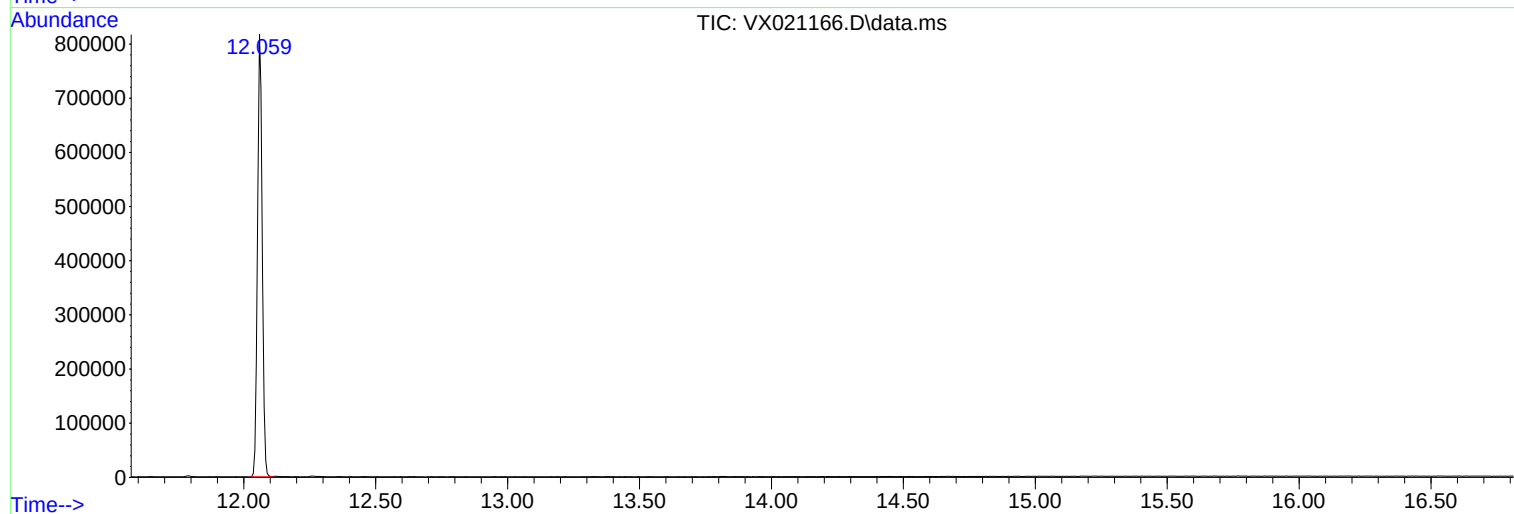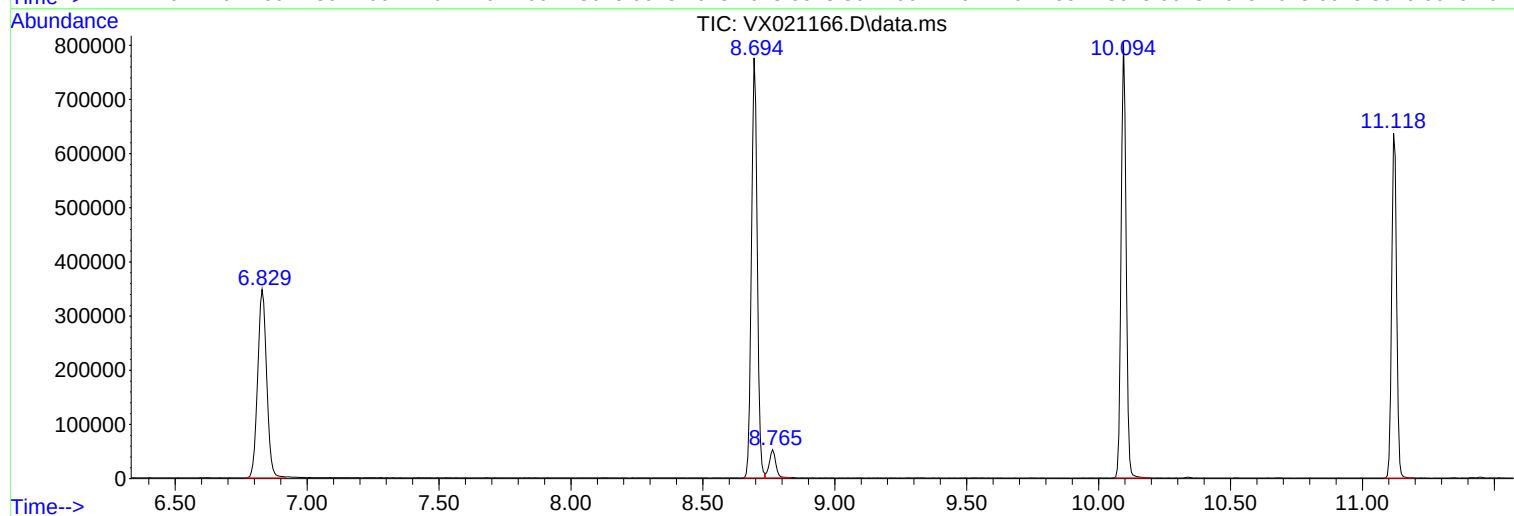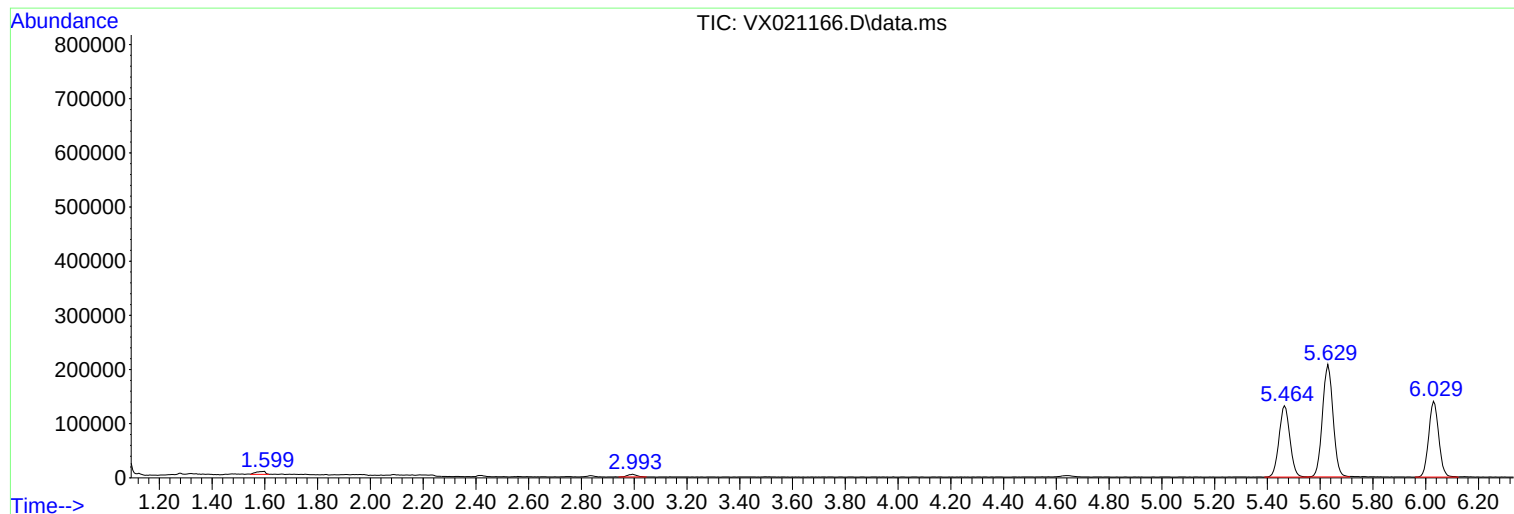

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031121\
Data File : VX021166.D
Acq On : 11 Mar 2021 19:08
Operator : JC/MD
Sample : M1648-07 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031121\
Data File : VX021166.D
Acq On : 11 Mar 2021 19:08
Operator : JC/MD
Sample : M1648-07 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP1-41727:28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
