

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031121\
 Data File : VX021167.D
 Acq On : 11 Mar 2021 19:32
 Operator : JC/MD
 Sample : M1648-09 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP2-30802:05

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
 Title : SW846 8260

Signal : TIC: VX021167.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.464	732	744	756	rBV2	136599	382186	31.40%	5.280%
2	5.629	759	772	790	rBV2	211731	597641	49.10%	8.256%
3	6.029	829	840	853	rBV	143885	378389	31.09%	5.227%
4	6.829	966	976	995	rBV	362353	852732	70.06%	11.780%
5	8.694	1286	1293	1301	rBV	789928	1217175	100.00%	16.815%
6	8.764	1301	1305	1320	rVB	12116	23500	1.93%	0.325%
7	10.094	1525	1531	1550	rBV	799009	1098902	90.28%	15.181%
8	10.341	1567	1573	1579	rBV	18212	25271	2.08%	0.349%
9	10.682	1626	1631	1641	rVB	27653	35667	2.93%	0.493%
10	11.117	1700	1705	1720	rVB	667615	864799	71.05%	11.947%
11	11.341	1739	1743	1749	rVB	30552	38296	3.15%	0.529%
12	11.418	1749	1756	1764	rVV	130546	224553	18.45%	3.102%
13	11.488	1764	1768	1779	rVB	59665	73036	6.00%	1.009%
14	11.653	1790	1796	1801	rBV	59394	74950	6.16%	1.035%
15	11.788	1814	1819	1827	rVB	193689	237726	19.53%	3.284%
16	12.059	1860	1865	1872	rBV	855821	1066367	87.61%	14.732%
17	12.124	1872	1876	1884	rVB	26860	34114	2.80%	0.471%
18	12.282	1897	1903	1911	rBV2	8884	13230	1.09%	0.183%




Sum of corrected areas: 7238534

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031121\
Data File : VX021167.D
Acq On : 11 Mar 2021 19:32
Operator : JC/MD
Sample : M1648-09 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP2-30802:05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

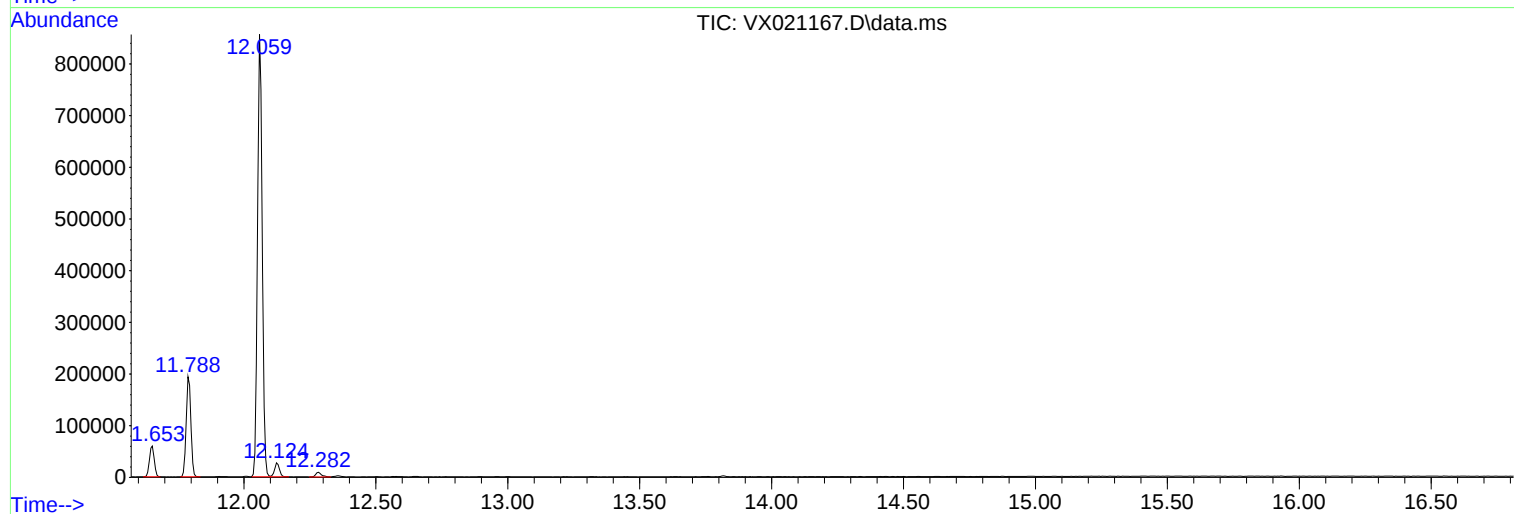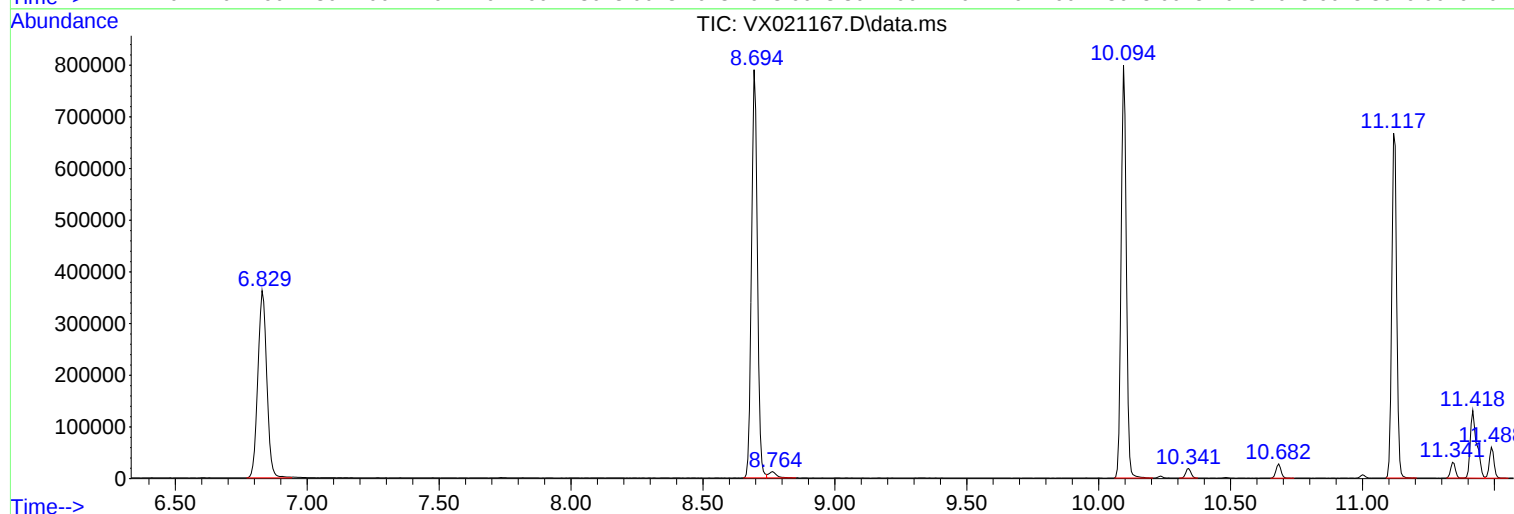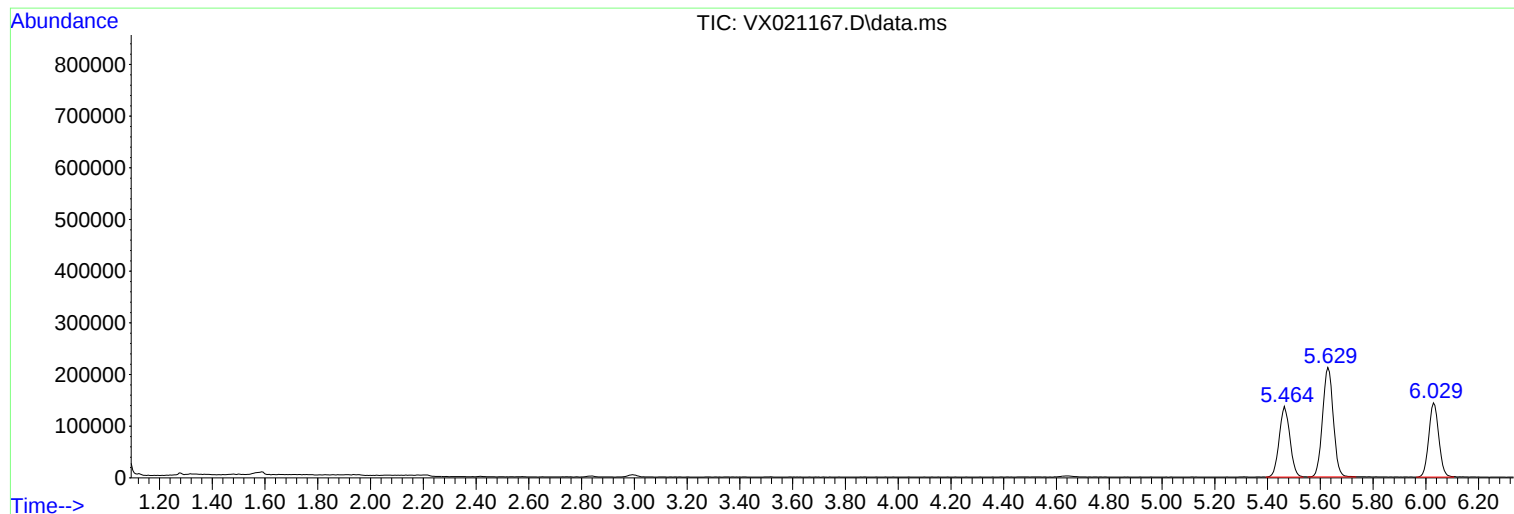

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031121\
Data File : VX021167.D
Acq On : 11 Mar 2021 19:32
Operator : JC/MD
Sample : M1648-09 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP2-30802:05










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, 1-ethyl-3-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.418	10.53 ug/l	224553	1,4-Dichlorobenzene-d4	12.059

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1-ethyl-3-methyl-	120	C9H12	000620-14-4	95
2			Benzene, 1-ethyl-2-methyl-	120	C9H12	000611-14-3	95
3			Mesitylene	120	C9H12	000108-67-8	91
4			Benzene, 1-ethyl-4-methyl-	120	C9H12	000622-96-8	91
5			Benzene, 1,2,3-trimethyl-	120	C9H12	000526-73-8	91

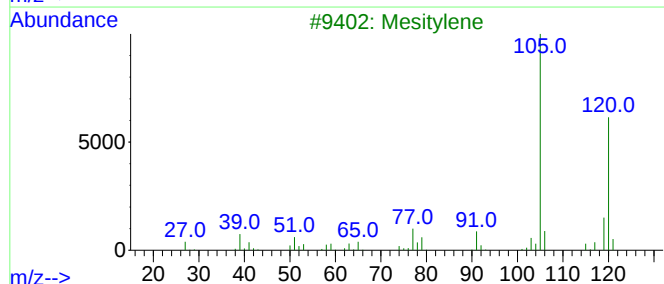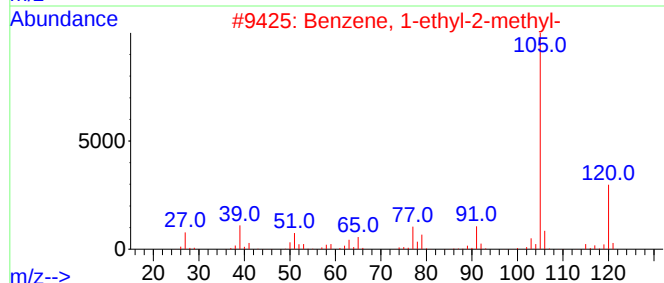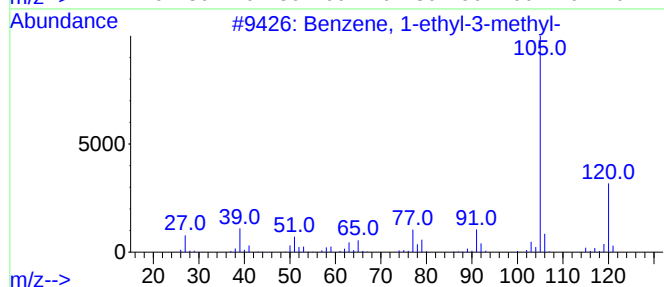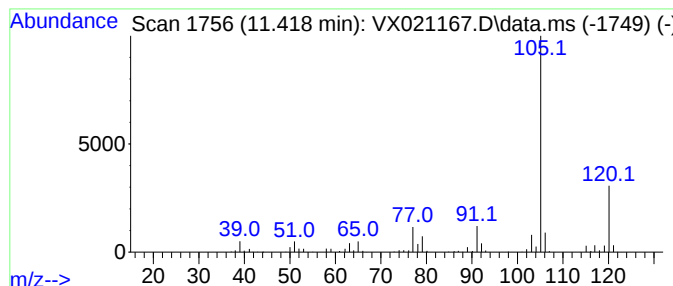

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031121\
Data File : VX021167.D
Acq On : 11 Mar 2021 19:32
Operator : JC/MD
Sample : M1648-09 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP2-30802:05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1-ethy...	11.418	10.5	ug/l	224553	4	12.059	1066370	50.0