

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031122\
 Data File : VX027401.D
 Acq On : 11 Mar 2022 14:55
 Operator : JC/MD
 Sample : N1870-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PT-VOA-WP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
 Title : SW846 8260

Signal : TIC: VX027401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	31	rBV	103283	165273	3.82%	0.267%
2	1.294	31	34	42	rVB	385694	359123	8.31%	0.580%
3	1.886	126	131	142	rVB	607420	862872	19.96%	1.393%
4	2.380	207	212	221	rVB	78817	132047	3.05%	0.213%
5	2.788	271	279	300	rBV	742649	1347667	31.17%	2.176%
6	3.105	318	331	349	rBV2	1318790	4034574	93.31%	6.514%
7	3.611	404	414	430	rBV	706199	1654264	38.26%	2.671%
8	4.495	543	559	565	rBV	791314	2152241	49.77%	3.475%
9	4.562	565	570	589	rVB	243747	669825	15.49%	1.081%
10	5.099	647	658	676	rVB	232465	698490	16.15%	1.128%
11	5.391	690	706	721	rBV	655087	2001054	46.28%	3.231%
12	5.556	721	733	749	rVB	351654	1000345	23.13%	1.615%
13	5.958	787	799	806	rBV	204586	537183	12.42%	0.867%
14	6.044	806	813	815	rVV	233044	517035	11.96%	0.835%
15	6.092	815	821	842	rVB	542559	1464242	33.86%	2.364%
16	6.763	920	931	948	rBV	504246	1210776	28.00%	1.955%
17	7.129	980	991	1009	rBV	880531	1885019	43.59%	3.044%
18	7.434	1028	1041	1051	rBV	236390	489488	11.32%	0.790%
19	7.824	1096	1105	1120	rBV	629273	1154879	26.71%	1.865%
20	8.366	1187	1194	1206	rBV	870059	1419613	32.83%	2.292%
21	8.653	1232	1241	1247	rBV	1070203	1702586	39.38%	2.749%
22	8.720	1247	1252	1266	rVB	611145	915729	21.18%	1.479%
23	8.982	1288	1295	1306	rBV	950072	1347172	31.16%	2.175%
24	9.153	1316	1323	1334	rBV	1803814	2595567	60.03%	4.191%
25	9.275	1337	1343	1353	rVB	1836825	2623846	60.68%	4.236%
26	9.610	1392	1398	1411	rBV	775546	1114018	25.76%	1.799%
27	10.055	1465	1471	1483	rBV	1071734	1397875	32.33%	2.257%
28	10.165	1483	1489	1491	rVV	1046939	1407914	32.56%	2.273%
29	10.195	1491	1494	1504	rVV	1977433	2453522	56.74%	3.961%
30	10.305	1506	1512	1521	rVB	727395	981717	22.70%	1.585%
31	10.646	1562	1568	1576	rBV	673053	888180	20.54%	1.434%
32	10.799	1587	1593	1605	rBV	711399	976767	22.59%	1.577%
33	11.079	1634	1639	1654	rBV	860582	1134416	26.24%	1.832%
34	11.451	1695	1700	1710	rVB	746202	931748	21.55%	1.504%
35	11.756	1739	1750	1764	rBV	3323573	4044300	93.53%	6.530%
36	11.969	1780	1785	1790	rBV	2473005	3031940	70.12%	4.895%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031122\
Data File : VX027401.D
Acq On : 11 Mar 2022 14:55
Operator : JC/MD
Sample : N1870-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Title : SW846 8260

37	12.042	1790	1797	1803	rVB2	2512727	4323978	100.00%	6.981%
38	12.945	1936	1945	1954	rBV	348684	435621	10.07%	0.703%
39	13.591	2045	2051	2060	rBV	2905813	3501587	80.98%	5.654%
40	13.780	2076	2082	2093	rBV	1865609	2370737	54.83%	3.828%


Sum of corrected areas: 61935230

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031122\
Data File : VX027401.D
Acq On : 11 Mar 2022 14:55
Operator : JC/MD
Sample : N1870-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

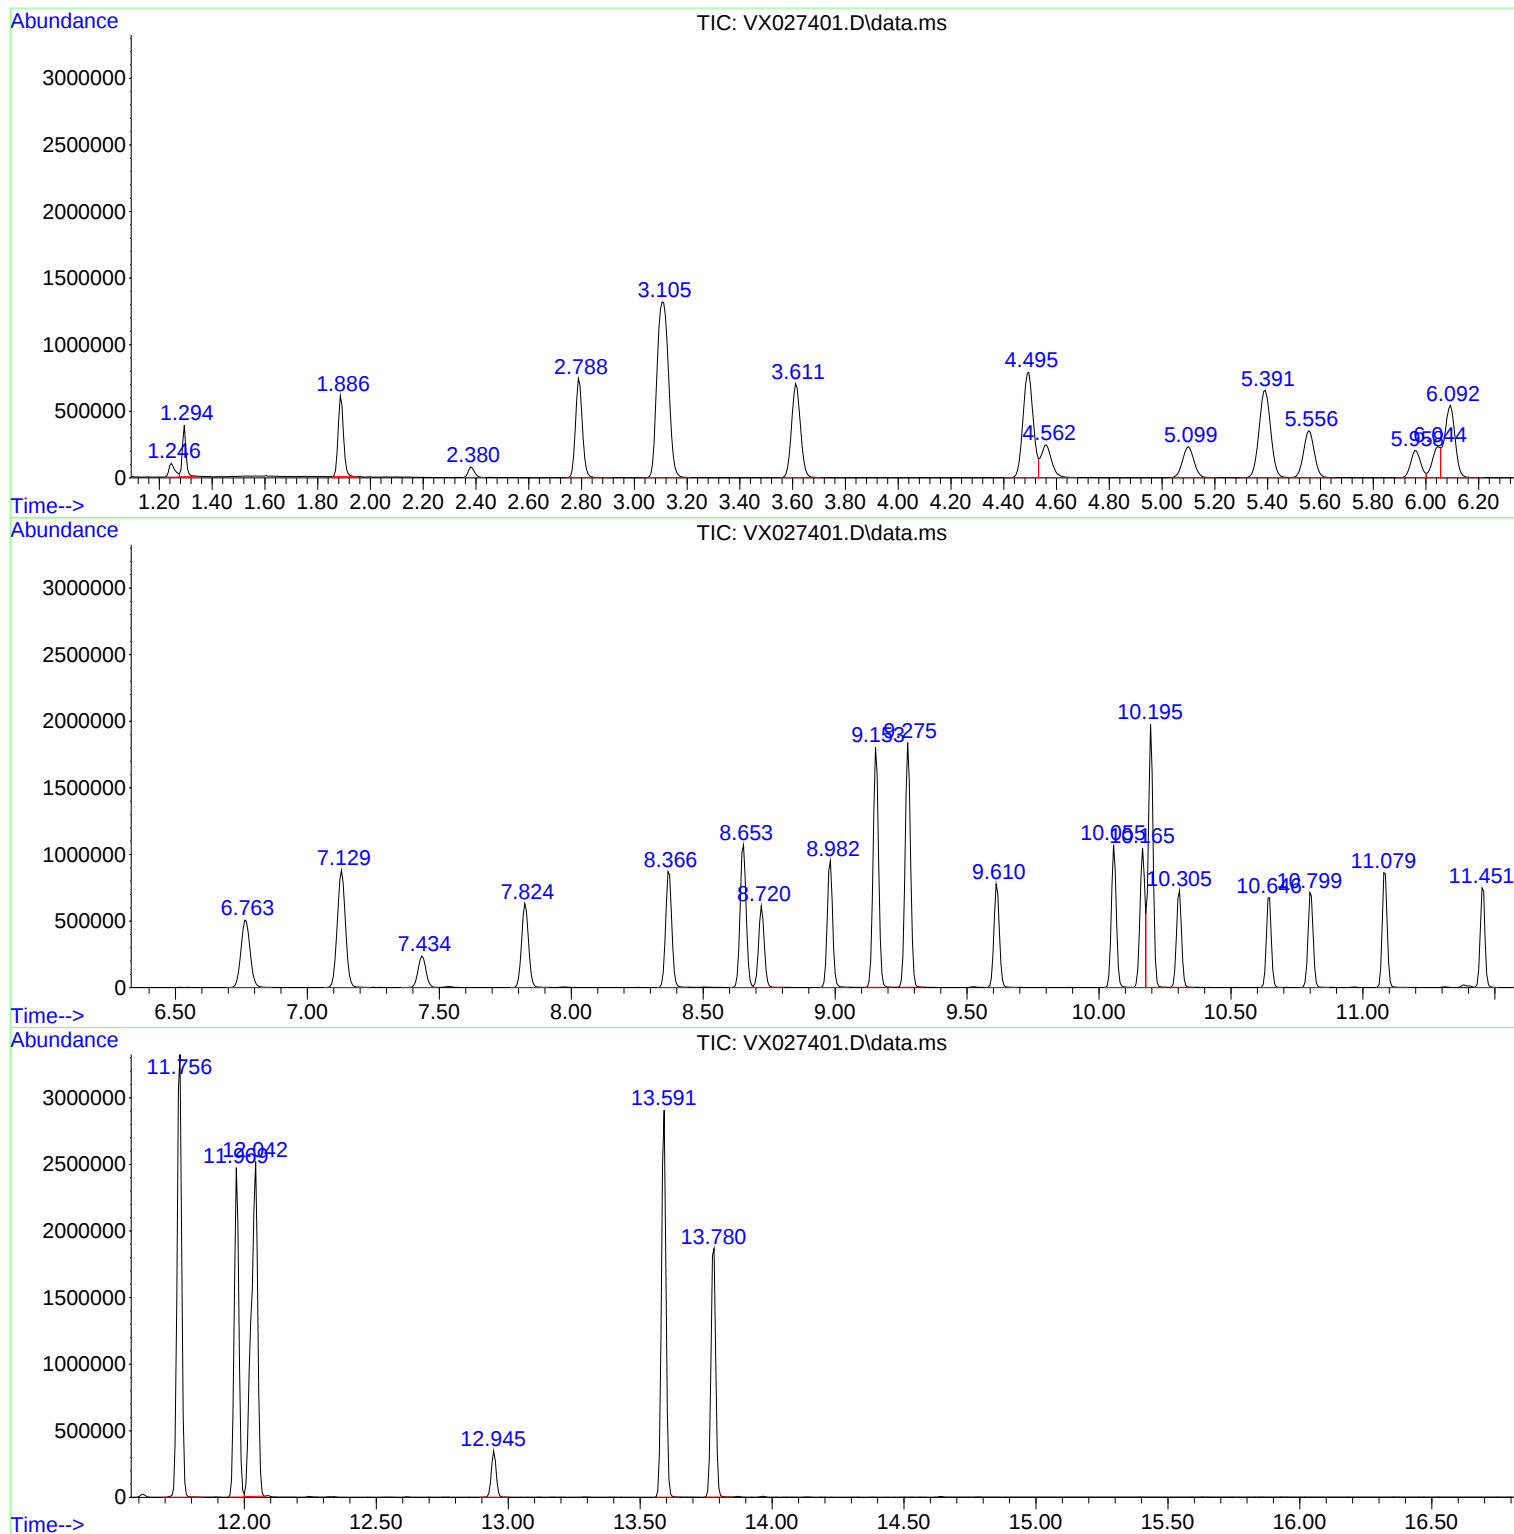

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031122\
Data File : VX027401.D
Acq On : 11 Mar 2022 14:55
Operator : JC/MD
Sample : N1870-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031122\
Data File : VX027401.D
Acq On : 11 Mar 2022 14:55
Operator : JC/MD
Sample : N1870-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------