

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031122\
 Data File : VX027403.D
 Acq On : 11 Mar 2022 15:42
 Operator : JC/MD
 Sample : N1895-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-120

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
 Title : SW846 8260

Signal : TIC: VX027403.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	40	rBV	60439	123859	6.87%	1.270%
2	2.538	232	238	250	rVB	12546	25534	1.42%	0.262%
3	5.391	693	706	721	rBV	222615	641429	35.59%	6.579%
4	5.556	721	733	752	rVB	380177	1064913	59.09%	10.922%
5	5.964	790	800	817	rBV	206688	552428	30.65%	5.666%
6	6.763	920	931	947	rBV	559269	1339845	74.34%	13.742%
7	8.653	1234	1241	1250	rBV	1178763	1802224	100.00%	18.484%
8	10.055	1465	1471	1481	rBV	1180319	1548006	85.89%	15.877%
9	10.305	1507	1512	1521	rVB	38607	55106	3.06%	0.565%
10	11.085	1634	1640	1652	rBV	928815	1181179	65.54%	12.114%
11	12.024	1789	1794	1802	rBV	1174011	1415768	78.56%	14.520%




Sum of corrected areas: 9750291

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031122\
Data File : VX027403.D
Acq On : 11 Mar 2022 15:42
Operator : JC/MD
Sample : N1895-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-120

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

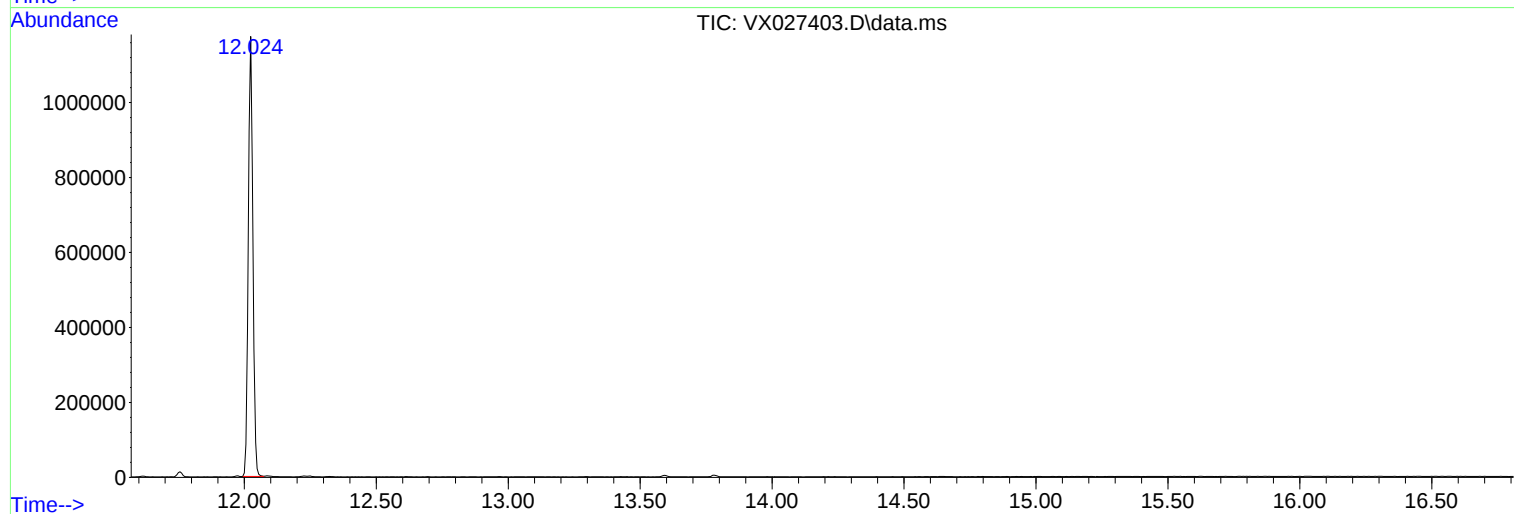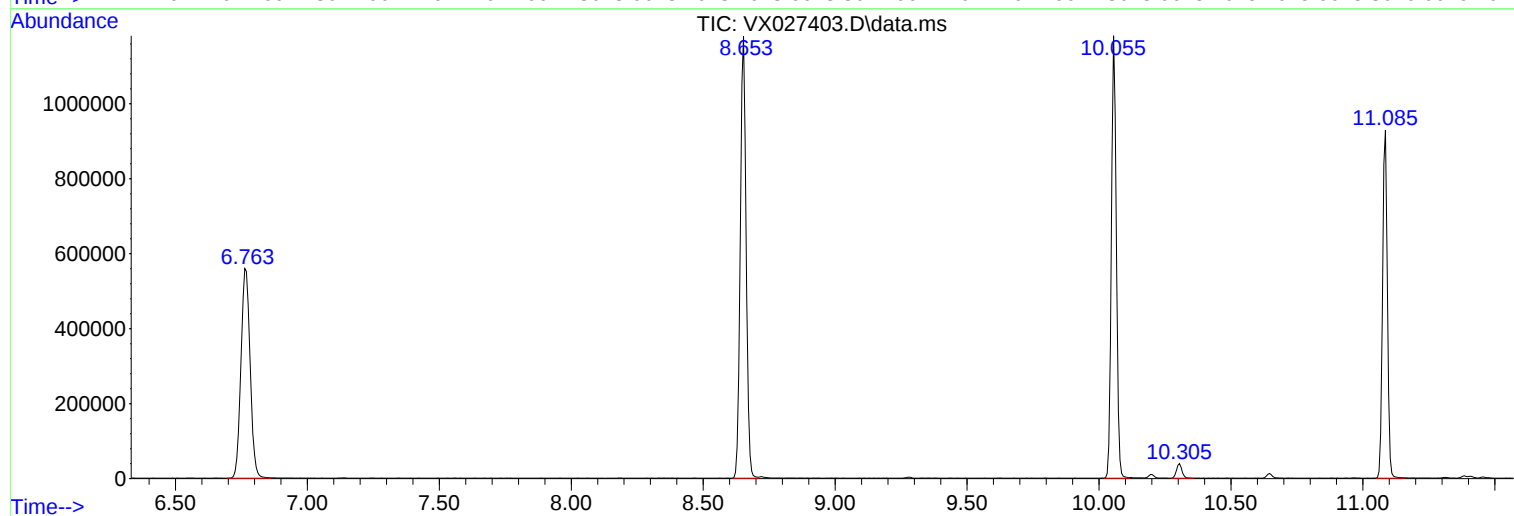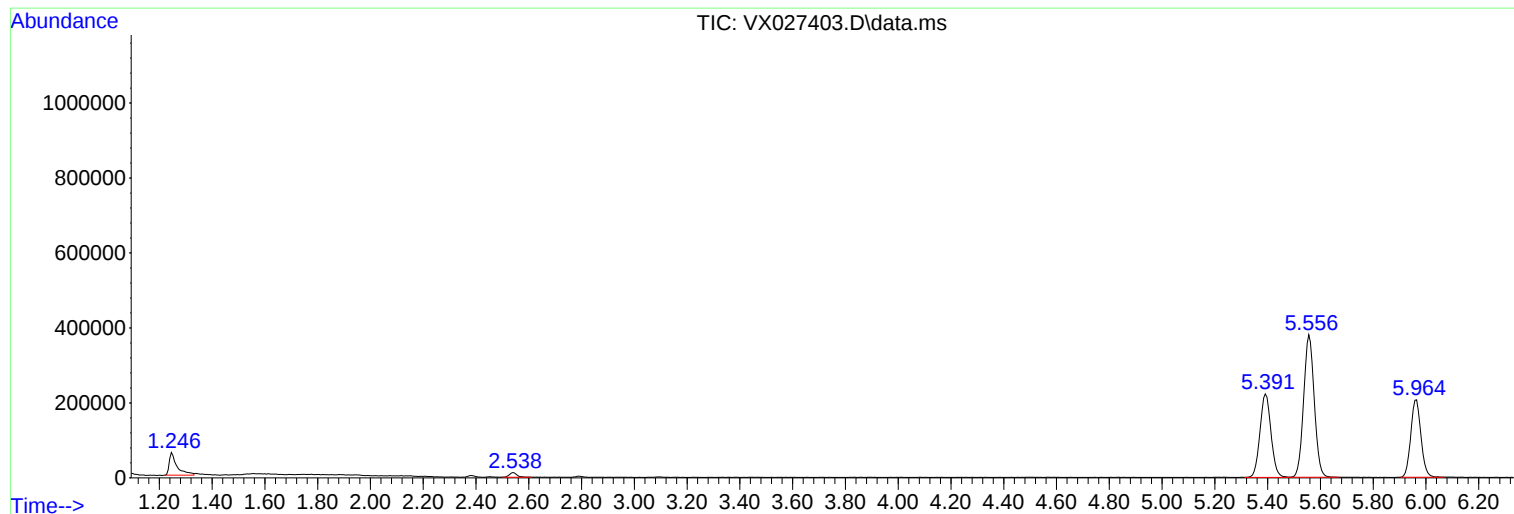

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031122\
Data File : VX027403.D
Acq On : 11 Mar 2022 15:42
Operator : JC/MD
Sample : N1895-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-120







Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.246	5.82 ug/l	123859	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	90
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	4

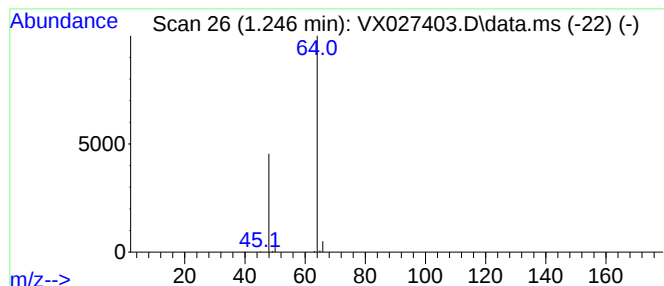

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031122\
Data File : VX027403.D
Acq On : 11 Mar 2022 15:42
Operator : JC/MD
Sample : N1895-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-120

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.246	5.8	ug/l	123859	1	5.556	1064910	50.0