

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031122\
Data File : VX027405.D
Acq On : 11 Mar 2022 16:29
Operator : JC/MD
Sample : N1895-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PZ-5

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M

Title : SW846 8260

Signal : TIC: VX027405.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	48	rBV	43557	106385	5.98%	1.098%
2	3.117	325	333	340	rBV	15307	34913	1.96%	0.360%
3	5.391	694	706	722	rBV	217984	629671	35.38%	6.501%
4	5.556	722	733	749	rVB	372665	1042125	58.55%	10.760%
5	5.958	789	799	813	rBV	202029	543418	30.53%	5.611%
6	6.763	921	931	945	rBV	554593	1311755	73.70%	13.544%
7	8.653	1234	1241	1250	rBV	1140918	1779772	100.00%	18.376%
8	10.055	1465	1471	1487	rBV	1181304	1551404	87.17%	16.018%
9	10.305	1507	1512	1519	rVB	24572	33272	1.87%	0.344%
10	11.085	1634	1640	1652	rBV	938080	1196336	67.22%	12.352%
11	12.024	1789	1794	1802	rBV	1218833	1456285	81.82%	15.036%




Sum of corrected areas: 9685336

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031122\
Data File : VX027405.D
Acq On : 11 Mar 2022 16:29
Operator : JC/MD
Sample : N1895-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PZ-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

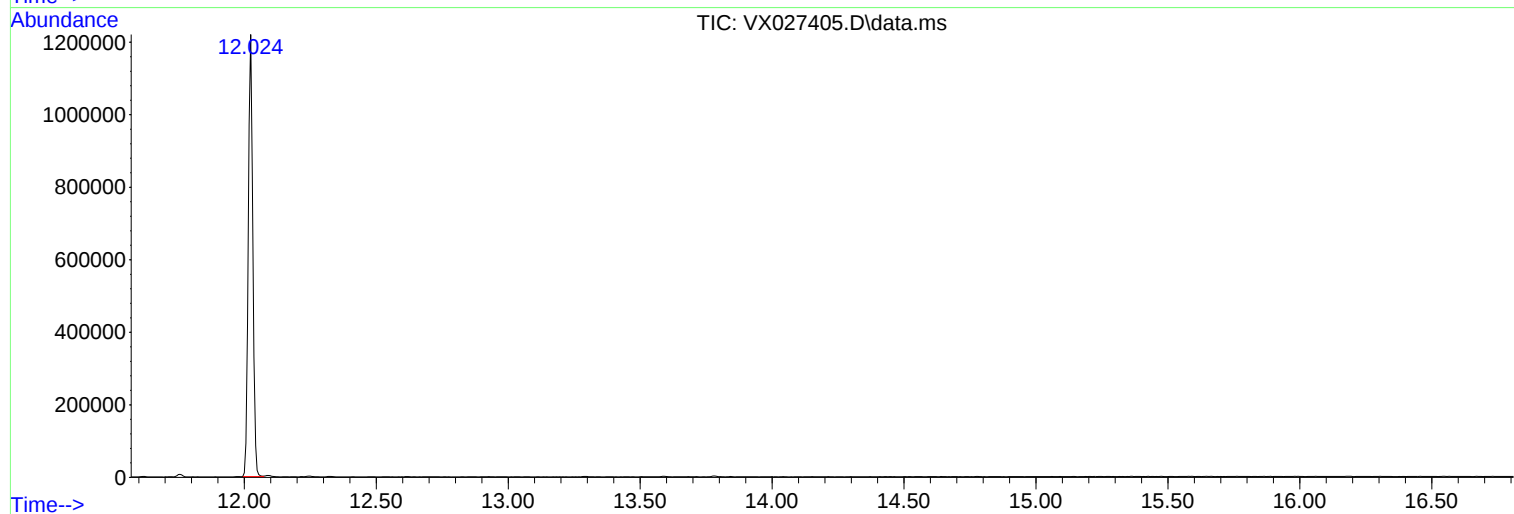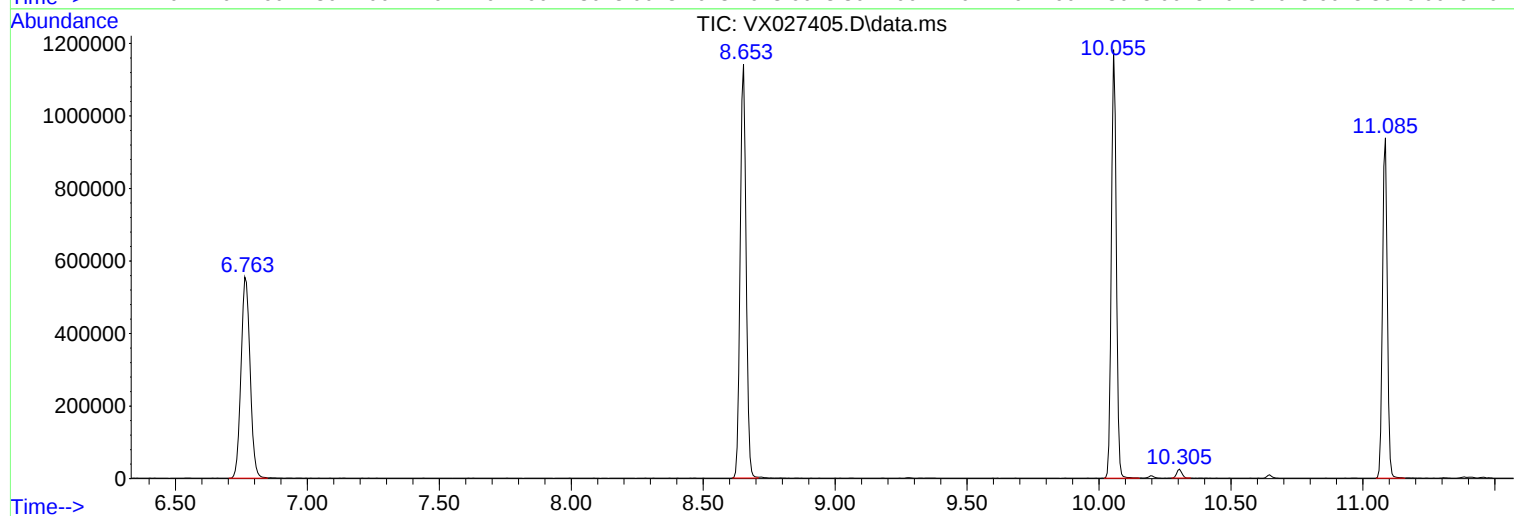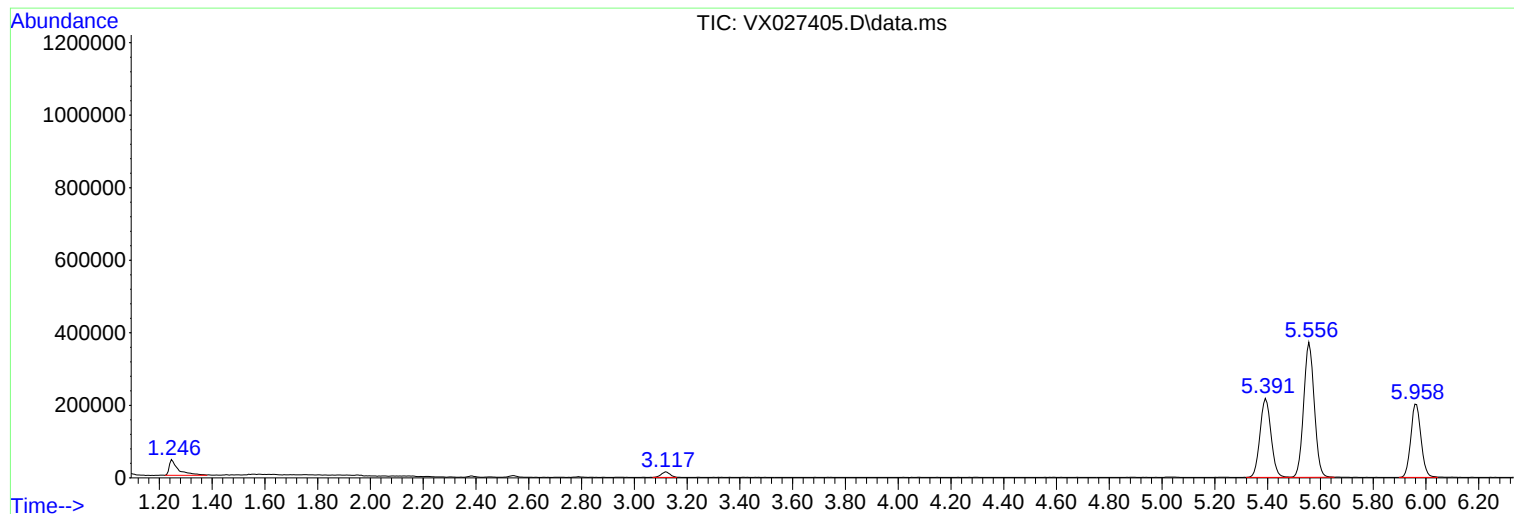

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031122\
Data File : VX027405.D
Acq On : 11 Mar 2022 16:29
Operator : JC/MD
Sample : N1895-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PZ-5







Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.246	5.10 ug/l	106385	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	83
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	3

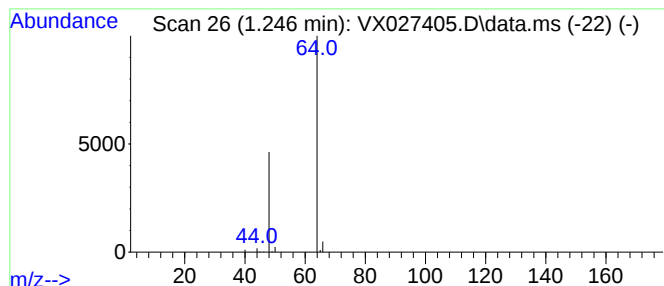

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031122\
Data File : VX027405.D
Acq On : 11 Mar 2022 16:29
Operator : JC/MD
Sample : N1895-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PZ-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.246	5.1	ug/l	106385	1	5.556	1042130	50.0