

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
 Data File : VX045216.D
 Acq On : 11 Mar 2025 12:03
 Operator : JC/MD
 Sample : Q1502-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PT-VOA-WP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Title : SW846 8260

Signal : TIC: VX045216.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.593	66	83	93	rBV	101651	136719	4.59%	0.570%
2	1.874	123	129	153	rBV	329445	462659	15.52%	1.929%
3	2.313	194	201	208	rBV	327685	530186	17.78%	2.211%
4	2.386	208	213	221	rVB	97287	162928	5.46%	0.679%
5	2.782	271	278	297	rBV	152061	305909	10.26%	1.275%
6	3.087	321	328	348	rBV2	281795	956471	32.08%	3.988%
7	4.483	546	557	566	rBV	270979	731707	24.54%	3.051%
8	4.562	566	570	583	rVB	23769	66256	2.22%	0.276%
9	5.087	644	656	673	rBV	140460	428488	14.37%	1.787%
10	5.379	693	704	719	rBV	66165	196950	6.61%	0.821%
11	5.544	721	731	742	rVV	105788	307020	10.30%	1.280%
12	5.666	742	751	767	rVB2	59276	174457	5.85%	0.727%
13	5.952	788	798	803	rBV2	82985	208162	6.98%	0.868%
14	6.031	803	811	836	rVB	489885	1458779	48.93%	6.082%
15	6.757	920	930	955	rBV	177483	434724	14.58%	1.813%
16	7.123	981	990	1003	rBV	163644	368218	12.35%	1.535%
17	7.428	1031	1040	1057	rBV	263412	546807	18.34%	2.280%
18	7.580	1057	1065	1081	rBV	228936	450947	15.12%	1.880%
19	7.824	1097	1105	1114	rBV	44678	88003	2.95%	0.367%
20	8.360	1187	1193	1205	rBV	218791	367927	12.34%	1.534%
21	8.574	1222	1228	1234	rBV	409461	645332	21.64%	2.691%
22	8.647	1234	1240	1246	rVV	354413	579423	19.43%	2.416%
23	8.714	1246	1251	1274	rVB	864981	1382152	46.36%	5.763%
24	8.976	1288	1294	1310	rBV	304731	441218	14.80%	1.840%
25	9.269	1335	1342	1363	rBV	673126	1006249	33.75%	4.195%
26	9.427	1363	1368	1383	rBV	359300	517234	17.35%	2.157%
27	10.073	1471	1474	1483	rVB	907241	1329514	44.59%	5.543%
28	10.159	1483	1488	1491	rVV	582491	816954	27.40%	3.406%
29	10.189	1491	1493	1505	rVB	355435	452450	15.18%	1.886%
30	10.299	1505	1511	1527	rVB	702163	952944	31.96%	3.973%
31	10.640	1561	1567	1590	rBV3	1729560	2981512	100.00%	12.431%
32	11.079	1634	1639	1653	rBV	268708	346482	11.62%	1.445%
33	11.451	1694	1700	1709	rVB	953906	1177789	39.50%	4.911%
34	11.963	1779	1784	1789	rBV	350034	466508	15.65%	1.945%
35	12.018	1789	1793	1805	rVB	365570	452457	15.18%	1.886%
36	12.329	1839	1844	1857	rBV	875450	1142007	38.30%	4.761%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
Data File : VX045216.D
Acq On : 11 Mar 2025 12:03
Operator : JC/MD
Sample : Q1502-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Title : SW846 8260

37	13.774	2076	2081	2092	rBV	753224	910872	30.55%	3.798%
----	--------	------	------	------	-----	--------	--------	--------	--------




Sum of corrected areas: 23984414

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
Data File : VX045216.D
Acq On : 11 Mar 2025 12:03
Operator : JC/MD
Sample : Q1502-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

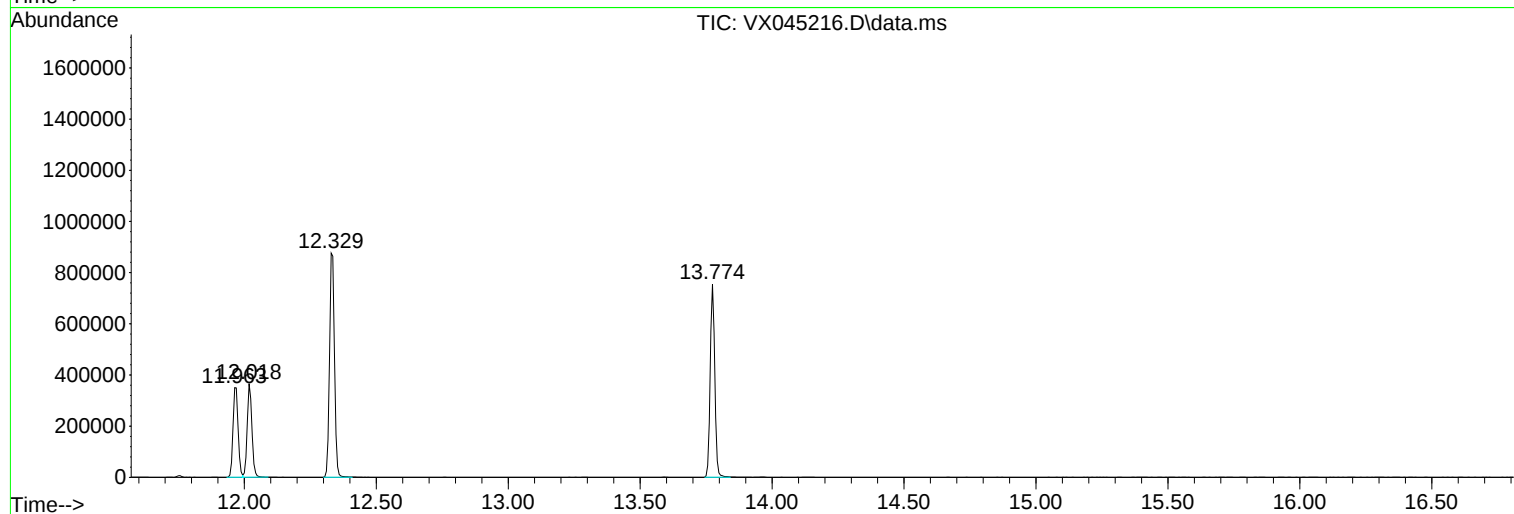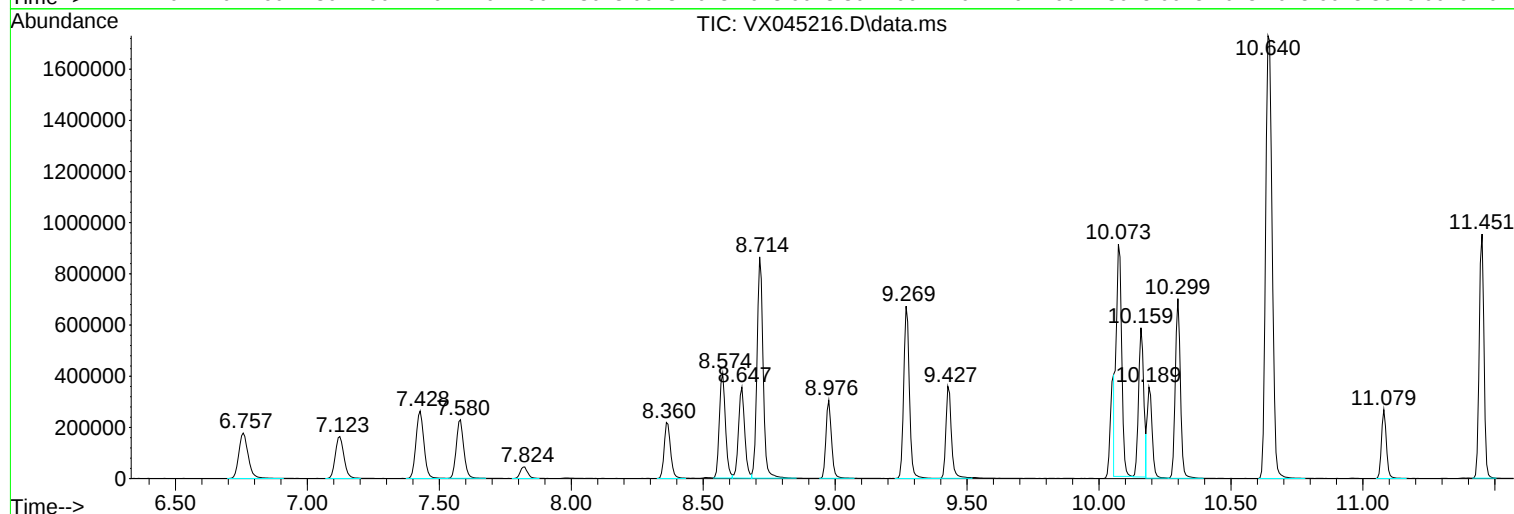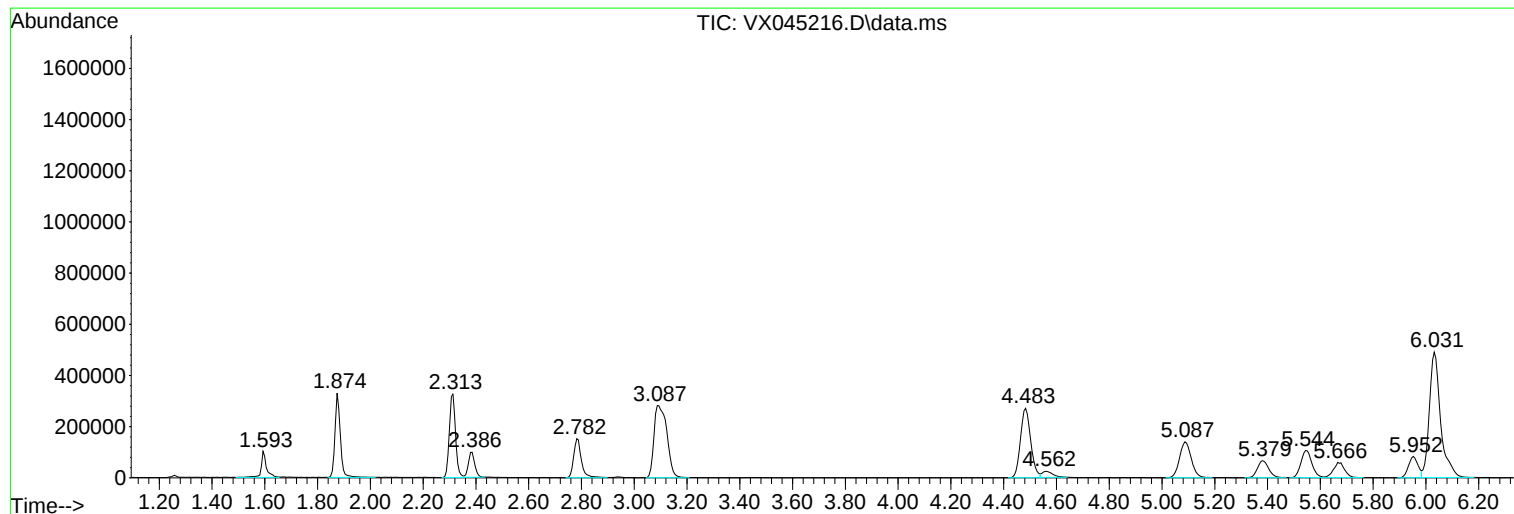

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
Data File : VX045216.D
Acq On : 11 Mar 2025 12:03
Operator : JC/MD
Sample : Q1502-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
Data File : VX045216.D
Acq On : 11 Mar 2025 12:03
Operator : JC/MD
Sample : Q1502-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc