


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031219\
Data File : VX008009.D
Acq On : 12 Mar 2019 11:35
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X030619W.M
Title : SW846 8260
Last Update : Thu Mar 07 07:33:26 2019

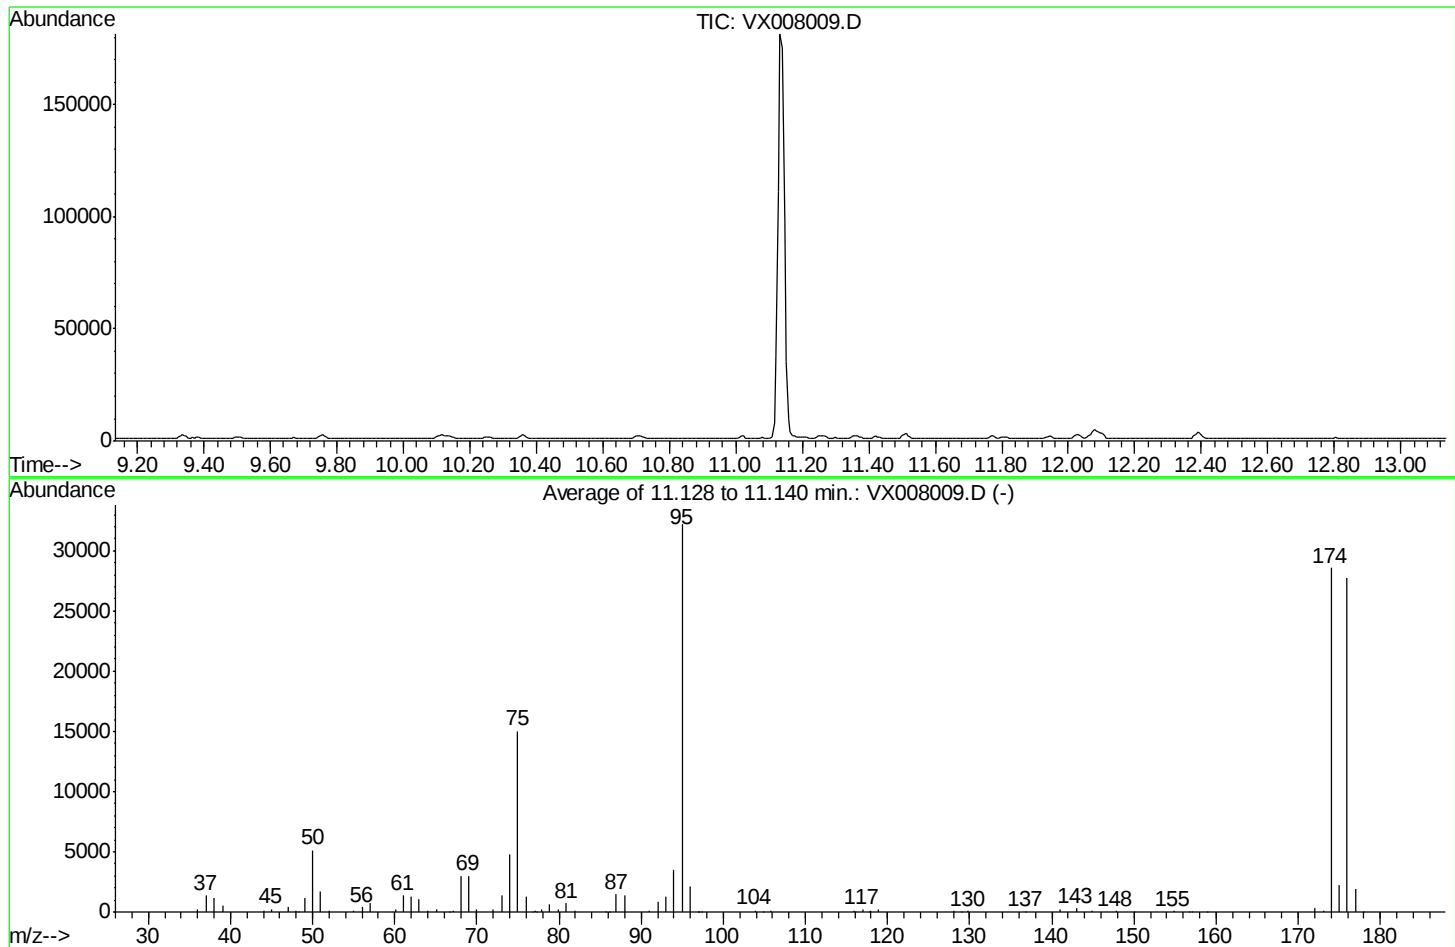

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	5120	PASS
75	95	30	60	46.6	15019	PASS
95	95	100	100	100.0	32197	PASS
96	95	5	9	6.7	2166	PASS
173	174	0.00	2	0.2	69	PASS
174	95	50	100	88.7	28549	PASS
175	174	5	9	7.8	2224	PASS
176	174	95	101	97.0	27701	PASS
177	176	5	9	6.8	1897	PASS