


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX031220\  
 Data File : VX015221.D  
 Acq On : 12 Mar 2020 08:23  
 Operator : JC/SP  
 Sample : BFB  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X030420W.M  
 Title : SW846 8260  
 Last Update : Wed Mar 04 14:19:10 2020

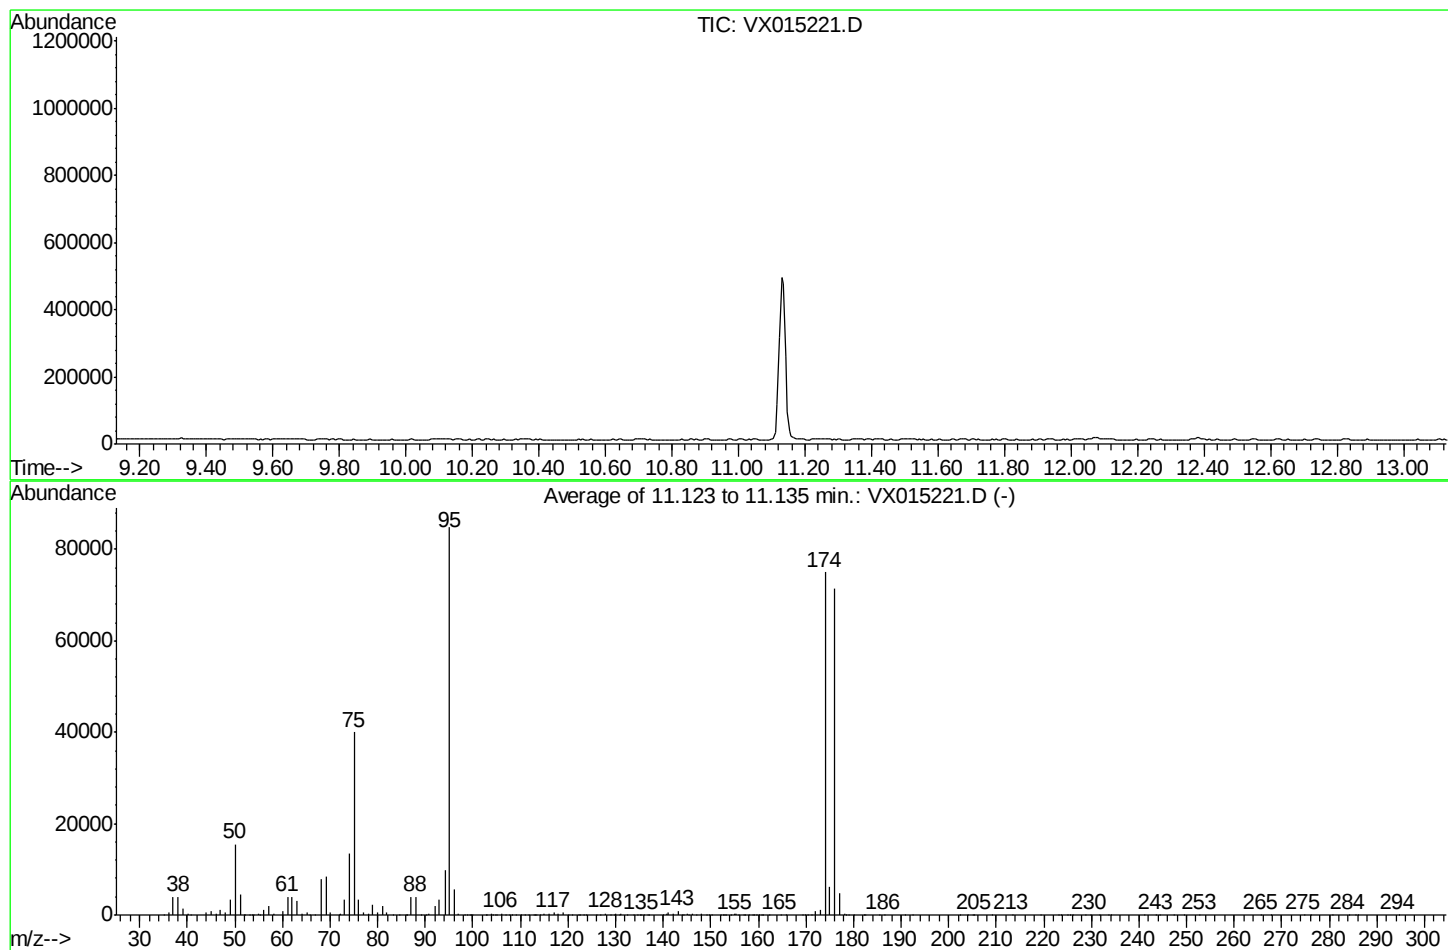

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1670

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 18.2      | 15461   | PASS             |
| 75          | 95           | 30           | 60           | 47.2      | 40056   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 84834   | PASS             |
| 96          | 95           | 5            | 9            | 6.7       | 5686    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.6       | 1177    | PASS             |
| 174         | 95           | 50           | 100          | 88.3      | 74950   | PASS             |
| 175         | 174          | 5            | 9            | 8.1       | 6055    | PASS             |
| 176         | 174          | 95           | 101          | 95.2      | 71352   | PASS             |
| 177         | 176          | 5            | 9            | 6.7       | 4749    | PASS             |