
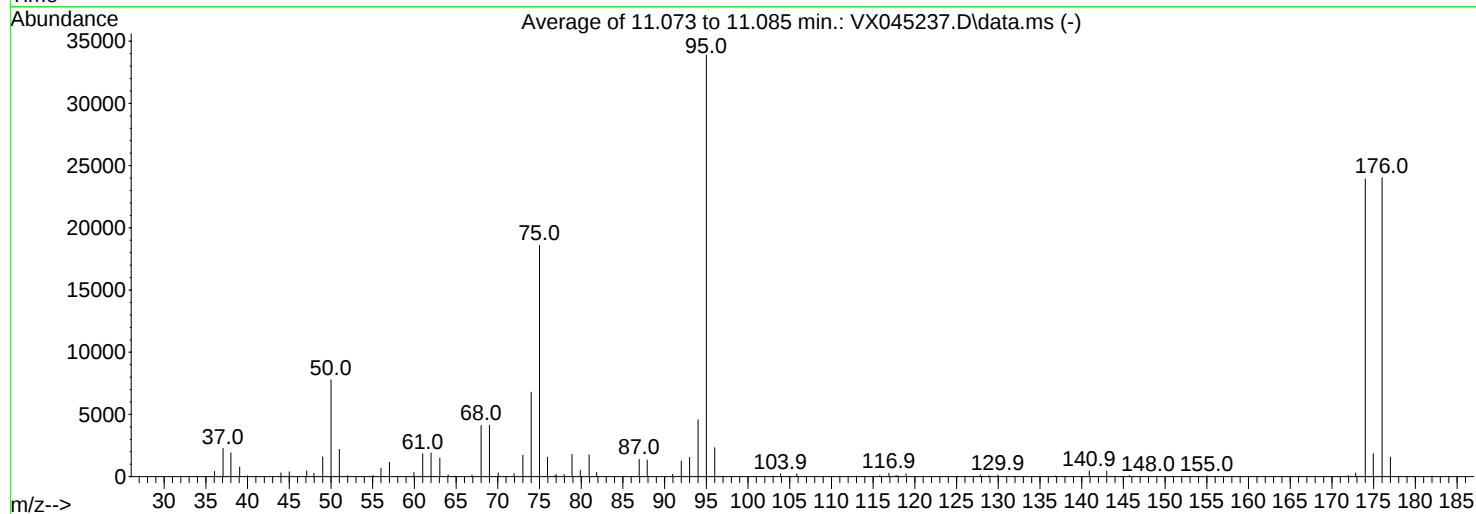


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031225\
Data File : VX045237.D
Acq On : 12 Mar 2025 10:30
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Title : SW846 8260
Last Update : Fri Feb 28 06:45:16 2025

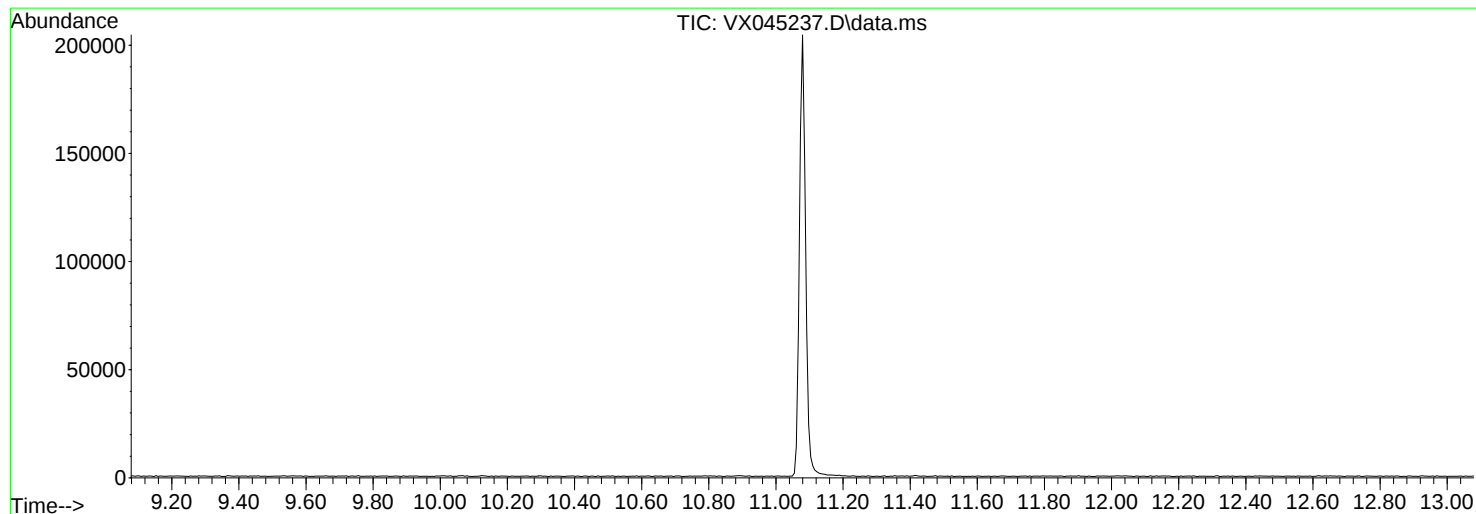

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	7782	PASS
75	95	30	60	54.8	18587	PASS
95	95	100	100	100.0	33899	PASS
96	95	5	9	6.9	2327	PASS
173	174	0.00	2	1.2	295	PASS
174	95	50	100	70.6	23949	PASS
175	174	5	9	7.7	1848	PASS
176	174	95	101	100.4	24037	PASS
177	176	5	9	6.5	1560	PASS