


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX031319\
Data File : VX008035.D
Acq On : 13 Mar 2019 08:32
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X030619W.M
Title : SW846 8260
Last Update : Thu Mar 07 07:33:26 2019

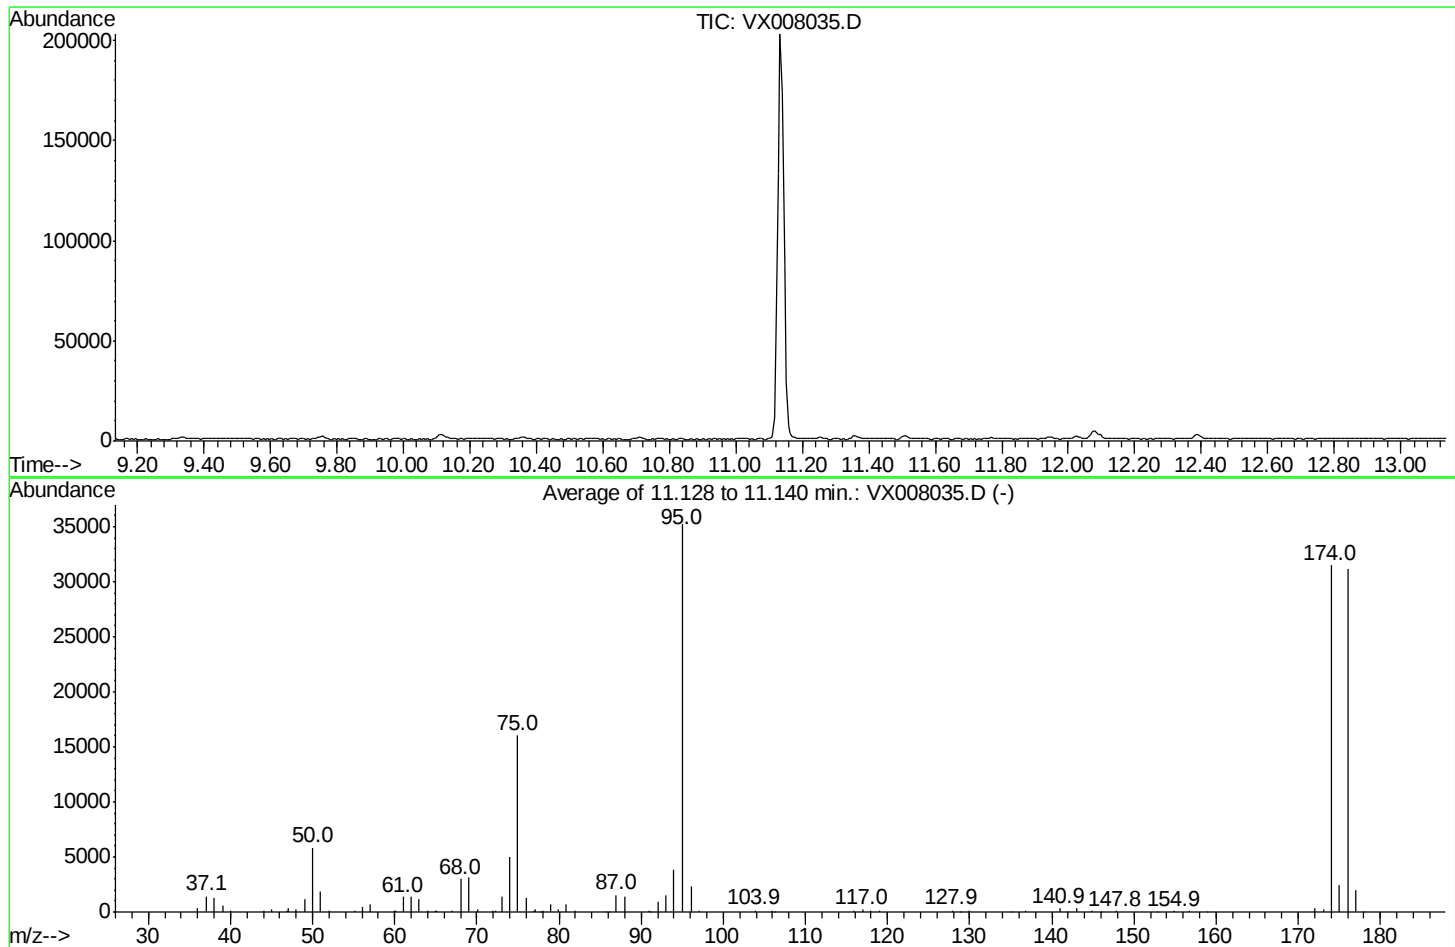

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	5869	PASS
75	95	30	60	45.5	16037	PASS
95	95	100	100	100.0	35213	PASS
96	95	5	9	6.7	2375	PASS
173	174	0.00	2	0.7	211	PASS
174	95	50	100	89.4	31469	PASS
175	174	5	9	7.9	2474	PASS
176	174	95	101	99.2	31210	PASS
177	176	5	9	6.5	2031	PASS