

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX031320\
 Data File : VX015247.D
 Acq On : 13 Mar 2020 10:26
 Operator : JC/SP
 Sample : L1903-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-20200307

Quant Time: Mar 16 08:17:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X030420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 04 14:19:10 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	295335	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	476029	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	450716	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	224980	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.05	65	166129	47.41	ug/l	0.00
Spiked Amount			Recovery	=	94.82%	
35) Dibromofluoromethane	5.49	113	143524	47.79	ug/l	0.00
Spiked Amount			Recovery	=	95.58%	
50) Toluene-d8	8.71	98	579309	50.71	ug/l	0.00
Spiked Amount			Recovery	=	101.42%	
62) 4-Bromofluorobenzene	11.13	95	209141	51.33	ug/l	0.00
Spiked Amount			Recovery	=	102.66%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	1.65	94	1189	0.521	ug/l #	61
10) Methyl Iodide	2.51	142	1549	0.493	ug/l #	52
11) Tert butyl alcohol	3.01	59	737	1.212	ug/l #	72
13) Acrolein	2.27	56	332	0.581	ug/l #	39
15) Acrylonitrile	3.14	53	649	0.429	ug/l #	37
16) Acetone	2.45	43	748	0.527	ug/l #	27
17) Carbon Disulfide	2.57	76	2557	0.321	ug/l	99
21) trans-1,2-Dichloroethene	3.17	96	980	0.320	ug/l #	4
25) 2-Butanone	4.66	43	1042	0.502	ug/l #	61
27) cis-1,2-Dichloroethene	4.59	96	689	0.200	ug/l	28
36) 1,1-Dichloropropene	5.65	75	19441	4.418	ug/l #	49
38) Carbon Tetrachloride	5.66	117	25421	6.120	ug/l #	16
44) Trichloroethene	7.21	130	871	0.240	ug/l	37
46) Dibromomethane	7.66	93	662	0.301	ug/l #	65
49) 1,4-Dioxane	7.74	88	316	3.999	ug/l #	49
76) 1,2,3-Trichloropropane	11.13	75	99019	22.065	ug/l #	33
81) trans-1,4-Dichloro-2-buten	11.13	75	99019	62.620	ug/l #	11
87) 1,3-Dichlorobenzene	12.03	146	1737	0.247	ug/l	92
88) 1,4-Dichlorobenzene	12.03	146	1737	0.239	ug/l	90
89) n-Butylbenzene	12.39	91	2391	0.209	ug/l	73
93) 1,2,4-Trichlorobenzene	13.64	180	1953	0.402	ug/l	85
94) Hexachlorobutadiene	13.78	225	1063	0.426	ug/l	76
95) Naphthalene	13.83	128	3692	1.661	ug/l #	90
96) 1,2,3-Trichlorobenzene	14.01	180	1409	0.291	ug/l	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX031320\
Data File : VX015247.D
Acq On : 13 Mar 2020 10:26
Operator : JC/SP
Sample : L1903-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-20200307

Quant Time: Mar 16 08:17:00 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X030420W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 04 14:19:10 2020
Response via : Initial Calibration

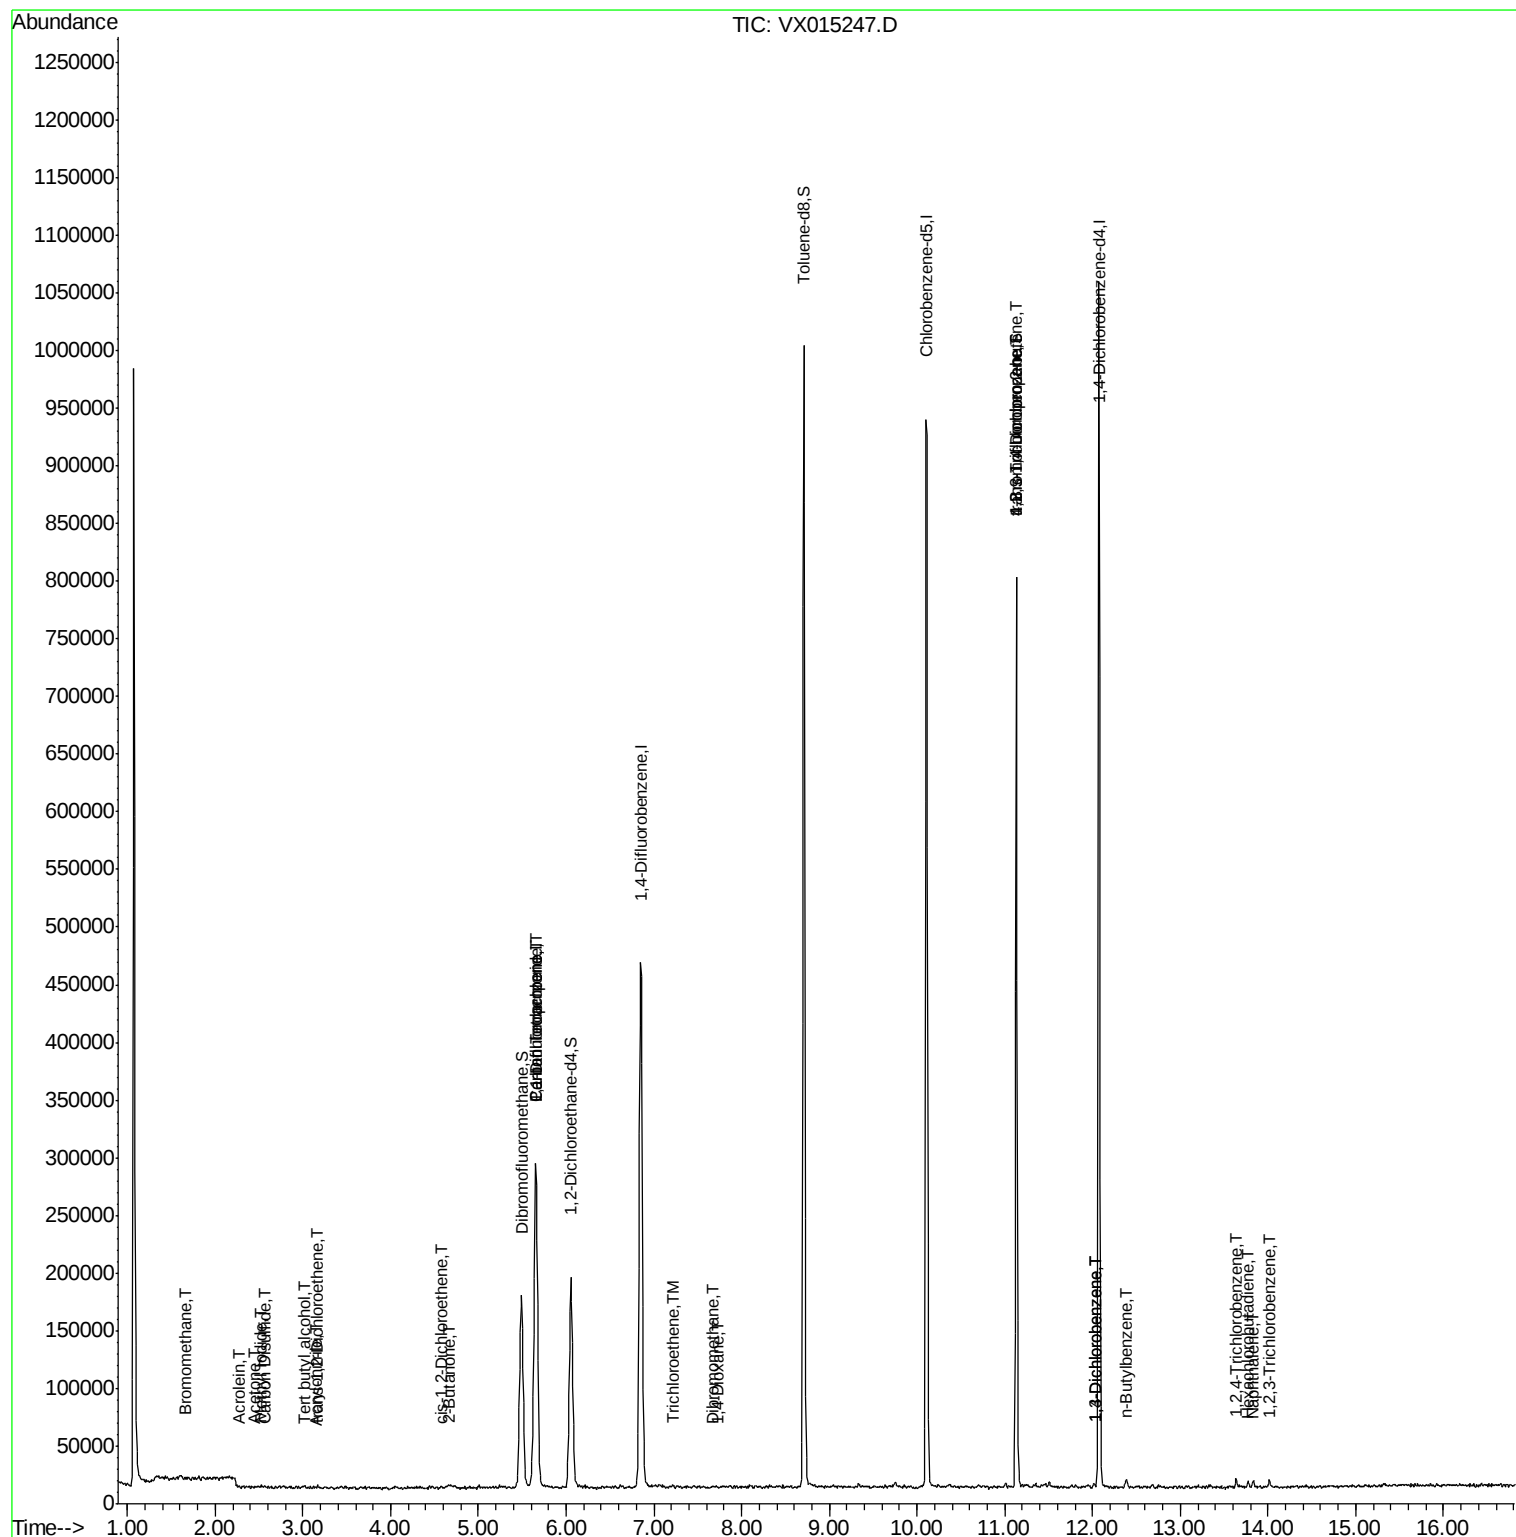



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 782

Delta R.T. 0.00 min

Lab File: VX015247.D

Acq: 13 Mar 2020 10:26

Instrument :

MSVOA_X

ClientSampleId :


TB-20200307

Tot Ion:168 Resp: 295335

Ion Ratio Lower Upper

168 100

99 49.7 39.4 59.2

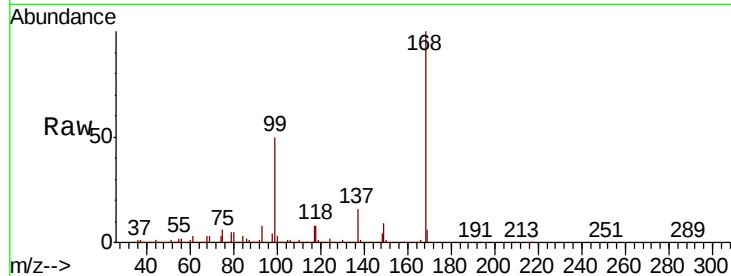

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.65

120000

100000

80000



60000

40000

20000

0

Time-->

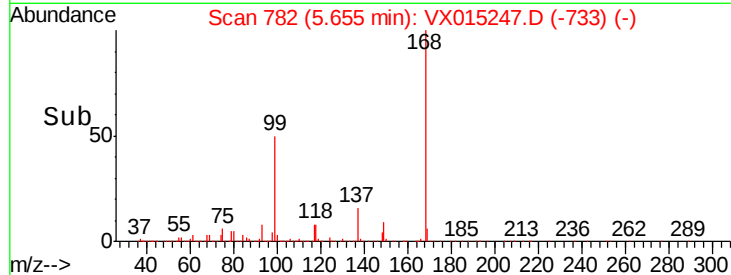

#5

Bromomethane

Concen: 0.521 ug/l

RT: 1.65 min Scan# 125

Delta R.T. 0.01 min

Lab File: VX015247.D


Acq: 13 Mar 2020 10:26

Tgt Ion: 94 Resp: 1189

Ion Ratio Lower Upper

94 100

96 55.6 74.6 111.8#

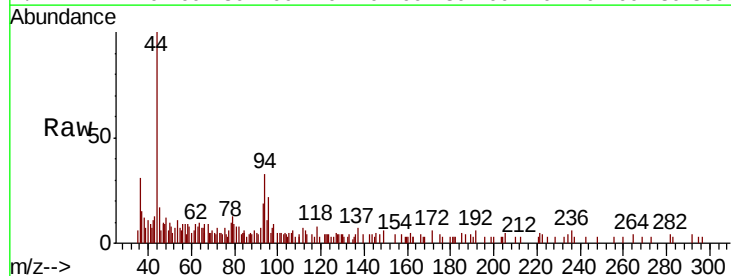

Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

1.65

800


600


400

200

0

Time-->




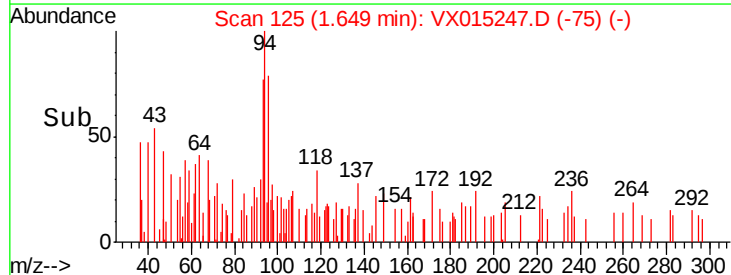


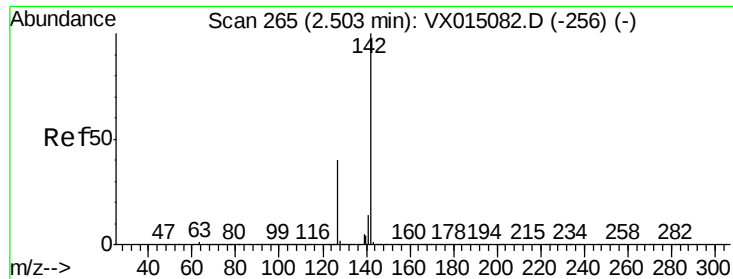

#10
Methvl Iodide
Concen: 0.493 ug/l
RT: 2.51 min Scan# 267
Delta R.T. 0.01 min
Lab File: VX015247.D
Acq: 13 Mar 2020 10:26




Instrument :
MSVOA_X
ClientSampleId :
TB-20200307


Tot Ion:142 Resp: 1549
Ion Ratio Lower Upper
142 100
127 0.0 31.7 47.5#
141 13.8 11.3 16.9

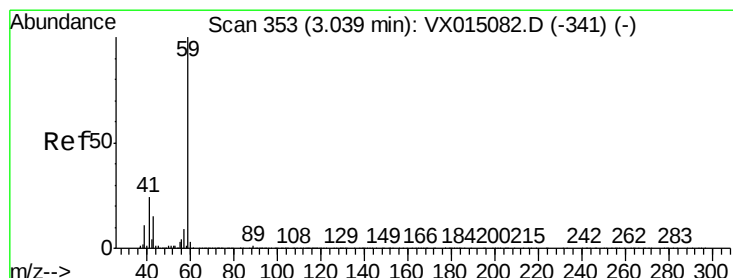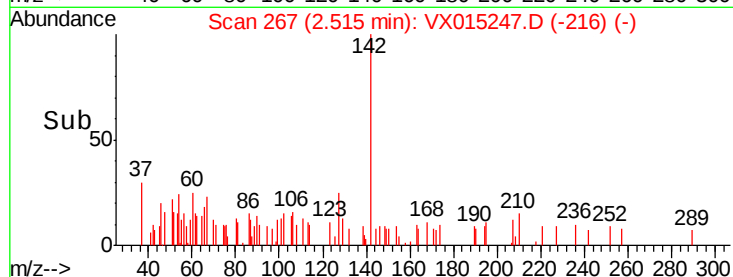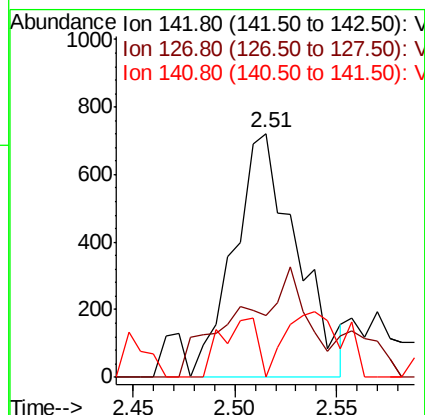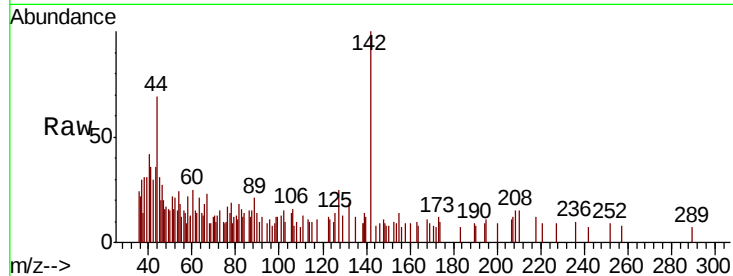

#11
Tert butyl alcohol
Concen: 1.212 ug/l
RT: 3.01 min Scan# 349
Delta R.T. -0.02 min
Lab File: VX015247.D
Acq: 13 Mar 2020 10:26

Tgt Ion: 59 Resp: 737
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

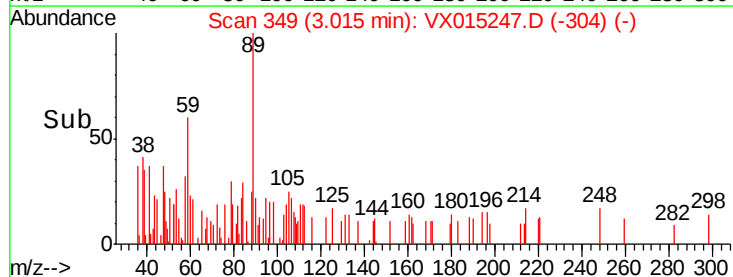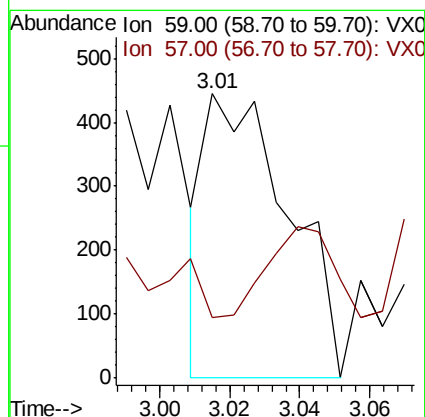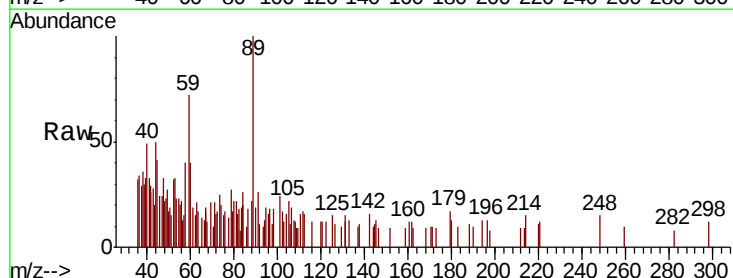

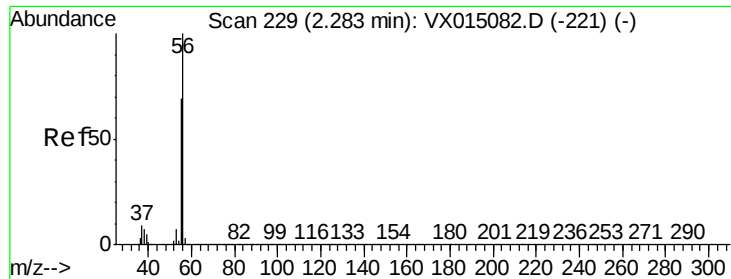

#13

Acrolein

Concen: 0.581 ug/l

RT: 2.27 min Scan# 227

Delta R.T. -0.01 min

Lab File: VX015247.D

Acq: 13 Mar 2020 10:26

Instrument :

MSVOA_X

ClientSampled :





TB-20200307

Tot Ion: 56 Resp: 332

Ion Ratio Lower Upper

56 100

55 119.3 55.4 83.0#

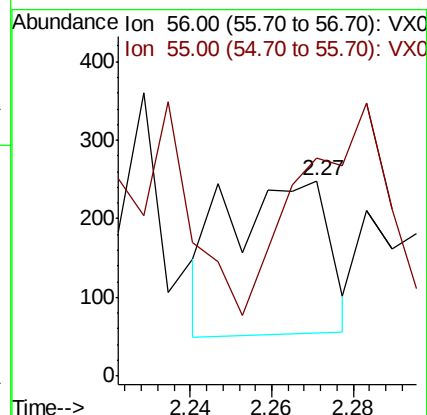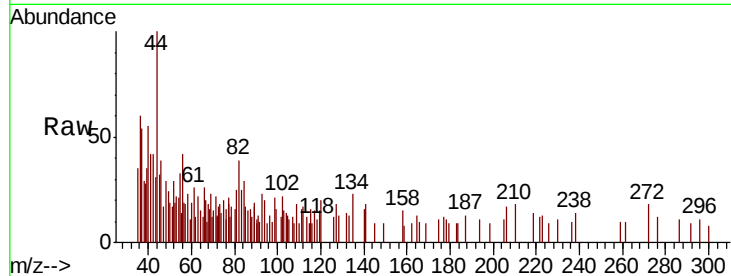

#15

Acrylonitrile

Concen: 0.429 ug/l

RT: 3.14 min Scan# 370

Delta R.T. 0.01 min

Lab File: VX015247.D

Acq: 13 Mar 2020 10:26




Tgt Ion: 53 Resp: 649


Ion Ratio Lower Upper

53 100

52 25.4 66.6 100.0#

51 0.0 29.0 43.6#

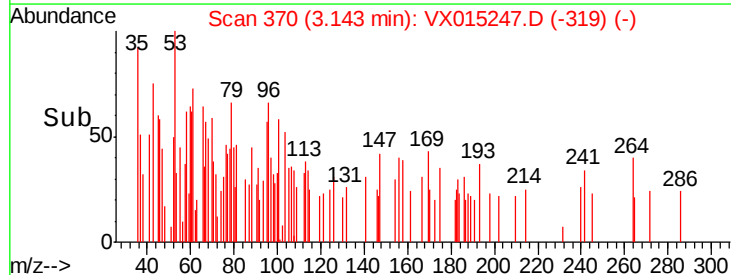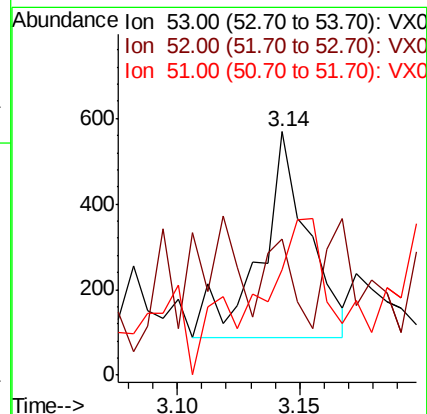



#16

Acetone

Concen: 0.527 ug/l

RT: 2.45 min Scan# 256

Delta R.T. 0.01 min

Lab File: VX015247.D

Acq: 13 Mar 2020 10:26

Instrument :

MSVOA_X

ClientSampleId :





TB-20200307

Tot Ion: 43 Resp: 748

Ion Ratio Lower Upper

43 100

58 71.0 24.8 37.2#

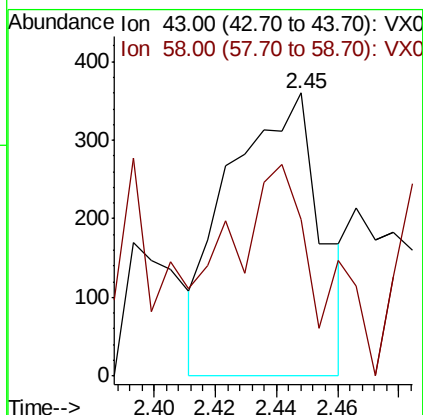

#17

Carbon Disulfide

Concen: 0.321 ug/l

RT: 2.57 min Scan# 276

Delta R.T. 0.01 min

Lab File: VX015247.D




Acq: 13 Mar 2020 10:26


Tgt Ion: 76 Resp: 2557

Ion Ratio Lower Upper

76 100

78 8.9 7.3 10.9

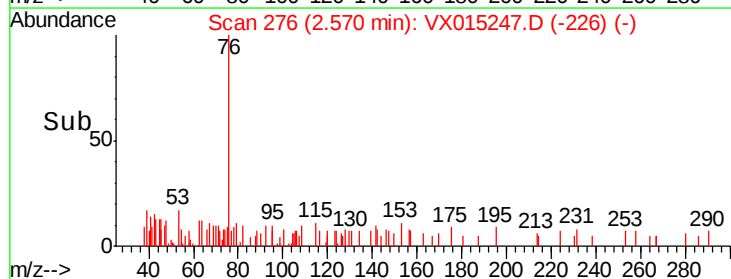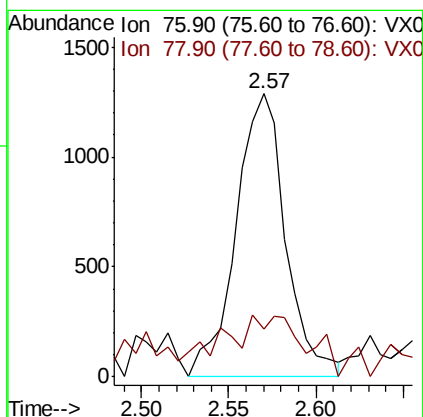

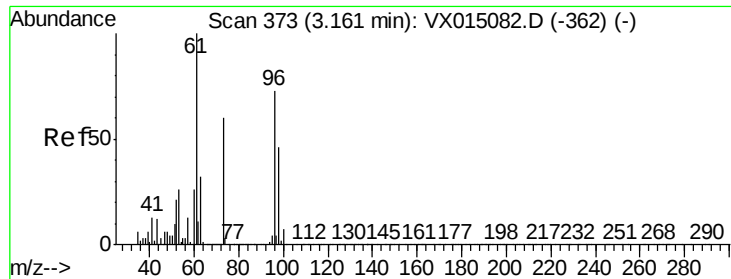

#21

trans-1,2-Dichloroethene

Concen: 0.320 ug/l

RT: 3.17 min Scan# 374

Delta R.T. 0.01 min

Lab File: VX015247.D

Acq: 13 Mar 2020 10:26

Instrument :

MSVOA_X

ClientSampleId :

TB-20200307


Tot Ion: 96 Resp: 980

Ion Ratio Lower Upper

96 100

61 10.9 109.9 164.9#




98 121.9 50.2 75.2#

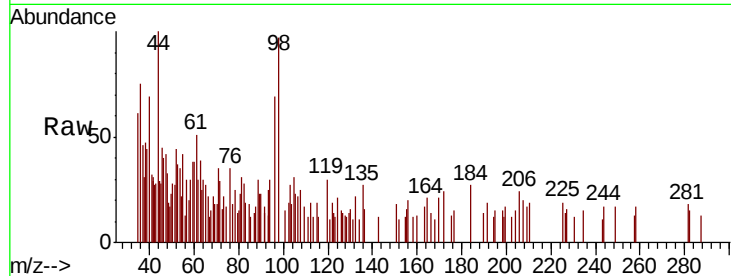

Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

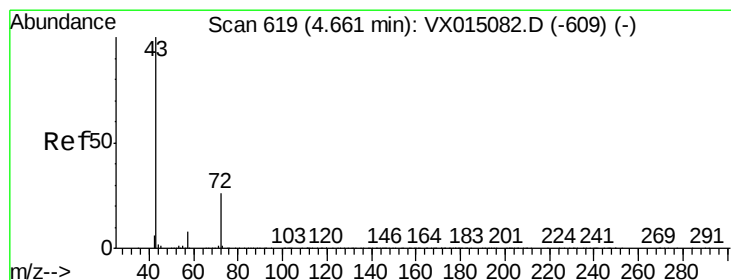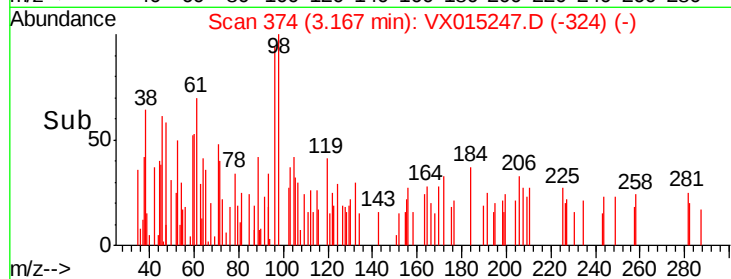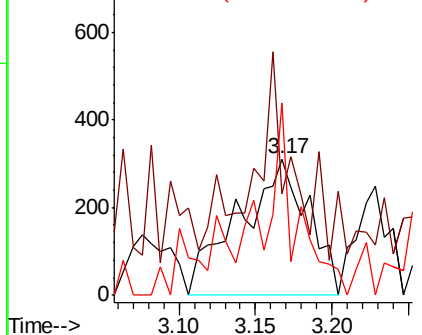

#25

2-Butanone

Concen: 0.502 ug/l

RT: 4.66 min Scan# 619

Delta R.T. 0.00 min

Lab File: VX015247.D


Acq: 13 Mar 2020 10:26

Tgt Ion: 43 Resp: 1042

Ion Ratio Lower Upper



43 100


72 6.0 20.6 30.8#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

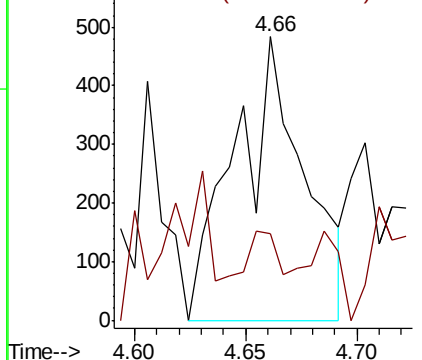







#27

cis-1,2-Dichloroethene
Concen: 0.200 ug/l
RT: 4.59 min Scan# 607
Delta R.T. 0.00 min
Lab File: VX015247.D
Acq: 13 Mar 2020 10:26

Instrument :
MSVOA_X
ClientSampled :
TB-20200307




Tot Ion: 96 Resp: 689
Ion Ratio Lower Upper
96 100
61 33.8 0.0 286.8
98 36.0 0.0 128.4

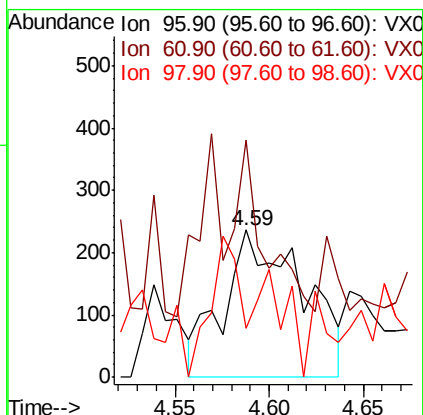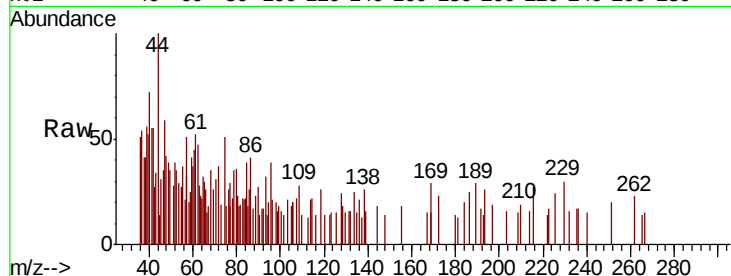


#33

1,2-Dichloroethane-d4
Concen: 47.414 ug/l
RT: 6.05 min Scan# 847
Delta R.T. 0.00 min
Lab File: VX015247.D
Acq: 13 Mar 2020 10:26

Tgt Ion: 65 Resp: 166129
Ion Ratio Lower Upper
65 100
67 54.8 0.0 105.6

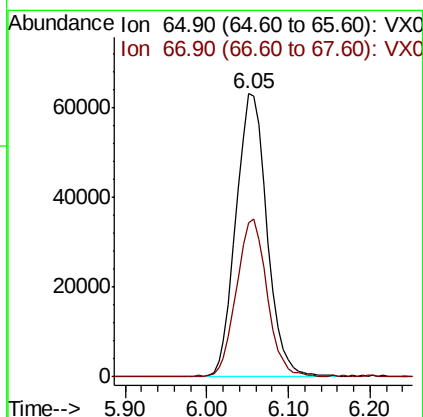

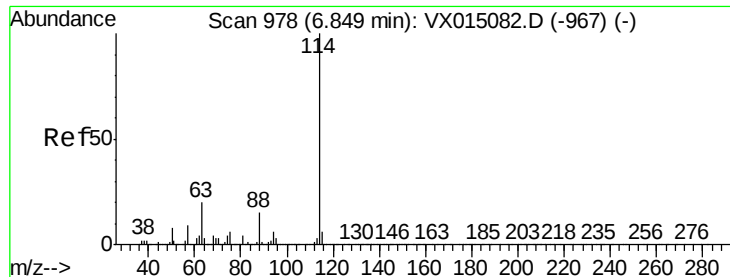

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 978

Delta R.T. 0.00 min

Lab File: VX015247.D

Acq: 13 Mar 2020 10:26

Instrument :

MSVOA_X

ClientSampleId :

TB-20200307


Tot Ion:114 Resp: 476029

Ion Ratio Lower Upper

114 100

63 20.0 0.0 40.0




88 15.9 0.0 30.6



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

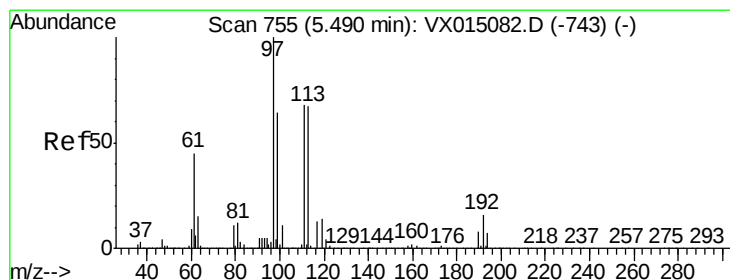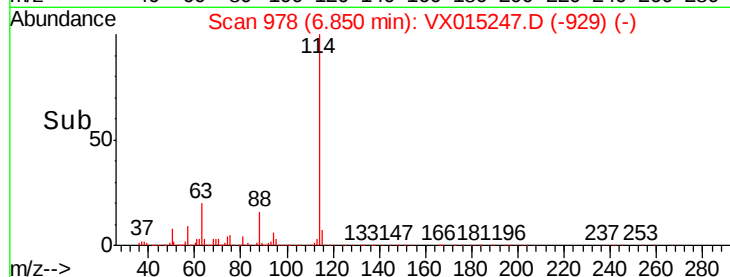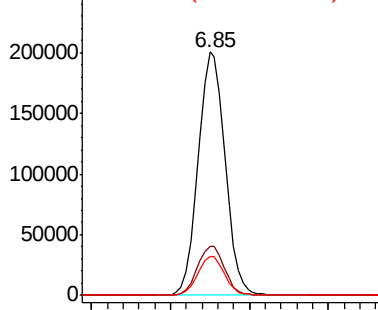

#35

Dibromofluoromethane

Concen: 47.792 ug/l

RT: 5.49 min Scan# 755

Delta R.T. 0.00 min

Lab File: VX015247.D

Acq: 13 Mar 2020 10:26


Tgt Ion:113 Resp: 143524

Ion Ratio Lower Upper

113 100

111 102.7 82.6 123.8



192 25.0 18.6 28.0




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



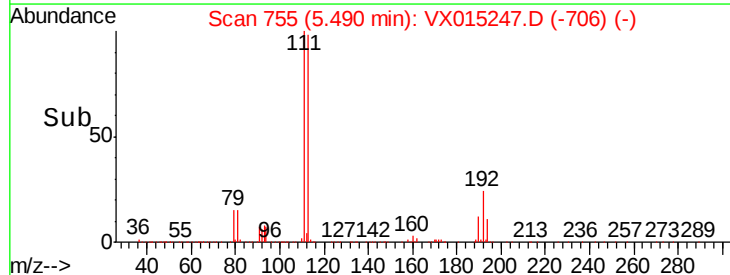
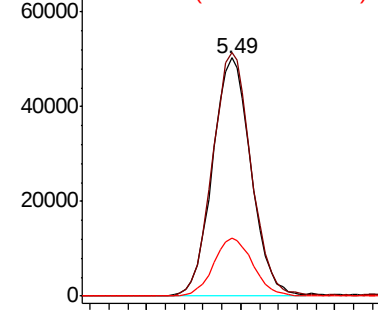




#36
 1,1-Dichloropropene
 Concen: 4.418 ug/l
 RT: 5.65 min Scan# 781
 Delta R.T. -0.15 min
 Lab File: VX015247.D
 Acq: 13 Mar 2020 10:26




Instrument :
 MSVOA_X
 ClientSampleId :
 TB-20200307


Tot Ion	Ratio	Lower	Upper
75	100		
110	9.0	17.9	53.8#
77	0.0	24.8	37.2#

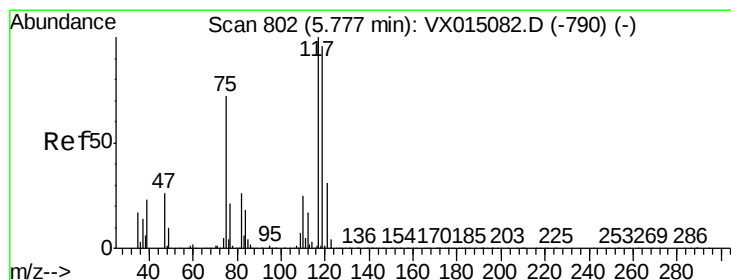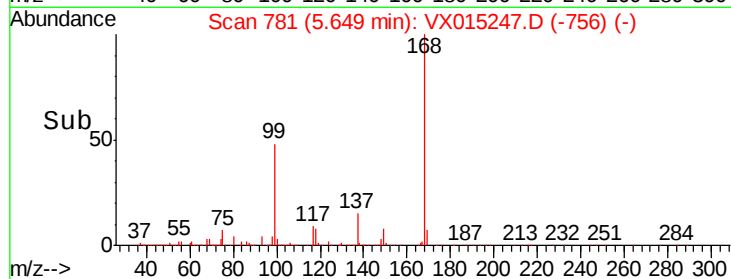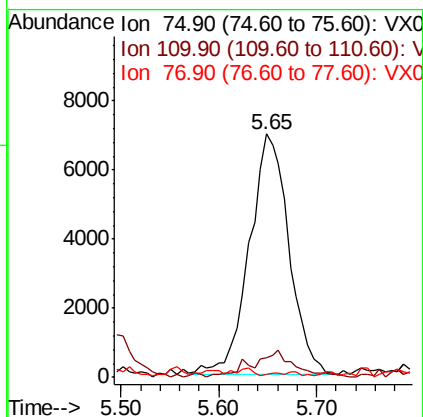

#38
 Carbon Tetrachloride
 Concen: 6.120 ug/l
 RT: 5.66 min Scan# 783
 Delta R.T. -0.12 min
 Lab File: VX015247.D
 Acq: 13 Mar 2020 10:26

Tgt Ion	Ratio	Lower	Upper
117	100		
119	5.8	76.9	115.3#
121	0.0	24.6	37.0#

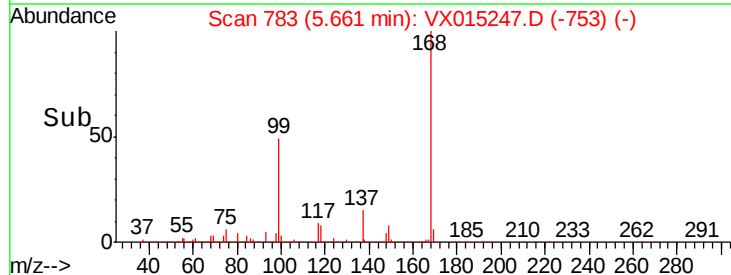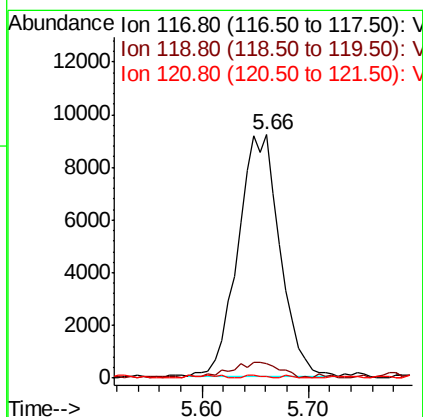

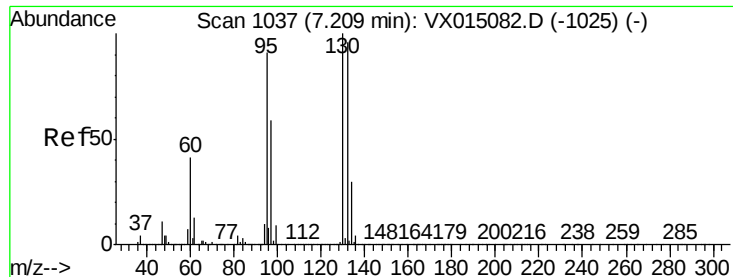

#44

Trichloroethene

Concen: 0.240 ug/l

RT: 7.21 min Scan# 1037

Delta R.T. 0.00 min

Lab File: VX015247.D

Acq: 13 Mar 2020 10:26

Instrument :

MSVOA_X

ClientSampleId :


TB-20200307

Tot Ion:130 Resp: 871

Ion Ratio Lower Upper

130 100

95 31.4 0.0 181.2

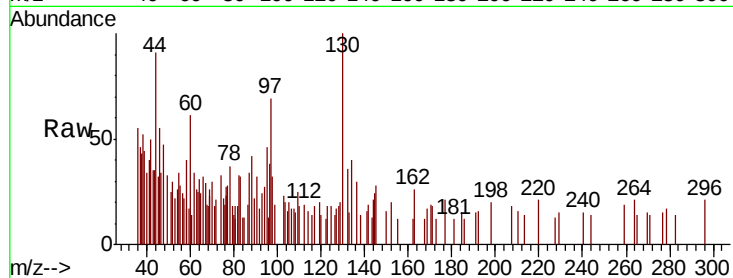

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

7.21

400

300



200

100

0

7.15 7.20 7.25

Time-->

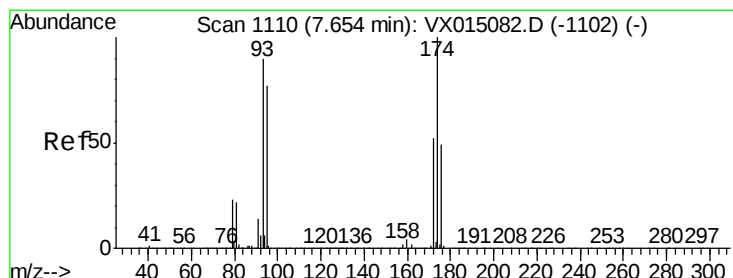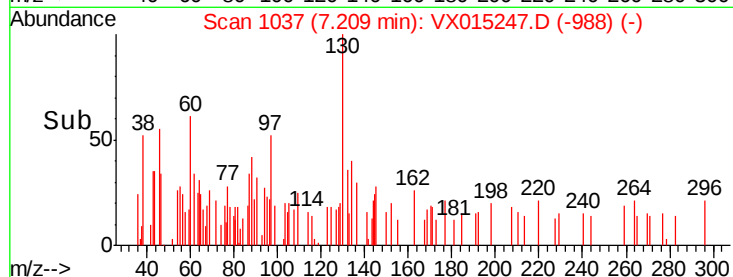

#46

Dibromomethane

Concen: 0.301 ug/l

RT: 7.66 min Scan# 1111

Delta R.T. 0.01 min

Lab File: VX015247.D

Acq: 13 Mar 2020 10:26


Tgt Ion: 93 Resp: 662

Ion Ratio Lower Upper

93 100

95 88.8 67.8 101.8

174 52.0 91.0 136.4#

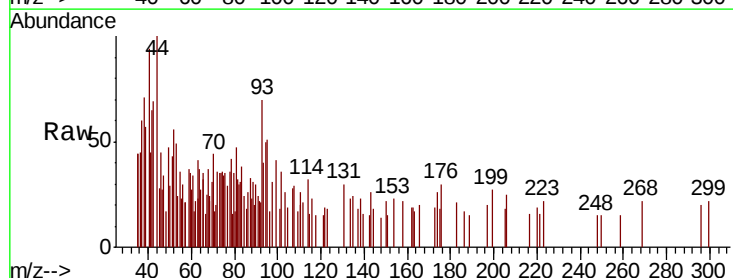

Abundance Ion 92.80 (92.50 to 93.50): VX0

Ion 94.80 (94.50 to 95.50): VX0

Ion 173.70 (173.40 to 174.40): V

7.66

400

300


200


100

0

7.60 7.65 7.70

Time-->




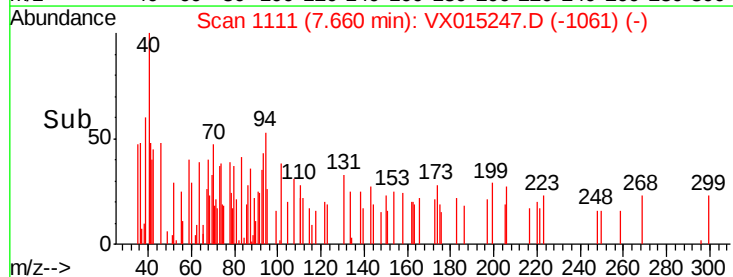


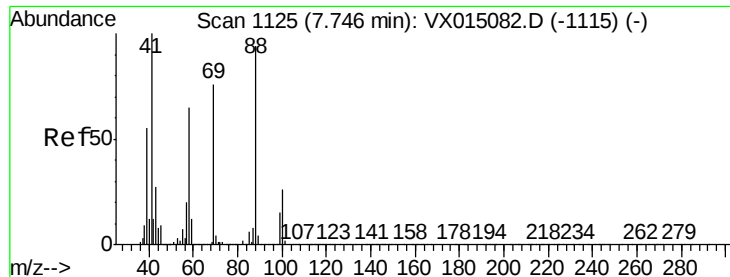

#49
1,4-Dioxane
Concen: 3.999 ug/l
RT: 7.74 min Scan# 1124
Delta R.T. -0.01 min
Lab File: VX015247.D
Acq: 13 Mar 2020 10:26




Instrument :
MSVOA_X
ClientSampleId :
TB-20200307


Tot Ion: 88 Resp: 316
Ion Ratio Lower Upper
88 100
43 78.2 27.0 40.4#
58 38.9 55.6 83.4#

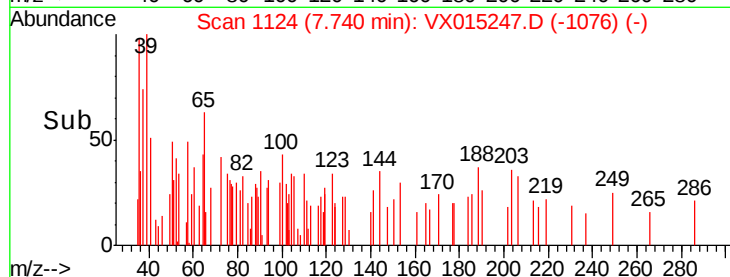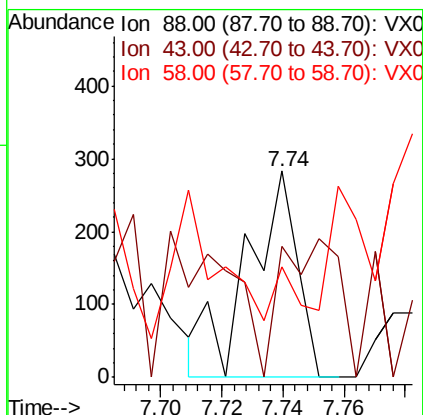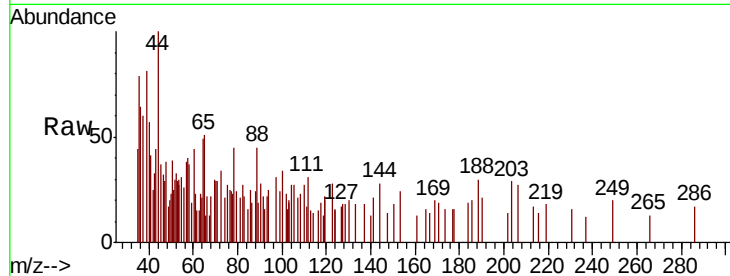

#50
Toluene-d8
Concen: 50.712 ug/l
RT: 8.71 min Scan# 1283
Delta R.T. 0.00 min
Lab File: VX015247.D
Acq: 13 Mar 2020 10:26

Tgt Ion: 98 Resp: 579309
Ion Ratio Lower Upper
98 100
100 65.2 52.4 78.6

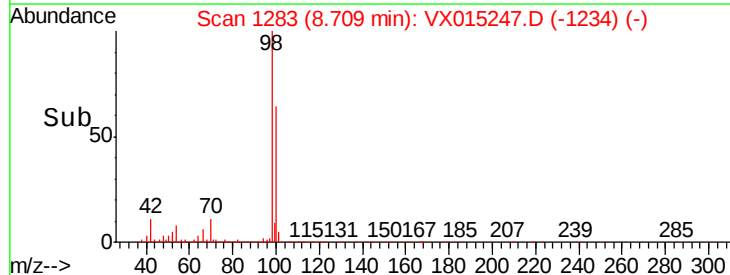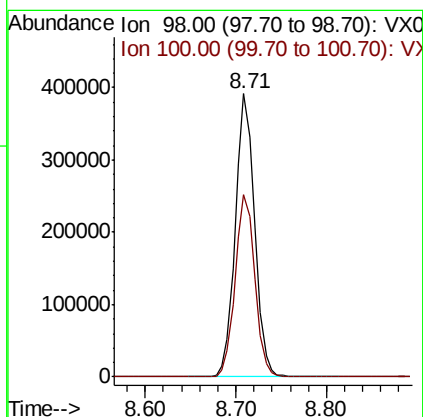

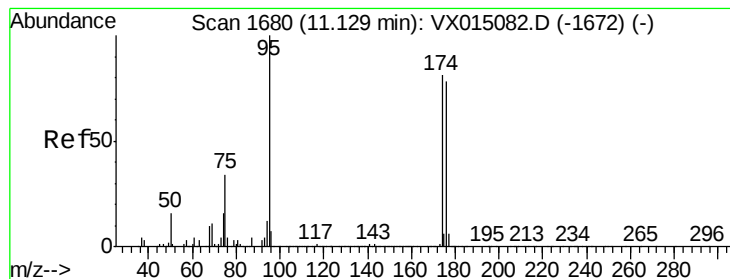

#62

4-Bromofluorobenzene

Concen: 51.328 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. 0.00 min

Lab File: VX015247.D

Acq: 13 Mar 2020 10:26

Instrument :

MSVOA_X

ClientSampleId :

TB-20200307


Tot Ion: 95 Resp: 209141

Ion Ratio Lower Upper

95 100

174 91.5 0.0 177.6

176 85.6 0.0 170.2




Abundance Ion 94.90 (94.60 to 95.60): VX015082.D (-1672) (-)

Ion 173.80 (173.50 to 174.50): VX015082.D (-1672) (-)

Ion 175.80 (175.50 to 176.50): VX015082.D (-1672) (-)

Time-->

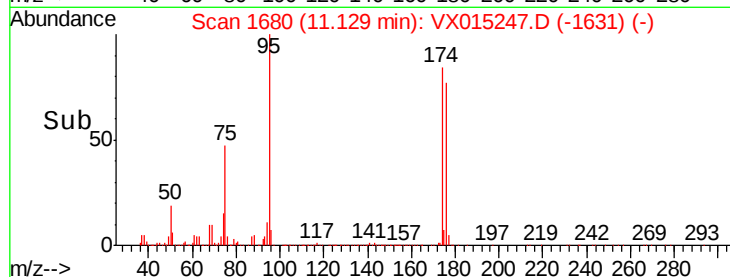


Abundance Ion 94.90 (94.60 to 95.60): VX015247.D (-1631) (-)

Ion 173.80 (173.50 to 174.50): VX015247.D (-1631) (-)

Ion 175.80 (175.50 to 176.50): VX015247.D (-1631) (-)

Time-->

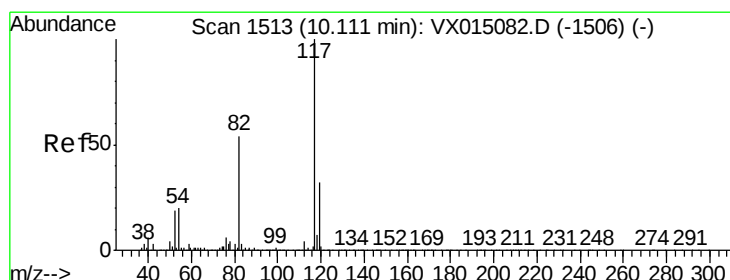

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1513

Delta R.T. 0.00 min

Lab File: VX015247.D

Acq: 13 Mar 2020 10:26


Tgt Ion: 117 Resp: 450716

Ion Ratio Lower Upper

117 100

82 54.5 43.3 64.9

119 33.3 25.8 38.8




Abundance Ion 116.90 (116.60 to 117.60): VX015082.D (-1506) (-)

Ion 82.00 (81.70 to 82.70): VX015082.D (-1506) (-)

Ion 118.90 (118.60 to 119.60): VX015082.D (-1506) (-)

Time-->

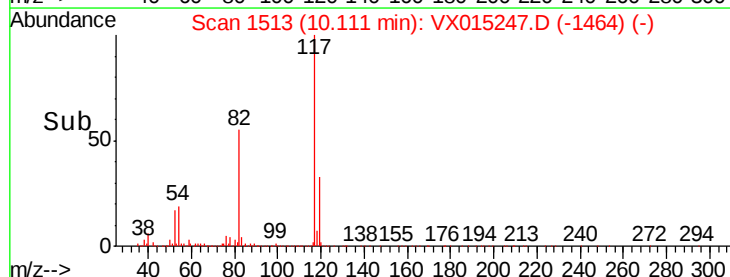


Abundance Ion 116.90 (116.60 to 117.60): VX015247.D (-1464) (-)

Ion 82.00 (81.70 to 82.70): VX015247.D (-1464) (-)

Ion 118.90 (118.60 to 119.60): VX015247.D (-1464) (-)

Time-->



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.07 min Scan# 1835

Delta R.T. 0.00 min

Lab File: VX015247.D

Acq: 13 Mar 2020 10:26

Instrument :

MSVOA_X

ClientSampleId :

TB-20200307


Tot Ion:152 Resp: 224980

Ion Ratio Lower Upper

152 100

115 56.0 38.2 114.6




150 157.4 0.0 343.8

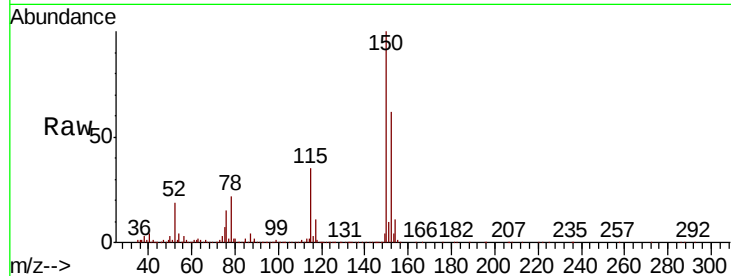

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

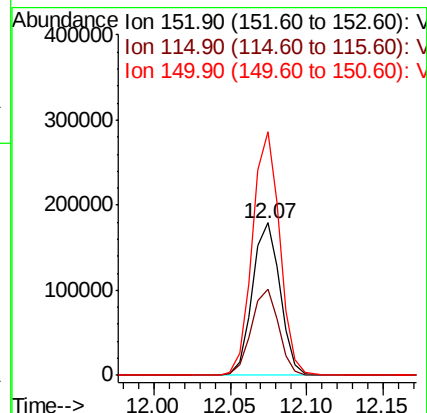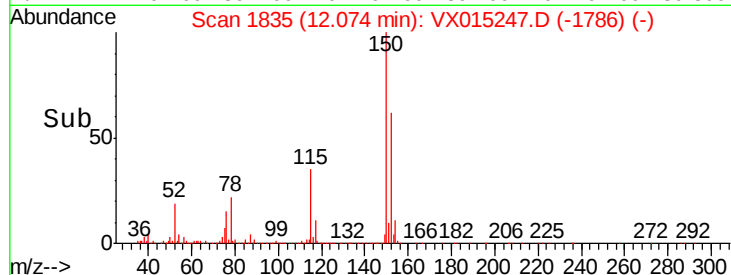

#76

1,2,3-Trichloropropane

Concen: 22.065 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.16 min

Lab File: VX015247.D


Acq: 13 Mar 2020 10:26

Tgt Ion: 75 Resp: 99019

Ion Ratio Lower Upper



75 100


77 1.6 22.6 67.8#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

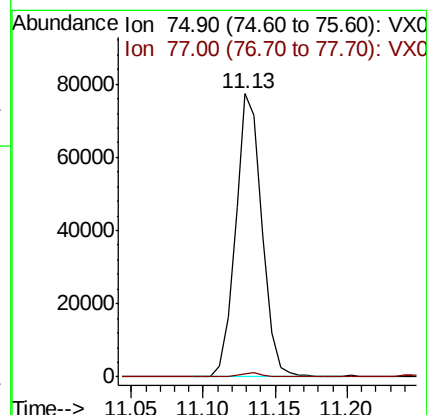

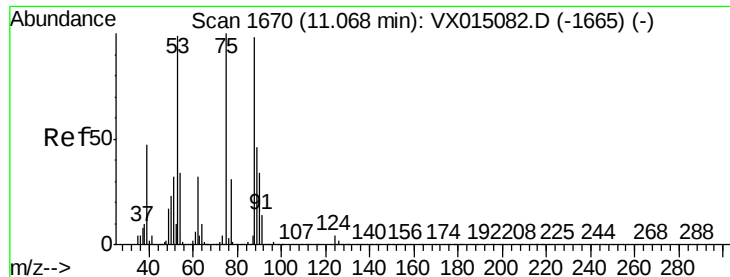

#81

trans-1,4-Dichloro-2-butene

Concen: 62.620 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. 0.06 min

Lab File: VX015247.D

Acq: 13 Mar 2020 10:26

Instrument :

MSVOA_X

ClientSampled :

TB-20200307


Tot Ion: 75 Resp: 99019

Ion Ratio Lower Upper

75 100

53 0.0 77.9 116.9#

89 0.0 36.2 54.2#



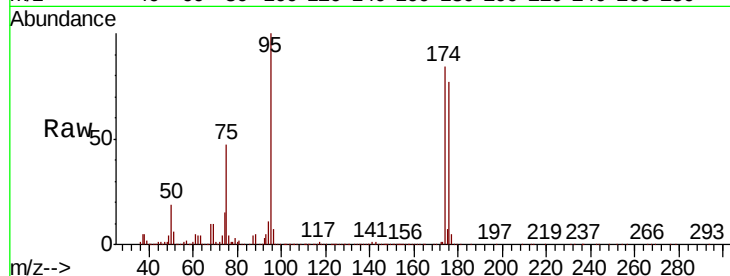


Abundance

Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

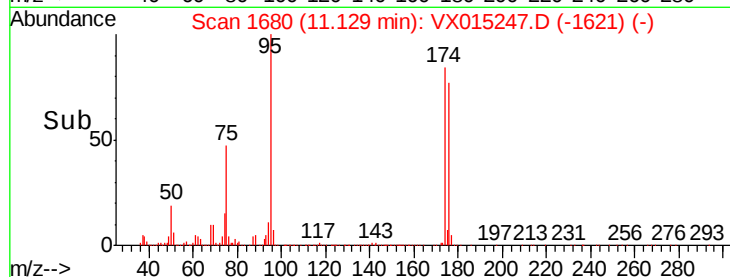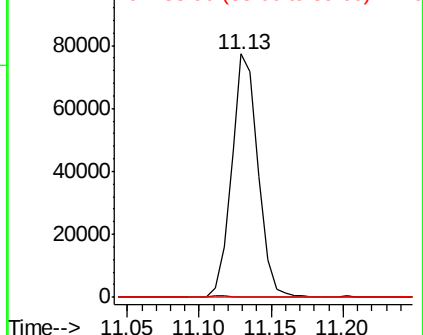

#87

1,3-Dichlorobenzene

Concen: 0.247 ug/l

RT: 12.03 min Scan# 1828

Delta R.T. 0.01 min

Lab File: VX015247.D

Acq: 13 Mar 2020 10:26


Tgt Ion: 146 Resp: 1737

Ion Ratio Lower Upper

146 100

111 40.1 19.1 57.1

148 55.1 31.9 95.5






Abundance

Ion 145.90 (145.60 to 146.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 147.90 (147.60 to 148.60): V



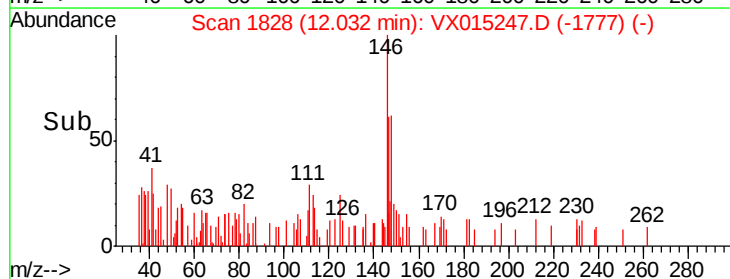
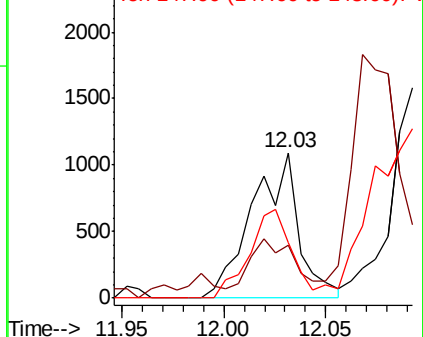


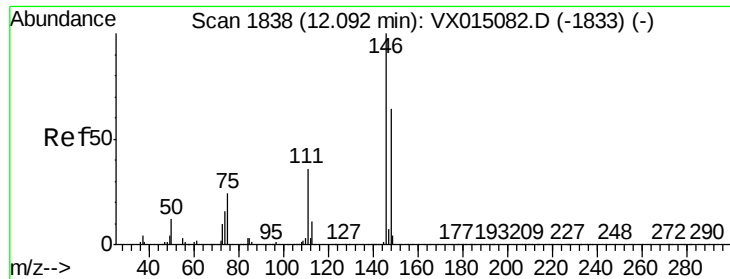

#88
 1,4-Dichlorobenzene
 Concen: 0.239 ug/l
 RT: 12.03 min Scan# 1828
 Delta R.T. -0.06 min
 Lab File: VX015247.D
 Acq: 13 Mar 2020 10:26




Instrument :
 MSVOA_X
 ClientSampleID :
 TB-20200307


Tot Ion:146 Resp: 1737
 Ion Ratio Lower Upper
 146 100
 111 40.1 18.7 56.1
 148 55.1 32.5 97.4

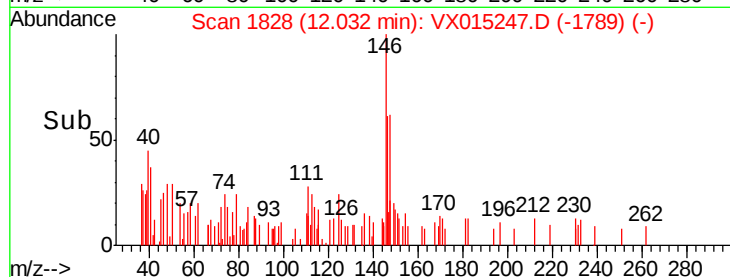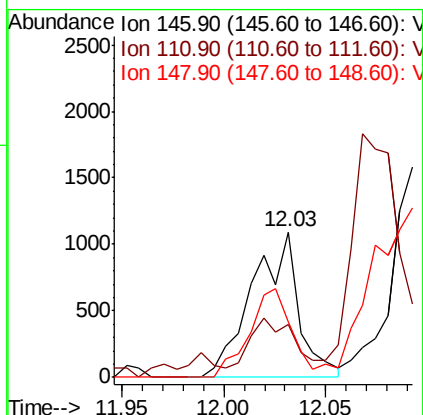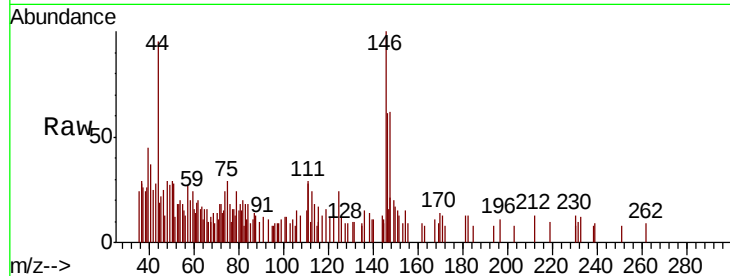

#89
 n-Butylbenzene
 Concen: 0.209 ug/l
 RT: 12.39 min Scan# 1886
 Delta R.T. 0.00 min
 Lab File: VX015247.D
 Acq: 13 Mar 2020 10:26

Tgt Ion: 91 Resp: 2391
 Ion Ratio Lower Upper
 91 100
 92 75.4 27.2 81.6
 134 39.2 13.5 40.5

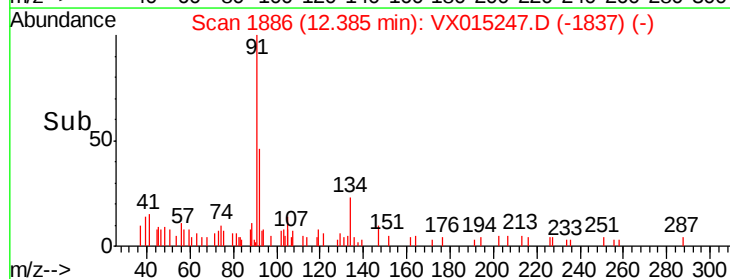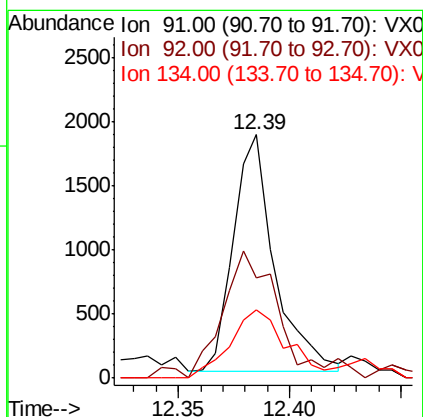







#93
 1,2,4-Trichlorobenzene
 Concen: 0.402 ug/l
 RT: 13.64 min Scan# 2092
 Delta R.T. 0.00 min
 Lab File: VX015247.D
 Acq: 13 Mar 2020 10:26

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-20200307

Tot Ion:180 Resp: 1953
 Ion Ratio Lower Upper
 180 100
 182 107.4 47.6 142.8
 145 40.4 14.1 42.2

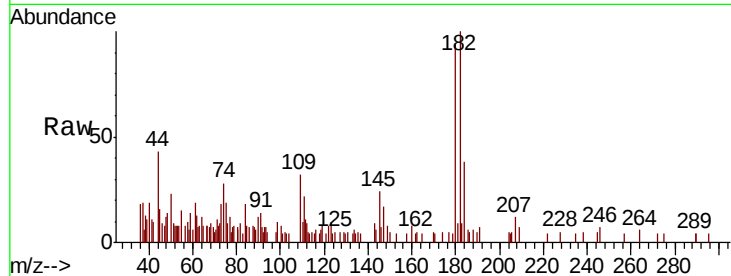


Abundance Ion 179.80 (179.50 to 180.50): V
 Ion 181.80 (181.50 to 182.50): V
 Ion 144.80 (144.50 to 145.50): V

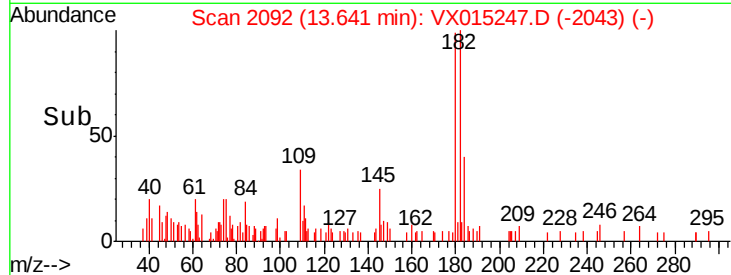
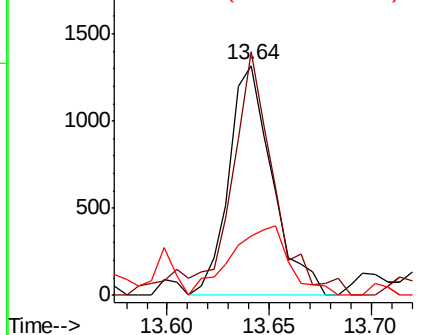



#94
 Hexachlorobutadiene
 Concen: 0.426 ug/l
 RT: 13.78 min Scan# 2114
 Delta R.T. 0.00 min
 Lab File: VX015247.D
 Acq: 13 Mar 2020 10:26

Tgt Ion:225 Resp: 1063
 Ion Ratio Lower Upper
 225 100
 223 44.7 31.3 93.9
 227 42.8 31.1 93.2



Abundance Ion 224.70 (224.40 to 225.40): V
 Ion 222.70 (222.40 to 223.40): V
 Ion 226.70 (226.40 to 227.40): V

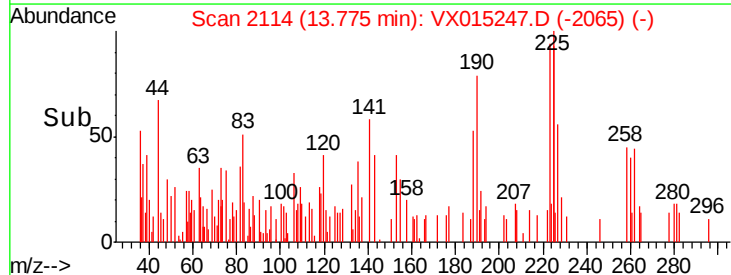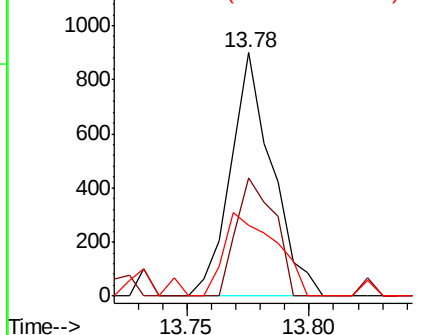

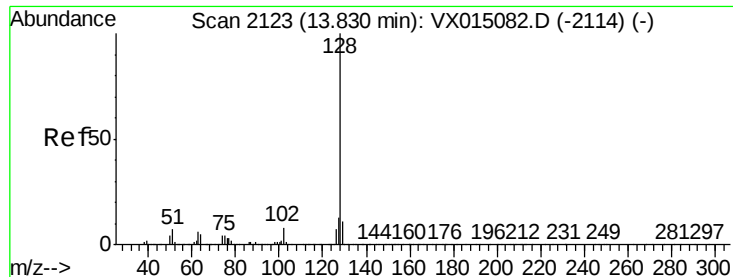

#95

Naphthalene

Concen: 1.661 ug/l

RT: 13.83 min Scan# 2123

Delta R.T. 0.00 min

Lab File: VX015247.D

Acq: 13 Mar 2020 10:26

Instrument :

MSVOA_X

ClientSampleId :

TB-20200307


Tot Ion:128 Resp: 3692

Ion Ratio Lower Upper

128 100

127 16.7 10.3 15.5#




129 15.1 8.6 13.0#

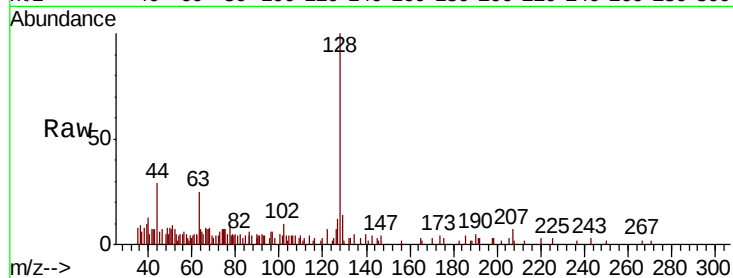

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

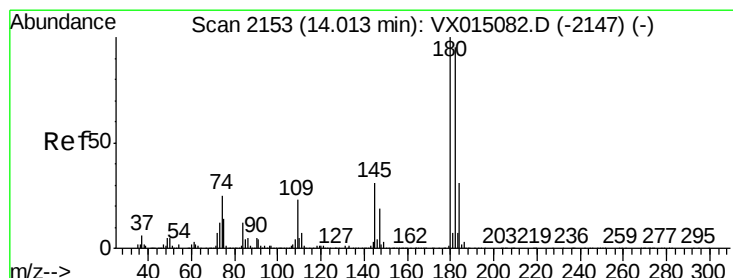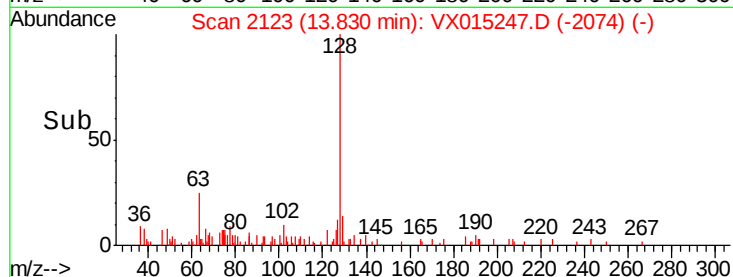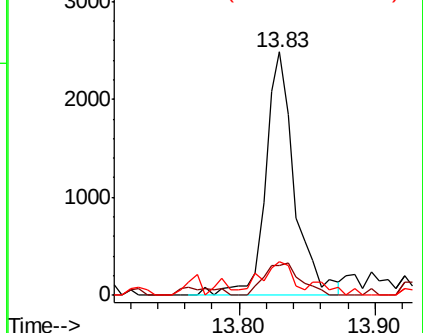

#96

1,2,3-Trichlorobenzene

Concen: 0.291 ug/l

RT: 14.01 min Scan# 2153

Delta R.T. 0.00 min

Lab File: VX015247.D

Acq: 13 Mar 2020 10:26


Tgt Ion:180 Resp: 1409

Ion Ratio Lower Upper

180 100

182 89.1 47.8 143.4

145 42.2 15.1 45.3

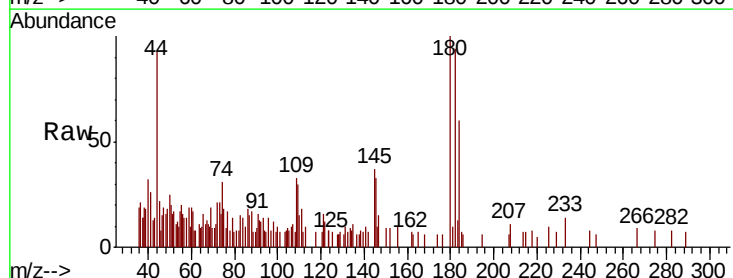

Abundance Ion 179.80 (179.50 to 180.50): V

Ion 181.80 (181.50 to 182.50): V

Ion 144.90 (144.60 to 145.60): V

