


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX031320\
 Data File : VX015272.D
 Acq On : 13 Mar 2020 20:37
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X030420W.M
 Title : SW846 8260
 Last Update : Wed Mar 04 14:19:10 2020

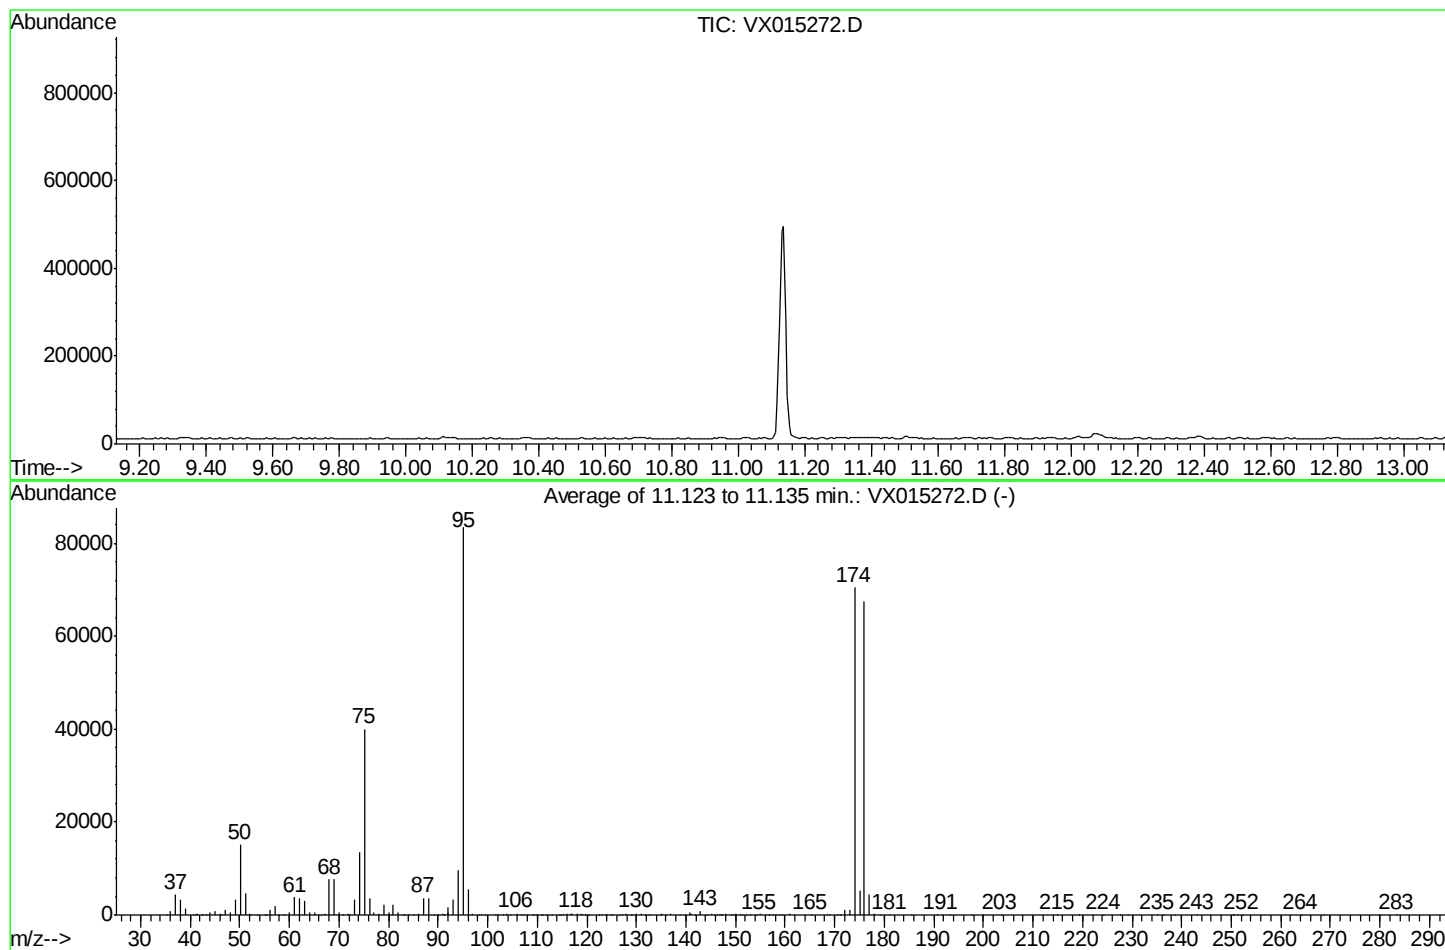

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1671

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	15146	PASS
75	95	30	60	48.0	40090	PASS
95	95	100	100	100.0	83486	PASS
96	95	5	9	6.5	5408	PASS
173	174	0.00	2	1.6	1153	PASS
174	95	50	100	84.5	70504	PASS
175	174	5	9	7.5	5296	PASS
176	174	95	101	95.7	67445	PASS
177	176	5	9	6.7	4493	PASS