

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
 Data File : VX034423.D
 Acq On : 13 Mar 2023 10:55
 Operator : JC/MD
 Sample : VX0313MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0313MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034423.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	36	rBV	21041	45999	2.79%	0.528%
2	1.557	71	77	84	rBV6	9257	19062	1.16%	0.219%
3	4.556	558	569	581	rBV2	6879	23330	1.41%	0.268%
4	5.379	692	704	719	rBV	185088	540598	32.77%	6.206%
5	5.544	720	731	746	rVB	319064	884660	53.62%	10.155%
6	5.952	785	798	814	rBV2	205128	553849	33.57%	6.358%
7	6.757	920	930	950	rBV	489981	1196318	72.51%	13.733%
8	8.647	1233	1240	1249	rBV	1055312	1649754	100.00%	18.938%
9	10.049	1465	1470	1481	rBV	1000238	1407412	85.31%	16.156%
10	11.079	1634	1639	1650	rBV	869296	1076283	65.24%	12.355%
11	12.018	1788	1793	1804	rBV	1001880	1314107	79.65%	15.085%




Sum of corrected areas: 8711372

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034423.D
Acq On : 13 Mar 2023 10:55
Operator : JC/MD
Sample : VX0313MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0313MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

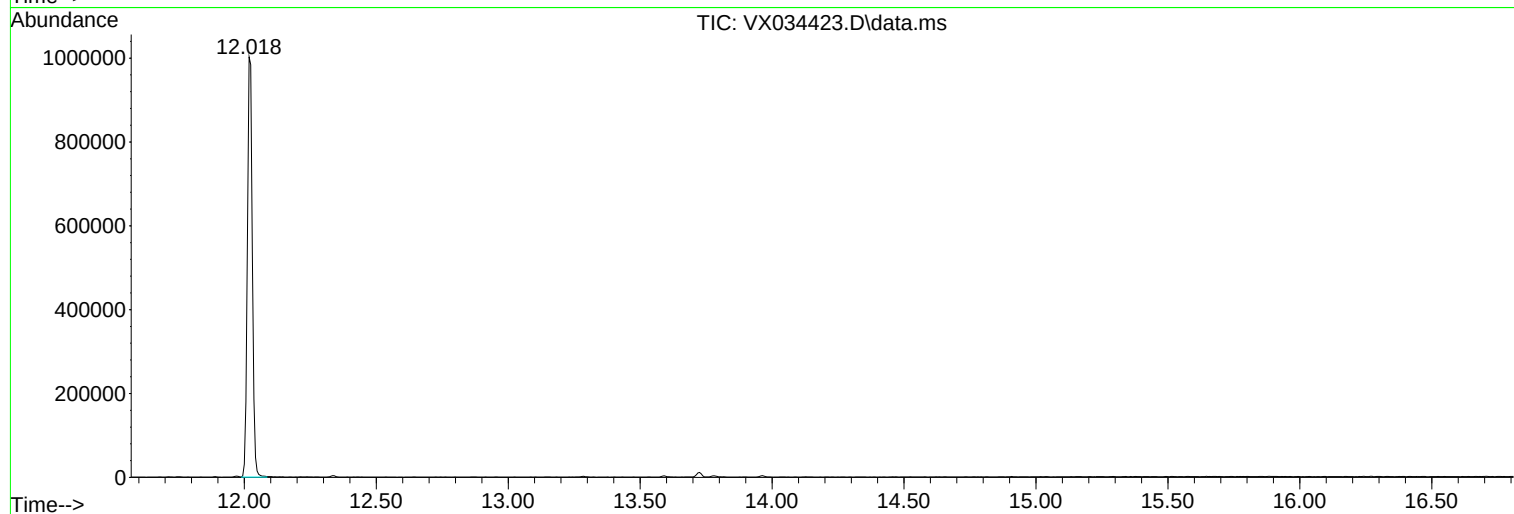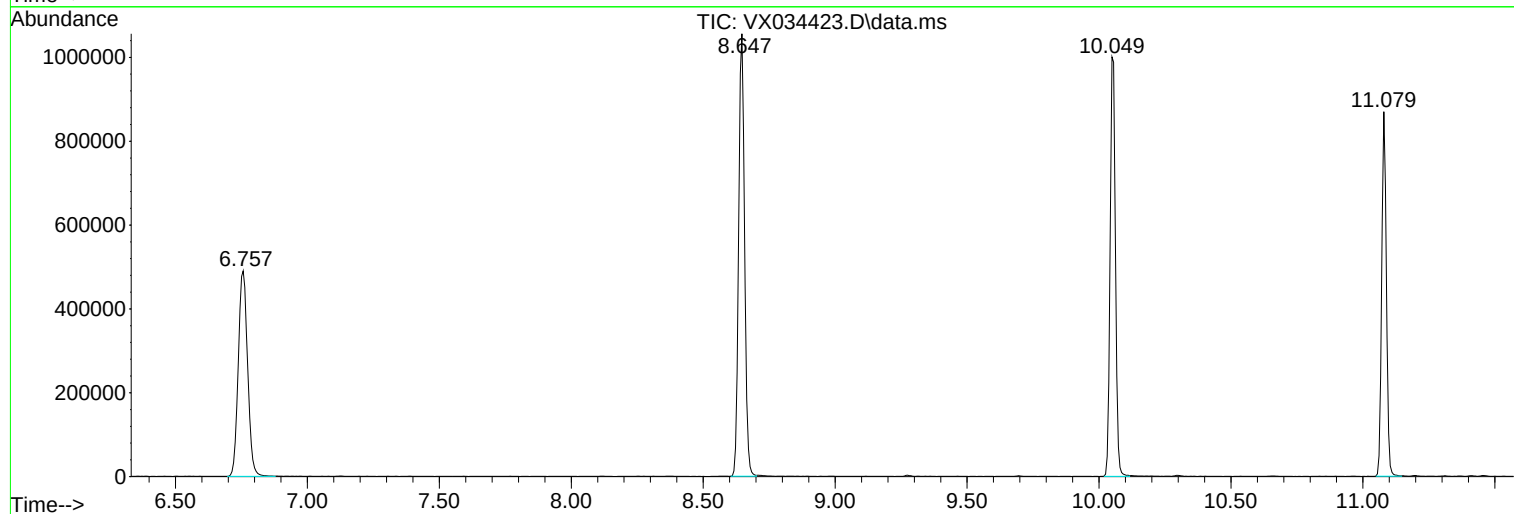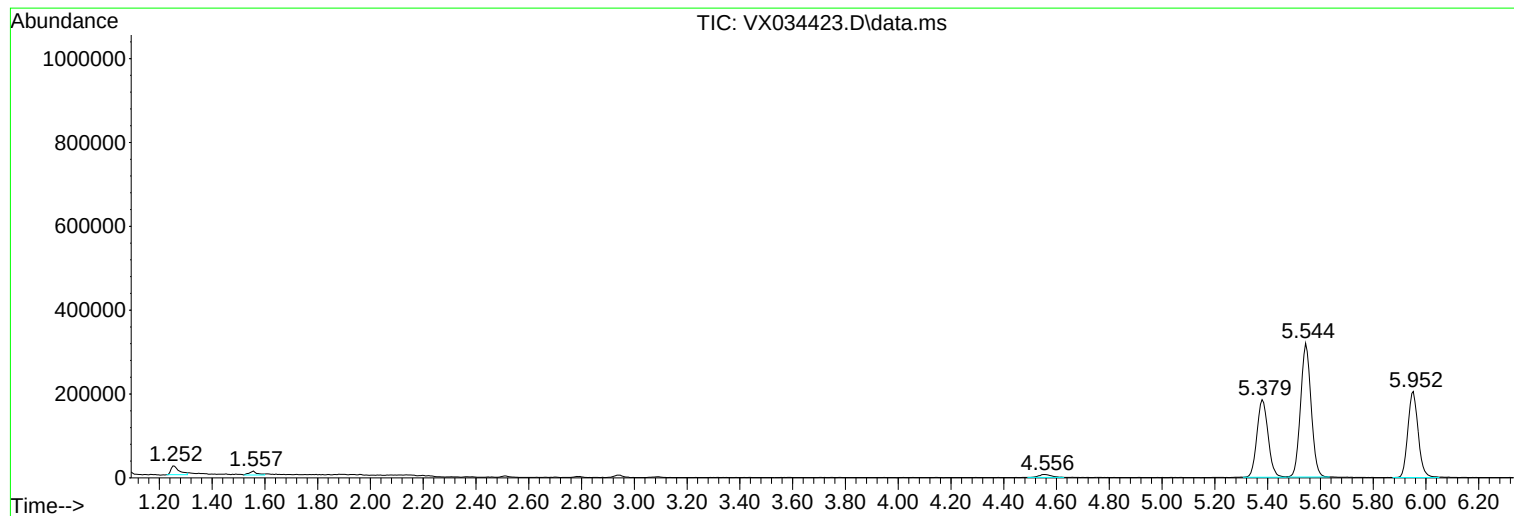

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034423.D
Acq On : 13 Mar 2023 10:55
Operator : JC/MD
Sample : VX0313MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0313MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034423.D
Acq On : 13 Mar 2023 10:55
Operator : JC/MD
Sample : VX0313MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0313MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc