

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
 Data File : VX034427.D
 Acq On : 13 Mar 2023 13:03
 Operator : JC/MD
 Sample : 01879-10 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP03-20230308

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
 Title : SW846 8260

Signal : TIC: VX034427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	37	rBV	34436	69648	1.93%	0.608%
2	4.556	563	569	586	rVB2	11310	39647	1.10%	0.346%
3	5.385	692	705	720	rBV	173793	496331	13.73%	4.333%
4	5.550	720	732	749	rVB	290559	820420	22.69%	7.162%
5	5.952	789	798	813	rBV2	188352	511243	14.14%	4.463%
6	6.763	918	931	947	rBV	458016	1105878	30.58%	9.654%
7	7.123	979	990	1012	rBV	1665966	3616067	100.00%	31.568%
8	8.647	1233	1240	1252	rBV	992156	1527941	42.25%	13.339%
9	10.055	1465	1471	1487	rBV	918550	1261382	34.88%	11.012%
10	11.079	1634	1639	1651	rBV	753629	930444	25.73%	8.123%
11	12.018	1788	1793	1810	rBV	825185	1075976	29.76%	9.393%




Sum of corrected areas: 11454977

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034427.D
Acq On : 13 Mar 2023 13:03
Operator : JC/MD
Sample : 01879-10 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP03-20230308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

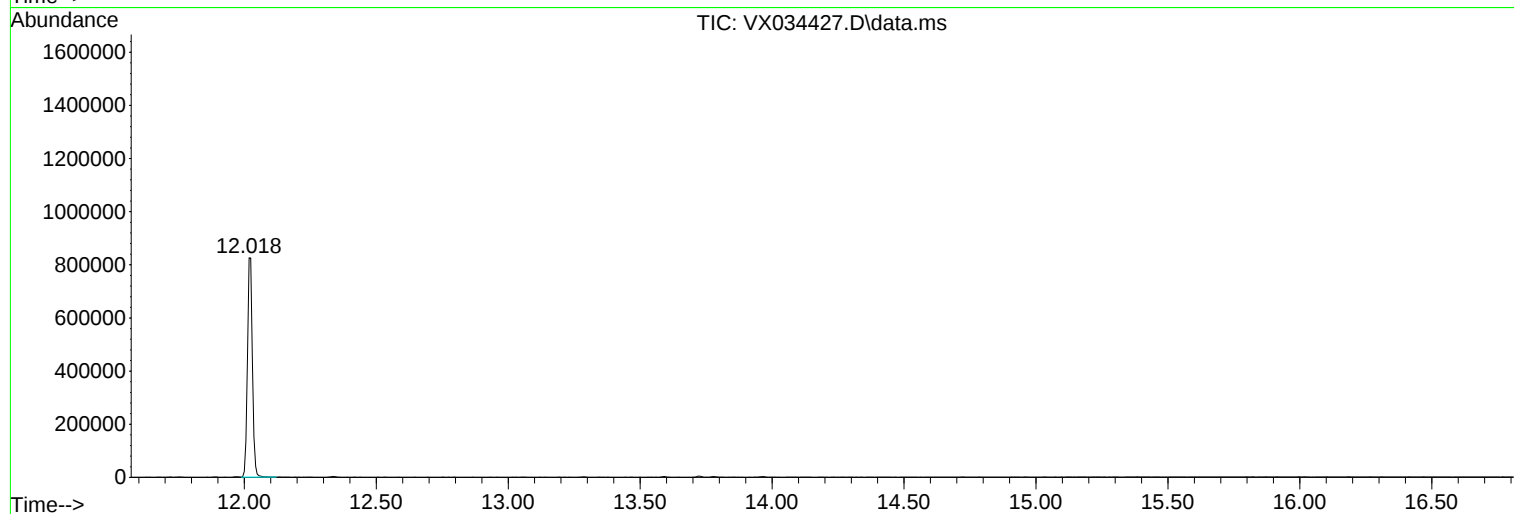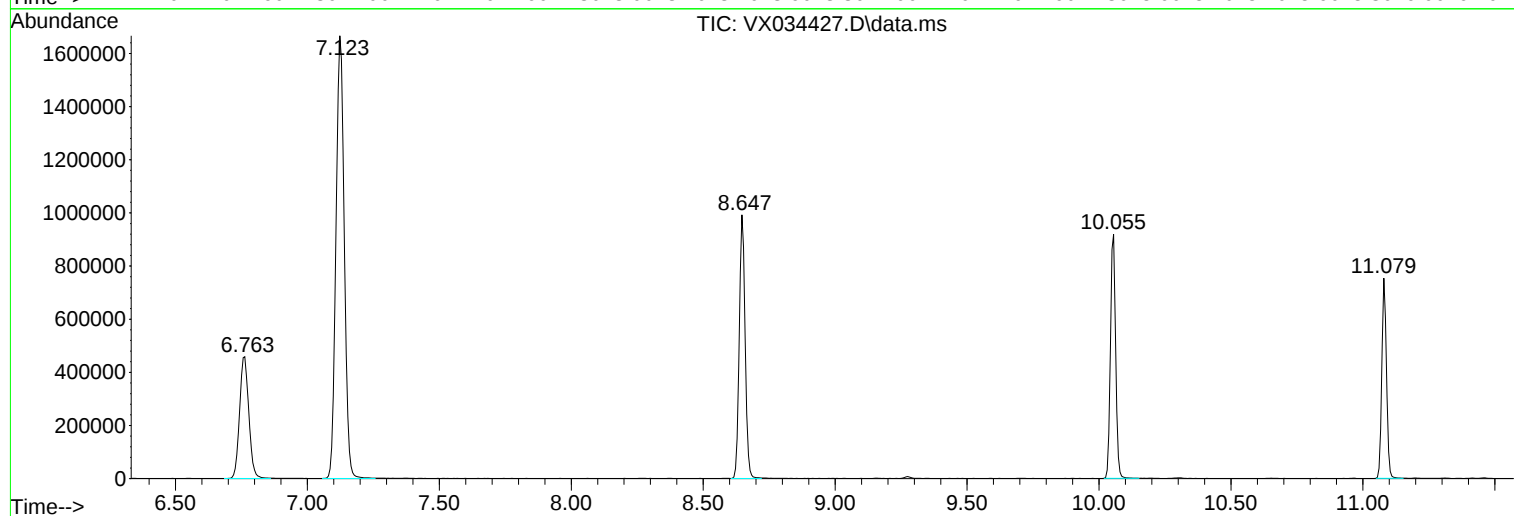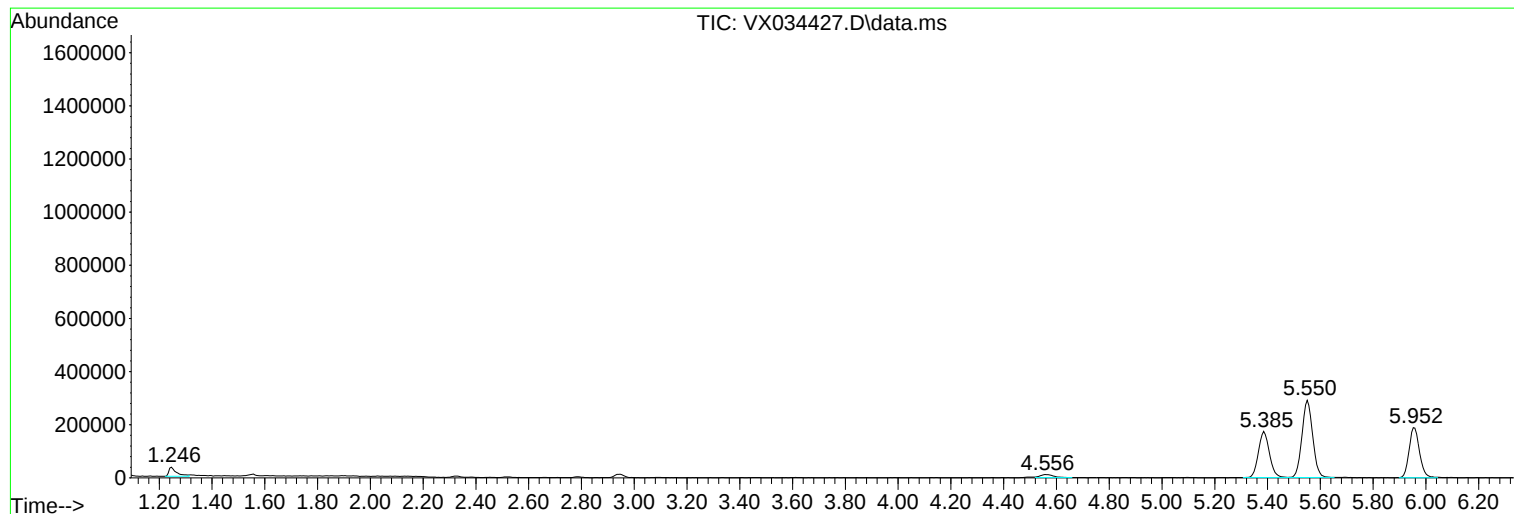

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034427.D
Acq On : 13 Mar 2023 13:03
Operator : JC/MD
Sample : 01879-10 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP03-20230308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034427.D
Acq On : 13 Mar 2023 13:03
Operator : JC/MD
Sample : 01879-10 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP03-20230308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------