

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
 Data File : VX034428.D
 Acq On : 13 Mar 2023 13:27
 Operator : JC/MD
 Sample : 01879-14 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP02-20230308

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034428.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	36	rBV	37419	69766	4.68%	0.906%
2	2.947	297	305	311	rBV	10266	21828	1.46%	0.284%
3	4.568	560	571	583	rBV2	8967	30368	2.04%	0.395%
4	5.385	691	705	721	rBV2	167699	489919	32.83%	6.366%
5	5.550	721	732	747	rVB	291079	810321	54.31%	10.529%
6	5.952	788	798	814	rBV	187406	506523	33.95%	6.581%
7	6.763	918	931	948	rBV	446826	1090238	73.07%	14.166%
8	8.647	1233	1240	1252	rBV	957295	1492124	100.00%	19.388%
9	10.055	1465	1471	1486	rBV	901035	1233565	82.67%	16.028%
10	11.079	1634	1639	1652	rBV	734935	911271	61.07%	11.840%
11	12.024	1788	1794	1804	rBV	797638	1040348	69.72%	13.518%




Sum of corrected areas: 7696271

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034428.D
Acq On : 13 Mar 2023 13:27
Operator : JC/MD
Sample : 01879-14 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20230308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

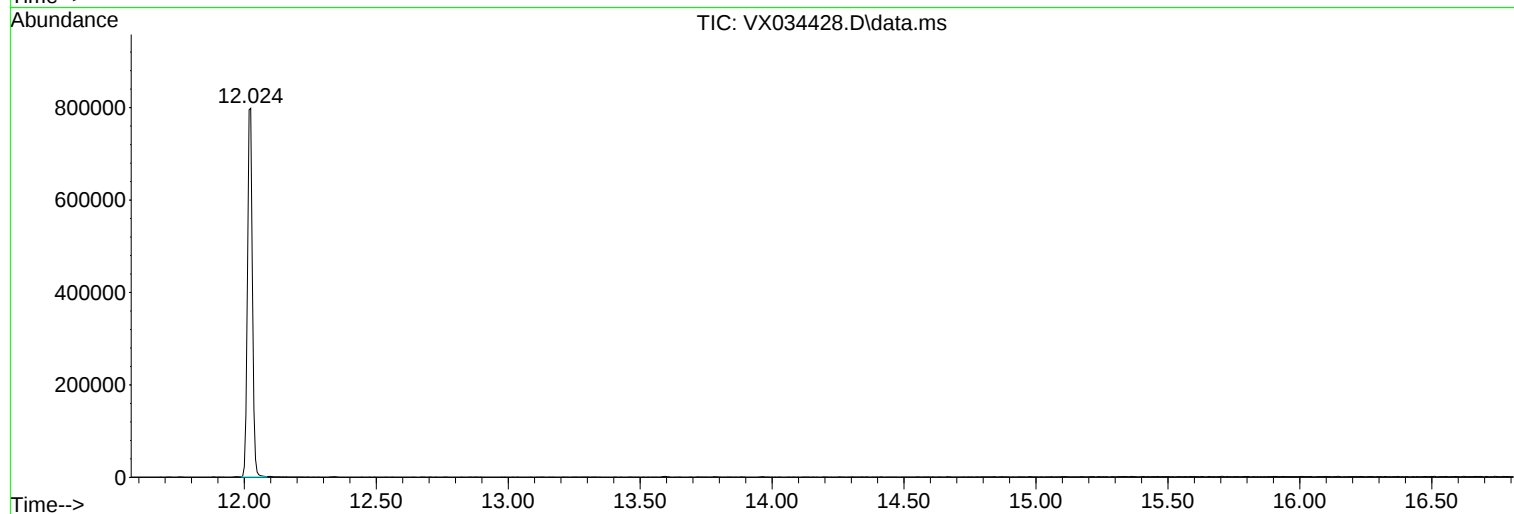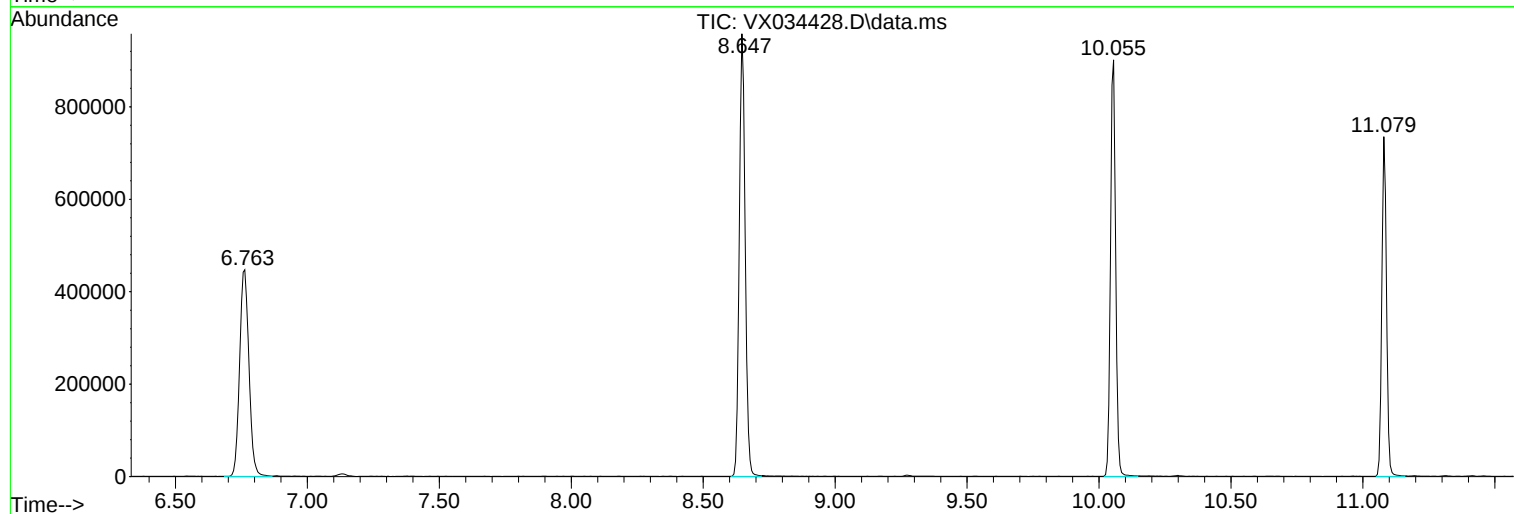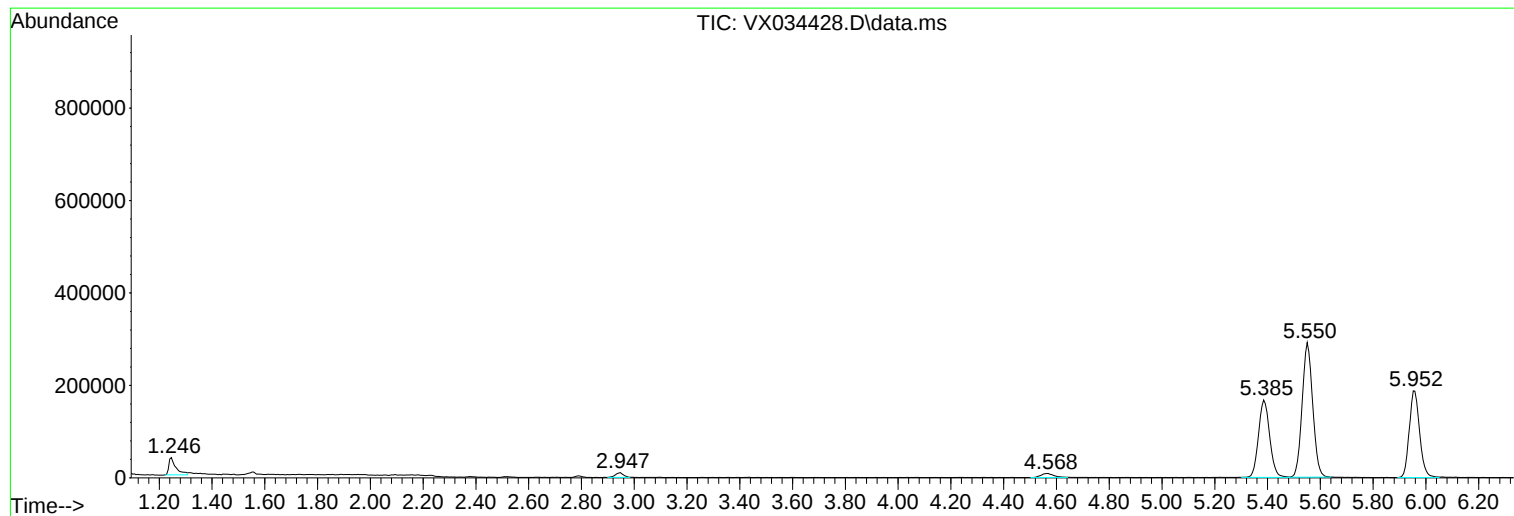

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034428.D
Acq On : 13 Mar 2023 13:27
Operator : JC/MD
Sample : 01879-14 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20230308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034428.D
Acq On : 13 Mar 2023 13:27
Operator : JC/MD
Sample : 01879-14 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20230308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------