

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
 Data File : VX034432.D
 Acq On : 13 Mar 2023 15:01
 Operator : JC/MD
 Sample : 01879-09 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE108D2-20230308

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034432.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	39	rBV	39711	80302	2.46%	0.745%
2	4.562	560	570	590	rVB	9806	33005	1.01%	0.306%
3	5.385	692	705	720	rBV2	161764	474497	14.51%	4.402%
4	5.550	721	732	748	rVB	271654	774612	23.69%	7.187%
5	5.958	787	799	818	rBV	182381	495814	15.16%	4.600%
6	6.763	919	931	947	rBV	435887	1053938	32.23%	9.778%
7	7.123	980	990	1007	rBV	1518887	3270004	100.00%	30.338%
8	8.647	1233	1240	1251	rBV	941562	1449780	44.34%	13.451%
9	10.055	1465	1471	1485	rBV	880776	1210200	37.01%	11.228%
10	11.079	1634	1639	1653	rBV	693131	892103	27.28%	8.277%
11	12.024	1788	1794	1808	rBV	800290	1044257	31.93%	9.688%




Sum of corrected areas: 10778512

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034432.D
Acq On : 13 Mar 2023 15:01
Operator : JC/MD
Sample : 01879-09 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE108D2-20230308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

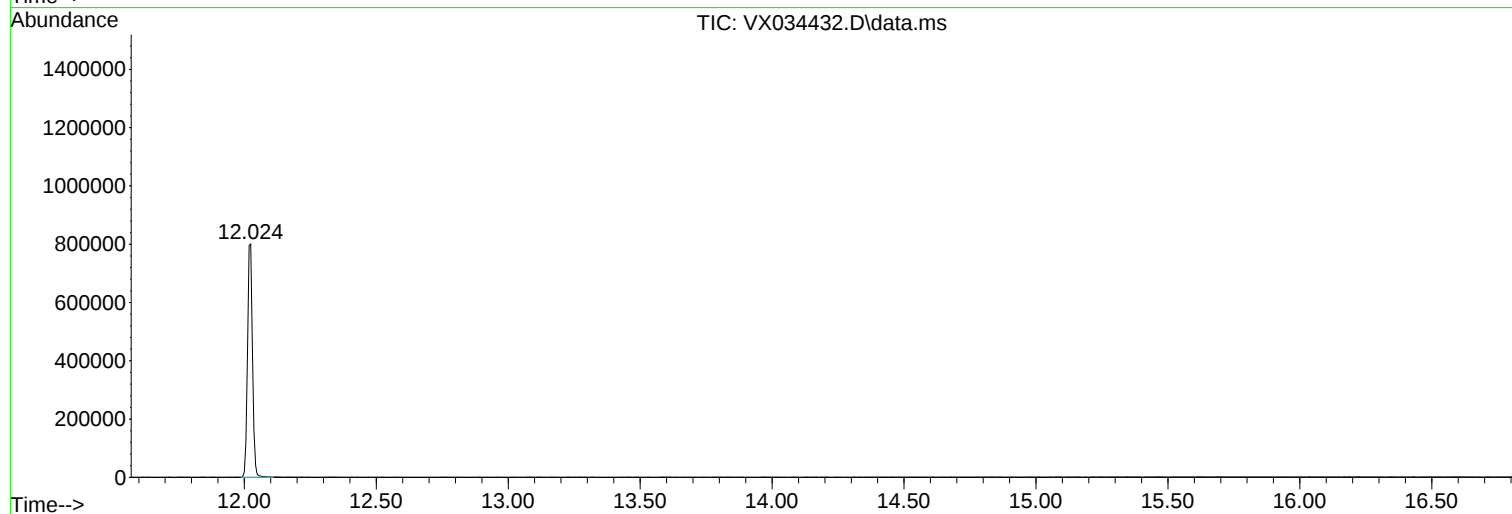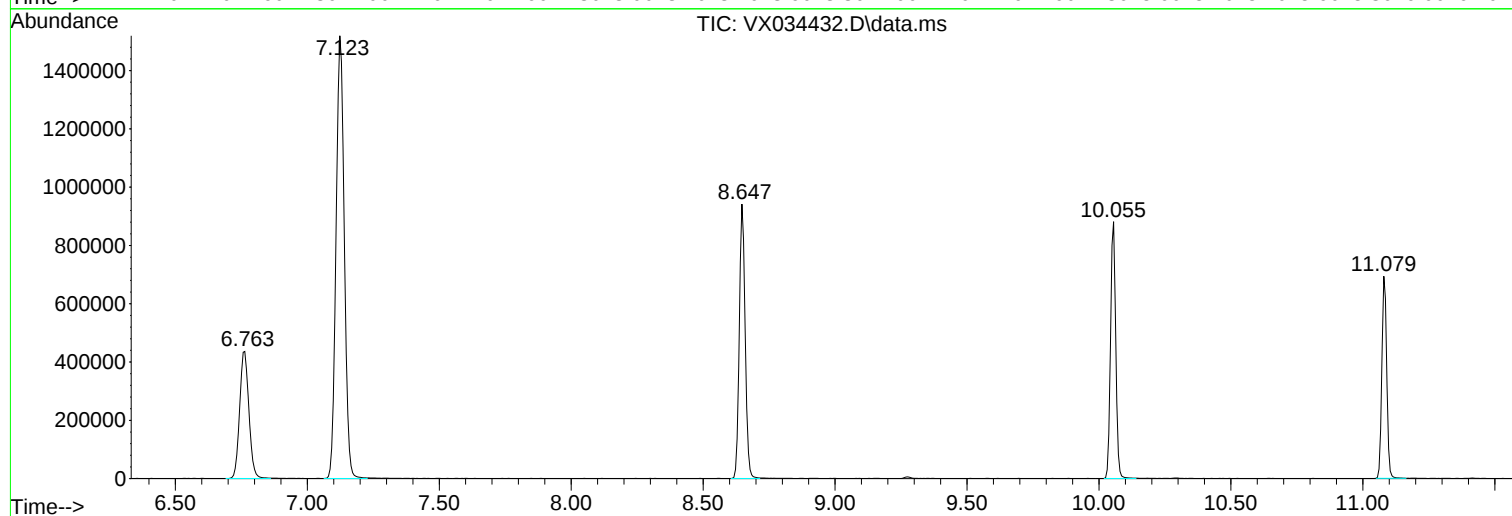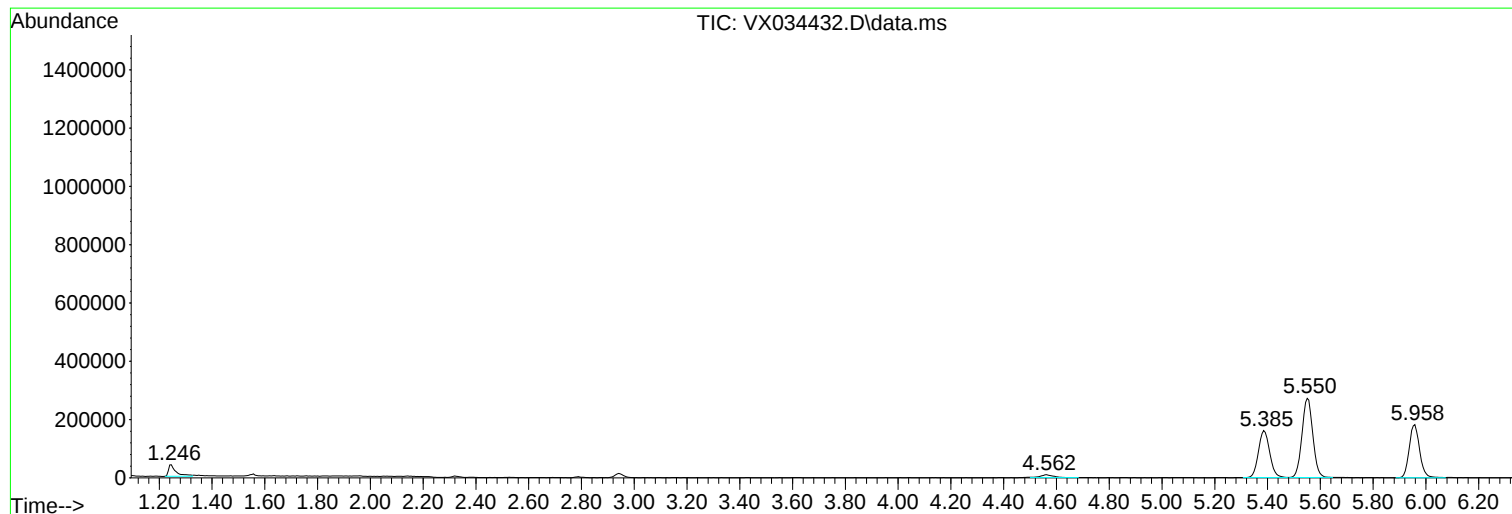

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034432.D
Acq On : 13 Mar 2023 15:01
Operator : JC/MD
Sample : 01879-09 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE108D2-20230308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034432.D
Acq On : 13 Mar 2023 15:01
Operator : JC/MD
Sample : 01879-09 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE108D2-20230308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc