

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
 Data File : VX034436.D
 Acq On : 13 Mar 2023 16:35
 Operator : JC/MD
 Sample : 01879-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D3-20230308

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	40	rBV	120602	181067	12.53%	2.368%
2	1.557	72	77	84	rBV	7966	15512	1.07%	0.203%
3	5.385	693	705	721	rBV2	162394	469861	32.51%	6.146%
4	5.550	721	732	747	rVB	268795	767642	53.12%	10.041%
5	5.952	787	798	818	rBV	182357	493770	34.17%	6.458%
6	6.763	921	931	948	rBV	431929	1044442	72.27%	13.661%
7	7.129	984	991	1007	rVB3	15959	38563	2.67%	0.504%
8	8.647	1233	1240	1257	rBV	926572	1445234	100.00%	18.904%
9	10.055	1465	1471	1483	rBV	874618	1200338	83.05%	15.700%
10	11.079	1634	1639	1652	rBV	761953	962210	66.58%	12.586%
11	12.024	1788	1794	1800	rBV	778359	1012182	70.04%	13.239%
12	15.115	2297	2301	2305	rBV2	9489	14454	1.00%	0.189%




Sum of corrected areas: 7645275

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034436.D
Acq On : 13 Mar 2023 16:35
Operator : JC/MD
Sample : 01879-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D3-20230308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

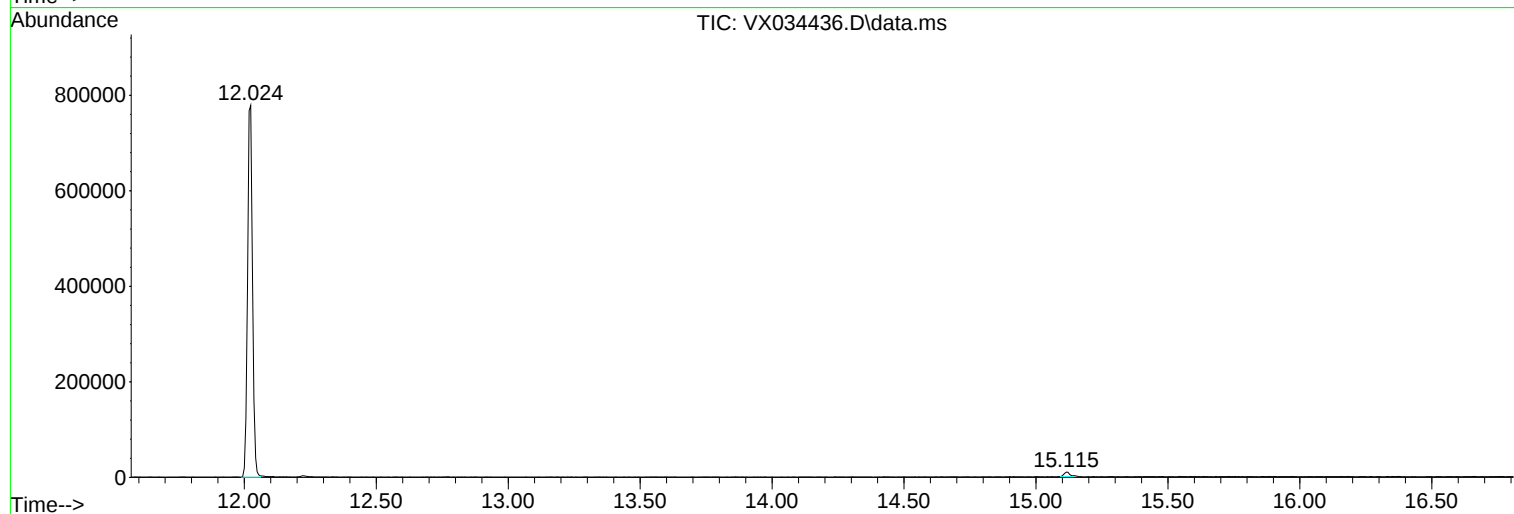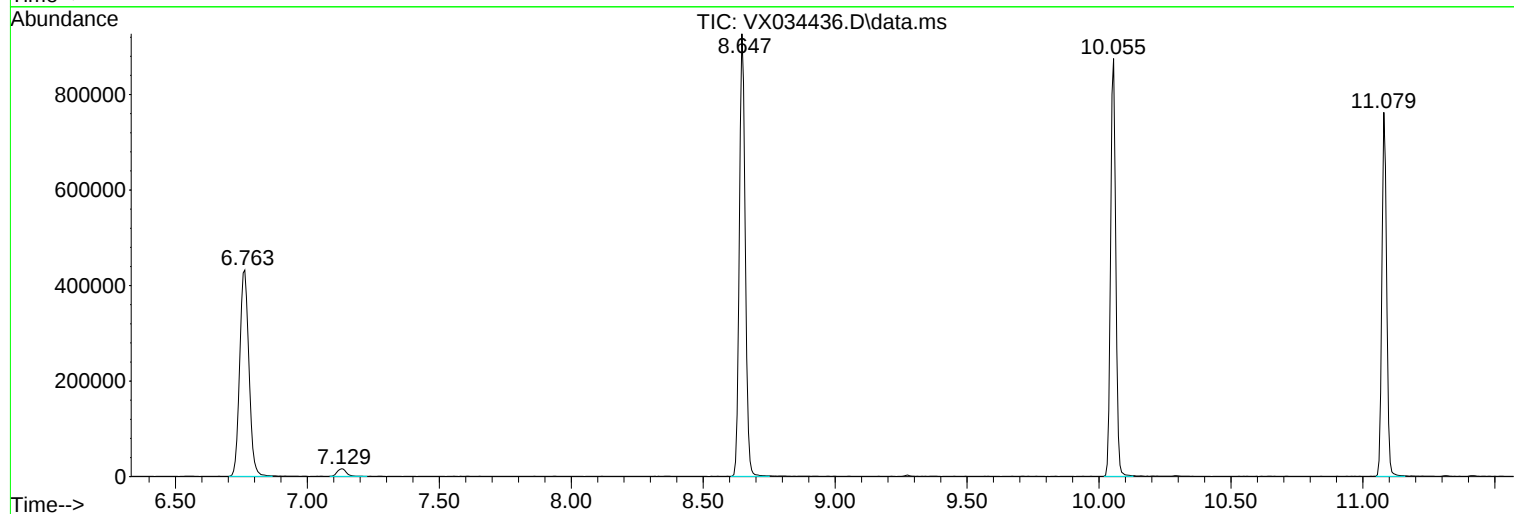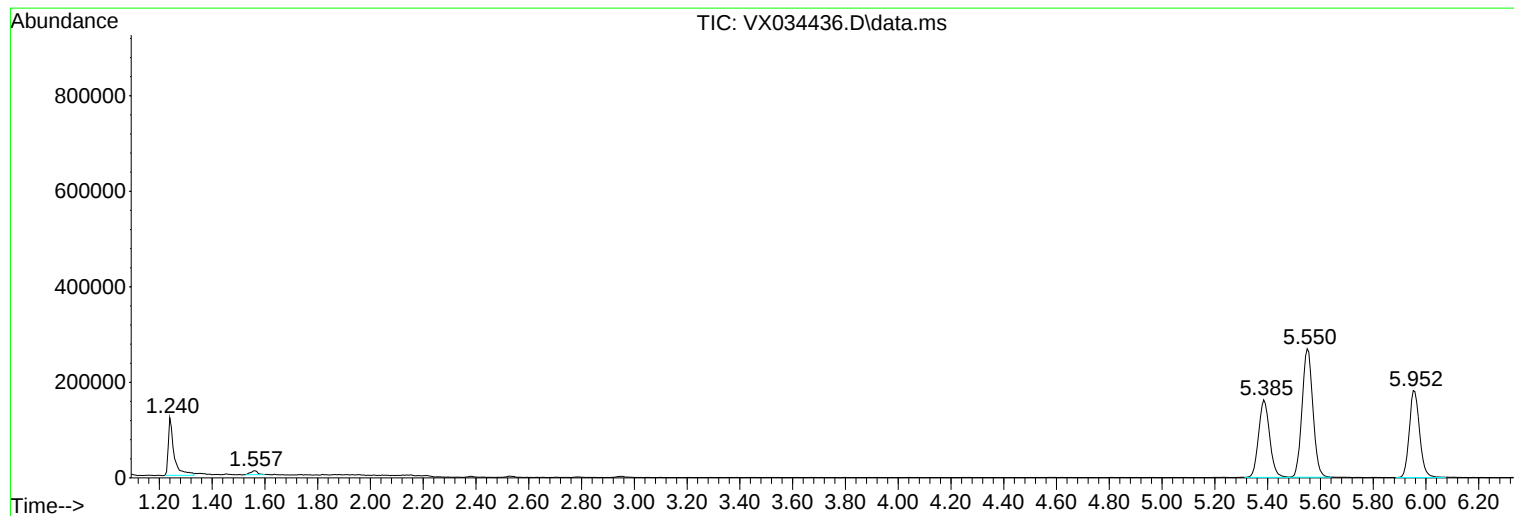

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034436.D
Acq On : 13 Mar 2023 16:35
Operator : JC/MD
Sample : 01879-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D3-20230308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034436.D
Acq On : 13 Mar 2023 16:35
Operator : JC/MD
Sample : 01879-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D3-20230308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------