

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034445.D
Acq On : 13 Mar 2023 20:07
Operator : JC/MD
Sample : 01879-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE104D2-20230308

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034445.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	21	25	35	rBV	74355	118346	3.10%	1.016%
2	4.489	546	558	576	rBV	103711	286227	7.50%	2.457%
3	5.385	693	705	720	rBV2	161382	470004	12.32%	4.034%
4	5.550	720	732	746	rVV	274022	767888	20.13%	6.591%
5	5.952	786	798	814	rBV	181467	489097	12.82%	4.198%
6	6.763	920	931	948	rBV	429512	1040735	27.28%	8.932%
7	7.123	981	990	1005	rBV	1779852	3815457	100.00%	32.747%
8	8.647	1233	1240	1258	rBV	939163	1448223	37.96%	12.430%
9	10.055	1465	1471	1485	rBV	889346	1209765	31.71%	10.383%
10	11.079	1634	1639	1655	rBV	777240	974914	25.55%	8.367%
11	12.018	1788	1793	1806	rBV	815786	1030675	27.01%	8.846%




Sum of corrected areas: 11651331

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034445.D
Acq On : 13 Mar 2023 20:07
Operator : JC/MD
Sample : 01879-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE104D2-20230308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

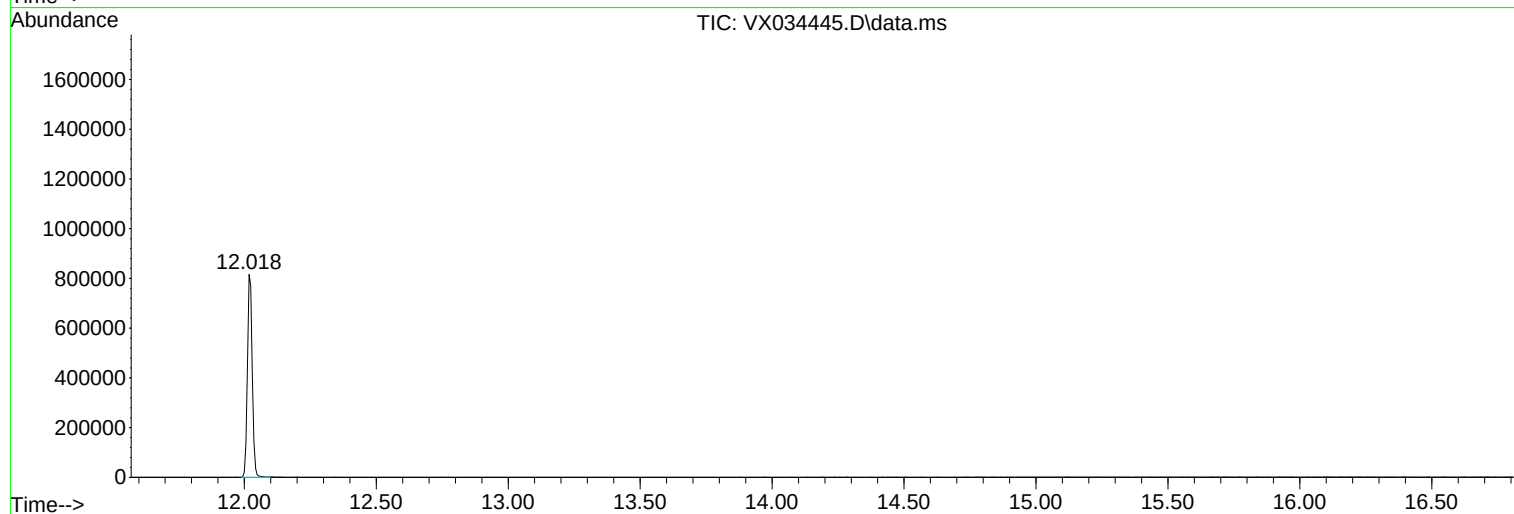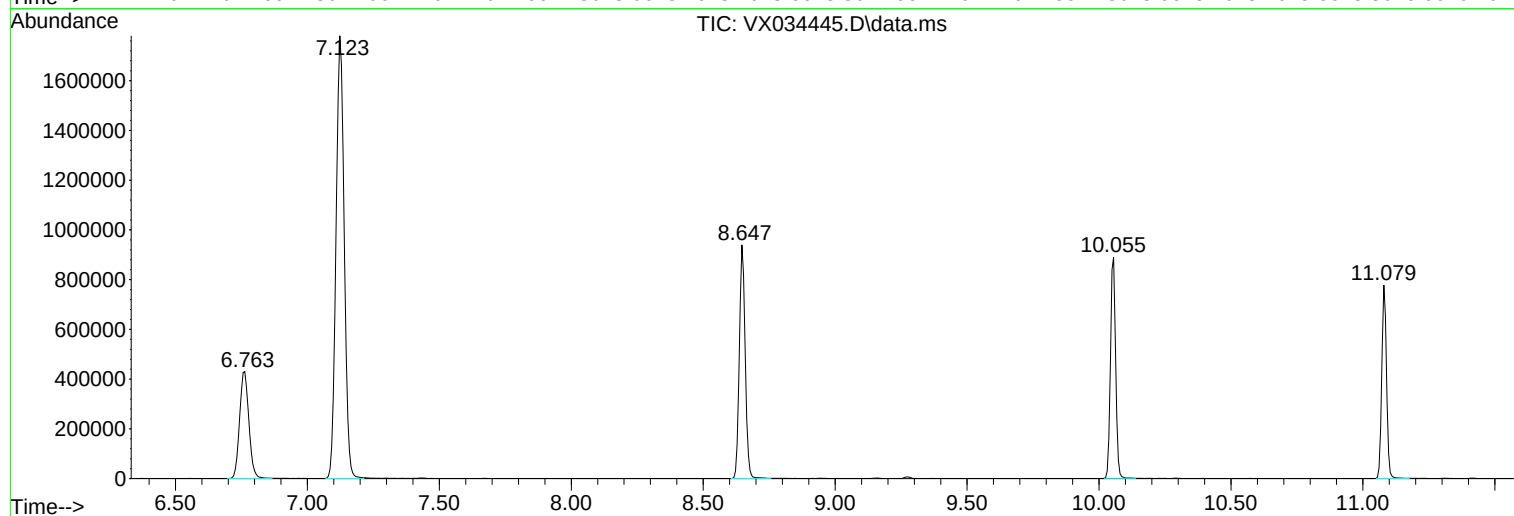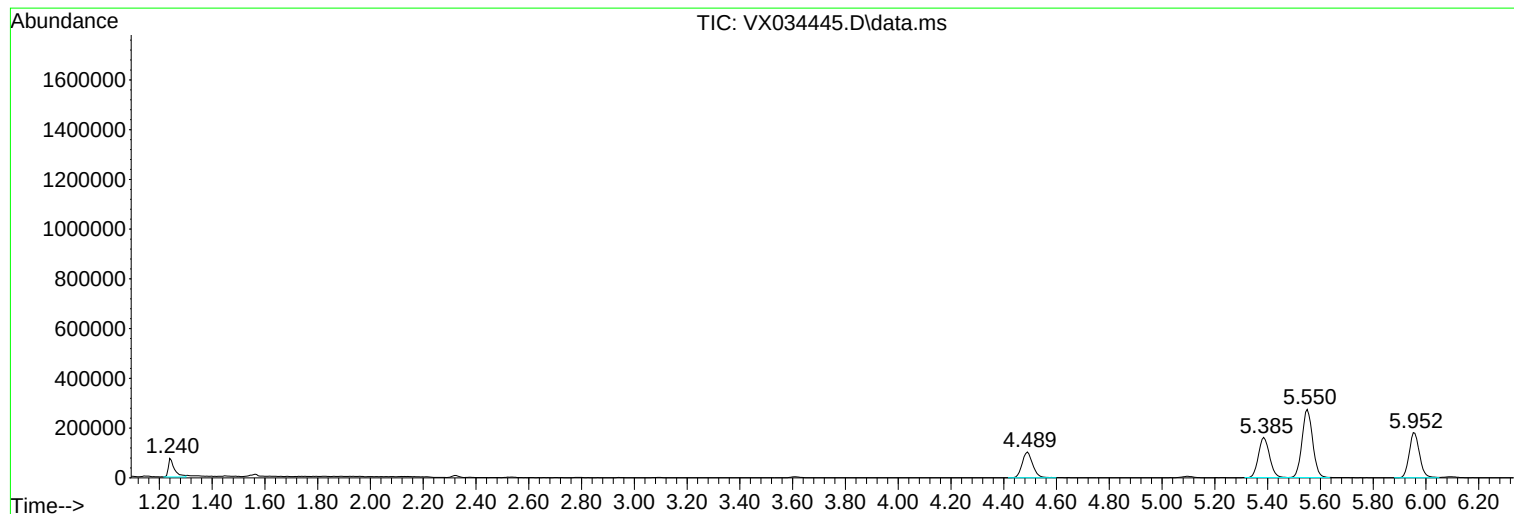

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034445.D
Acq On : 13 Mar 2023 20:07
Operator : JC/MD
Sample : 01879-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE104D2-20230308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031323\
Data File : VX034445.D
Acq On : 13 Mar 2023 20:07
Operator : JC/MD
Sample : 01879-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE104D2-20230308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
