

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031325\
 Data File : VX045266.D
 Acq On : 13 Mar 2025 14:00
 Operator : JC/MD
 Sample : Q1526-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Storage-Blank-SAMPLE-MANAGEMENT

Quant Time: Mar 14 12:28:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	65435	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	128551	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	119631	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	51355	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	56242	54.035	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	108.080%
35) Dibromofluoromethane	5.379	113	44345	51.589	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	103.180%
50) Toluene-d8	8.647	98	161746	51.903	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	103.800%
62) 4-Bromofluorobenzene	11.079	95	56263	54.484	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	108.960%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031325\
Data File : VX045266.D
Acq On : 13 Mar 2025 14:00
Operator : JC/MD
Sample : Q1526-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-SAMPLE-MANAGEMENT

Quant Time: Mar 14 12:28:20 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration




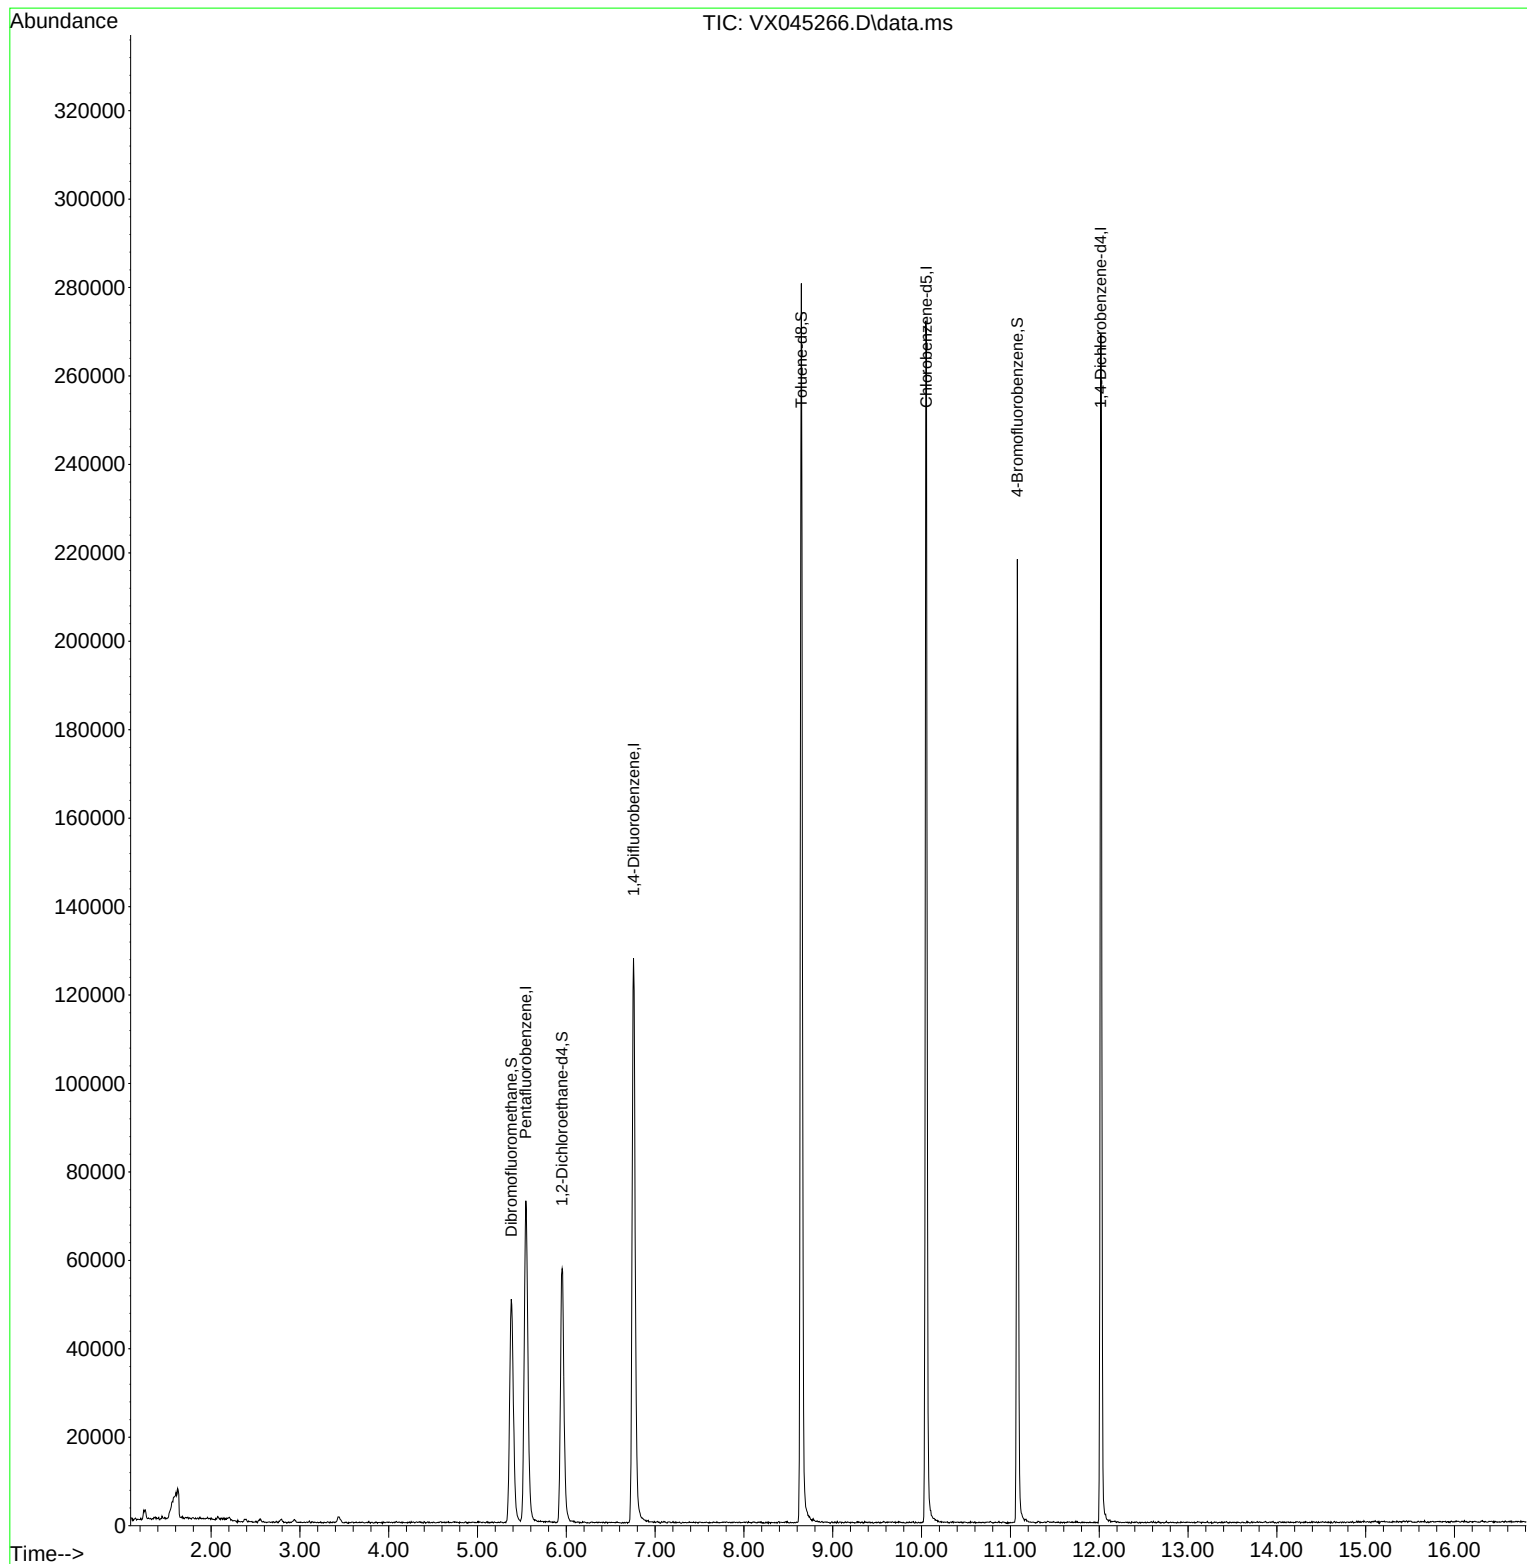


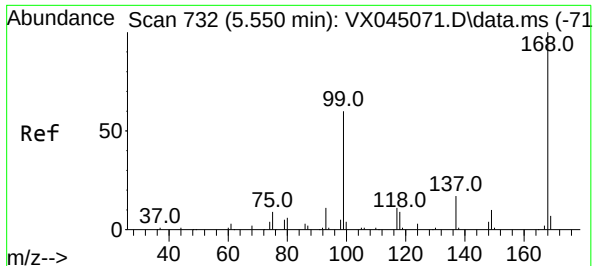

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.006 min
Lab File: VX045266.D
Acq: 13 Mar 2025 14:00




Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-SAMPLE-MANAGEMENT


Tgt Ion:168 Resp: 65435
Ion Ratio Lower Upper
168 100
99 63.8 48.2 72.4

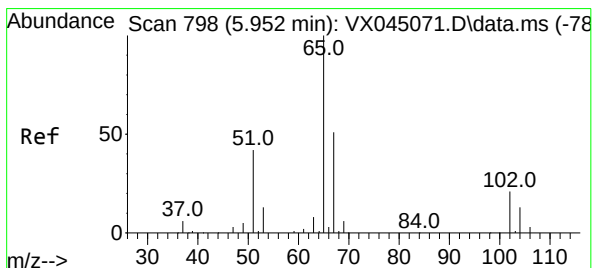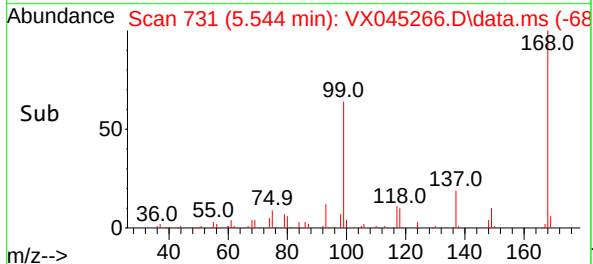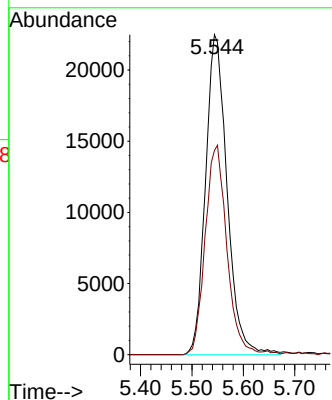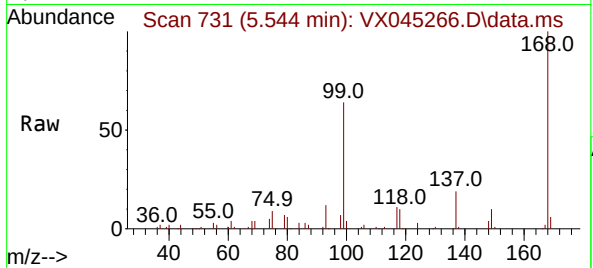

#33
1,2-Dichloroethane-d4
Concen: 54.035 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX045266.D
Acq: 13 Mar 2025 14:00

Tgt Ion: 65 Resp: 56242
Ion Ratio Lower Upper
65 100
67 51.8 0.0 106.2


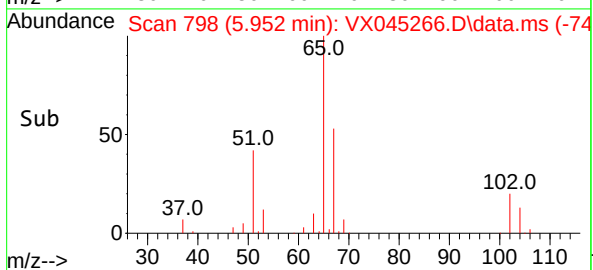
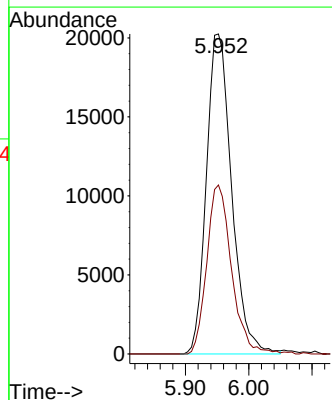
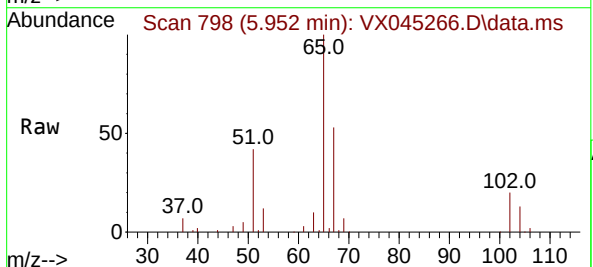


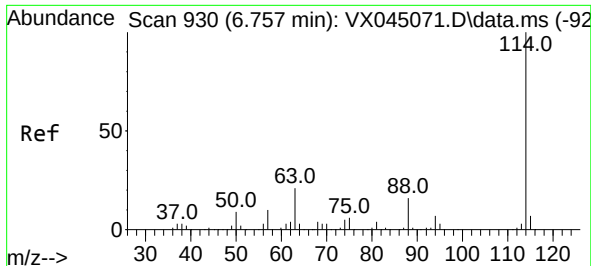

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX045266.D
Acq: 13 Mar 2025 14:00




Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-SAMPLE-MANAGEMENT


Tgt Ion:114 Resp: 128551
Ion Ratio Lower Upper
114 100
63 22.3 0.0 41.8
88 16.1 0.0 32.8

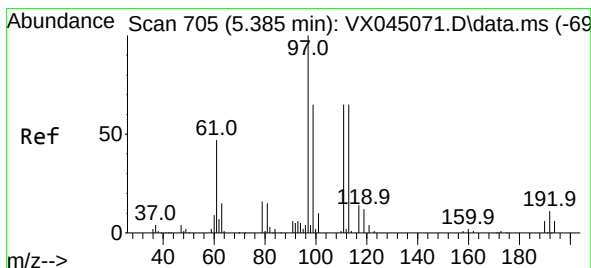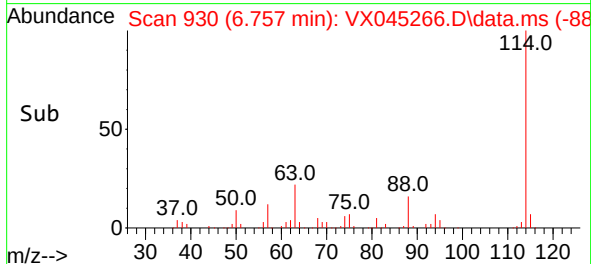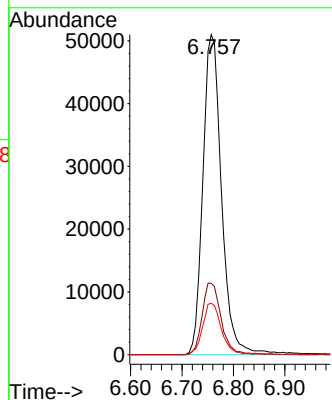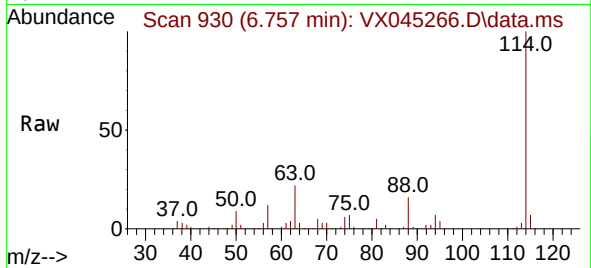

#35
Dibromofluoromethane
Concen: 51.589 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.006 min
Lab File: VX045266.D
Acq: 13 Mar 2025 14:00

Tgt Ion:113 Resp: 44345
Ion Ratio Lower Upper
113 100
111 104.2 81.8 122.6
192 16.8 14.3 21.5


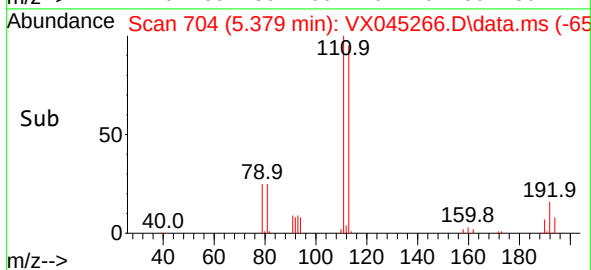
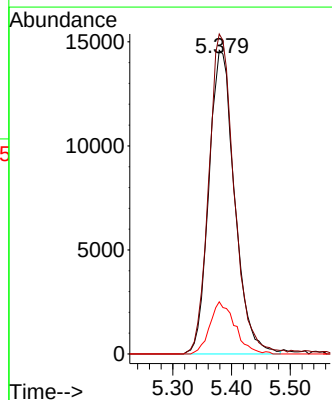
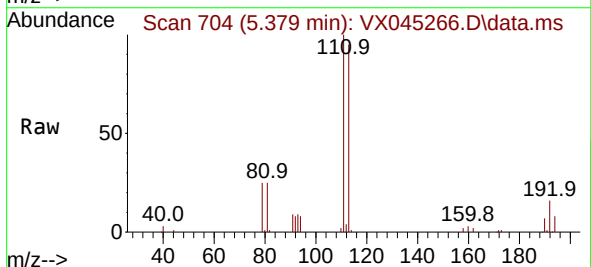


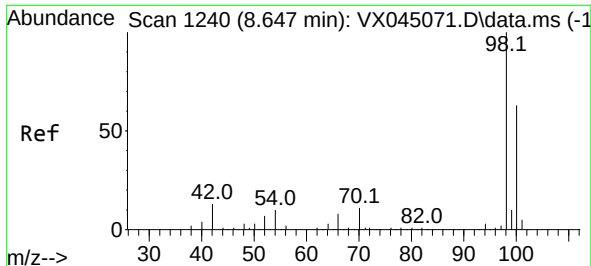

#50
Toluene-d8
Concen: 51.903 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX045266.D
Acq: 13 Mar 2025 14:00




Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-SAMPLE-MANAGEMENT


Tgt Ion: 98 Resp: 161746
Ion Ratio Lower Upper
98 100
100 64.6 52.0 78.0

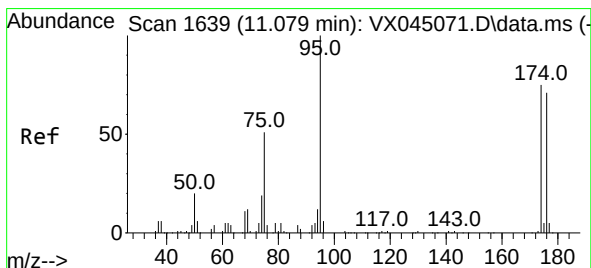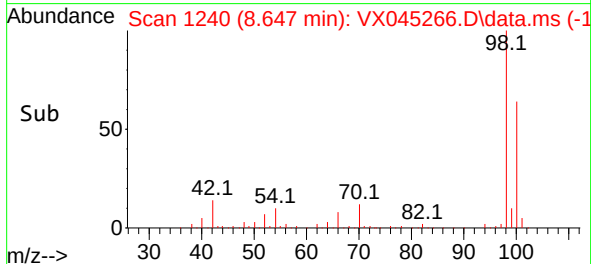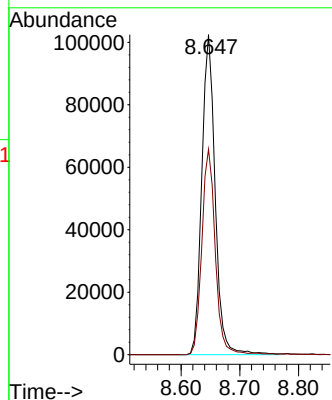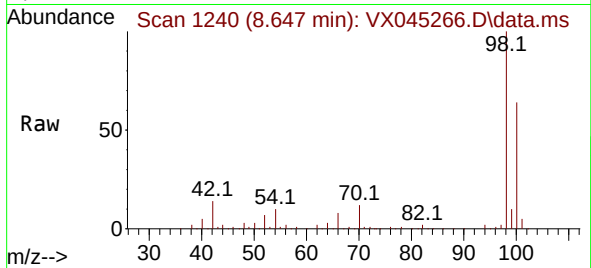

#62
4-Bromofluorobenzene
Concen: 54.484 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045266.D
Acq: 13 Mar 2025 14:00

Tgt Ion: 95 Resp: 56263
Ion Ratio Lower Upper
95 100
174 72.3 0.0 148.2
176 68.5 0.0 141.4


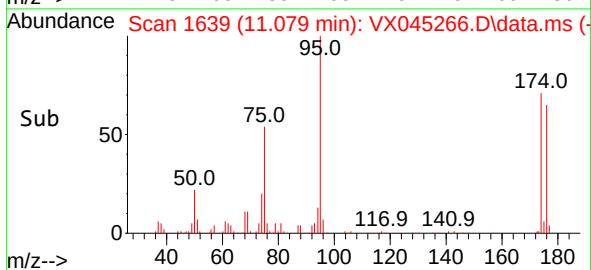
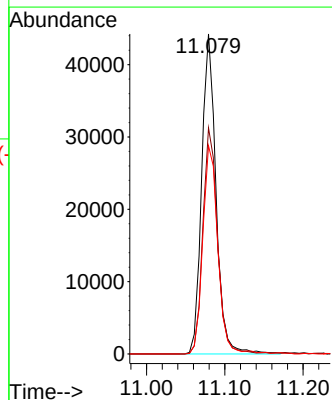
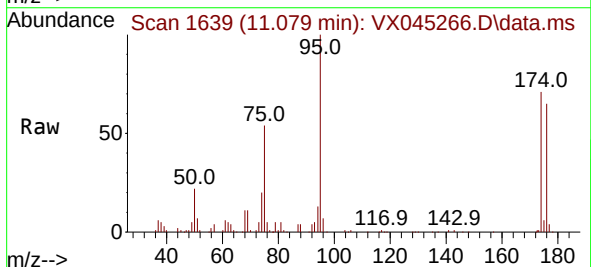


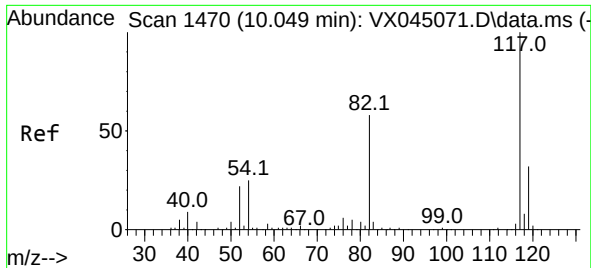

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1470
Delta R.T. 0.006 min
Lab File: VX045266.D
Acq: 13 Mar 2025 14:00

Instrument : MSVOA_X
ClientSampleId :
Storage-Blank-SAMPLE-MANAGEMENT

Tgt Ion:117 Resp: 119631
Ion Ratio Lower Upper
117 100
82 56.7 46.3 69.5
119 32.3 25.7 38.5

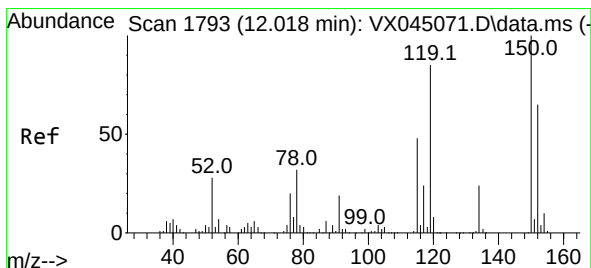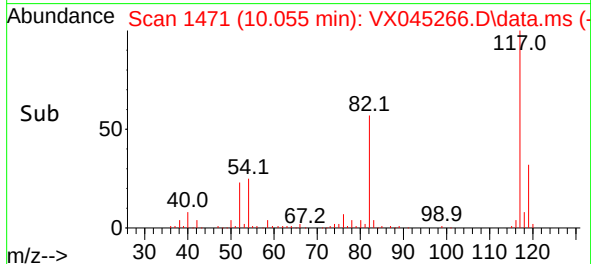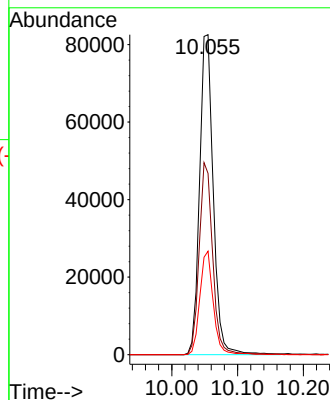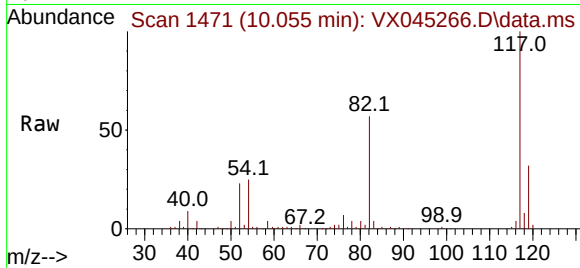

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX045266.D
Acq: 13 Mar 2025 14:00

Tgt Ion:152 Resp: 51355
Ion Ratio Lower Upper
152 100
115 62.9 44.2 132.6
150 154.9 0.0 349.0

