

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031325\
 Data File : VX045259.D
 Acq On : 13 Mar 2025 11:15
 Operator : JC/MD
 Sample : VX0313WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0313WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M

Title : SW846 8260

Signal : TIC: VX045259.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	32	rBV5	2352	4894	1.06%	0.205%
2	1.569	67	79	80	rBV4	4337	9553	2.08%	0.399%
3	2.935	297	303	312	rBV3	2618	6028	1.31%	0.252%
4	5.379	693	704	721	rBV2	54010	161311	35.05%	6.742%
5	5.550	721	732	750	rVV	73007	214475	46.60%	8.963%
6	5.952	787	798	811	rBV	60761	165351	35.93%	6.910%
7	6.757	921	930	946	rBV	133729	326702	70.98%	13.654%
8	8.647	1233	1240	1255	rBV	286495	460266	100.00%	19.236%
9	10.049	1465	1470	1484	rBV	283806	406684	88.36%	16.996%
10	11.079	1634	1639	1652	rBV	231384	292546	63.56%	12.226%
11	12.018	1788	1793	1804	rBV	277430	344952	74.95%	14.416%




Sum of corrected areas: 2392762

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031325\
Data File : VX045259.D
Acq On : 13 Mar 2025 11:15
Operator : JC/MD
Sample : VX0313WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0313WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

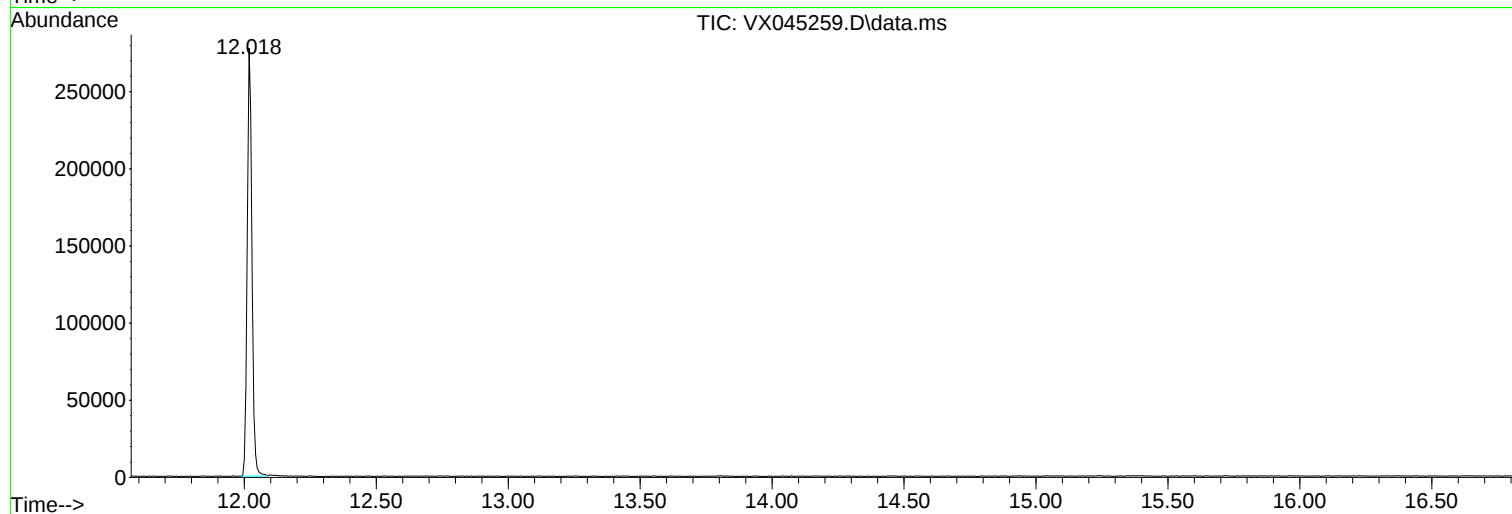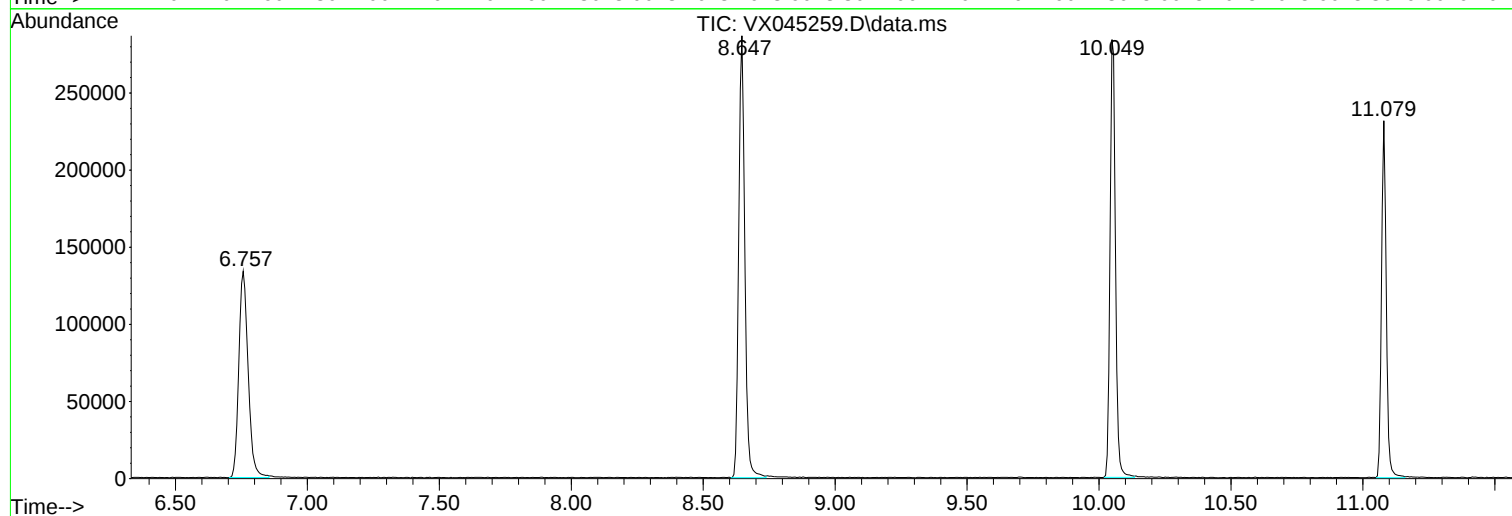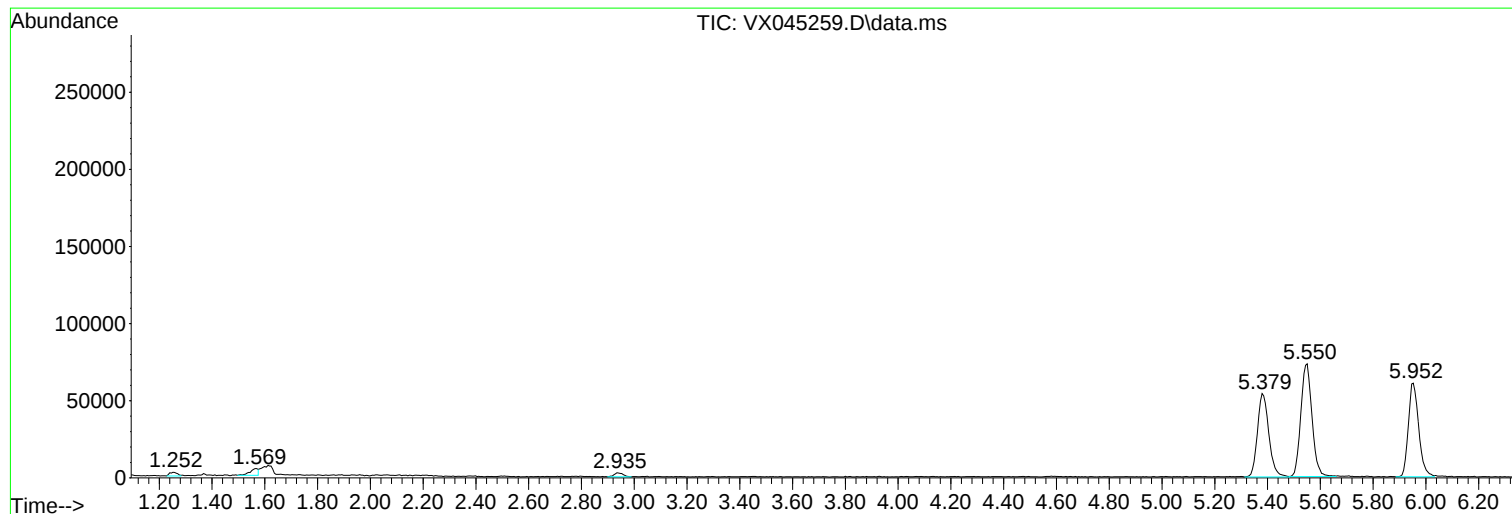

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031325\
Data File : VX045259.D
Acq On : 13 Mar 2025 11:15
Operator : JC/MD
Sample : VX0313WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0313WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031325\
Data File : VX045259.D
Acq On : 13 Mar 2025 11:15
Operator : JC/MD
Sample : VX0313WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0313WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc