

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX031419\
 Data File : VX008078.D
 Acq On : 14 Mar 2019 19:21
 Operator : JC/SP
 Sample : VX0314WBL02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0314WBL02

Quant Time: Mar 15 04:58:40 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X031419W.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 15 03:56:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	329258	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	502484	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	474939	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	235827	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	162230	48.84	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.68%	
35) Dibromofluoromethane	5.51	113	158362	49.70	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.40%	
50) Toluene-d8	8.71	98	603377	49.79	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.58%	
62) 4-Bromofluorobenzene	11.13	95	222444	51.24	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.48%	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX031419\
Data File : VX008078.D
Acq On : 14 Mar 2019 19:21
Operator : JC/SP
Sample : VX0314WBL02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0314WBL02

Quant Time: Mar 15 04:58:40 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X031419W.M
Quant Title : SW846 8260
QLast Update : Fri Mar 15 03:56:35 2019
Response via : Initial Calibration

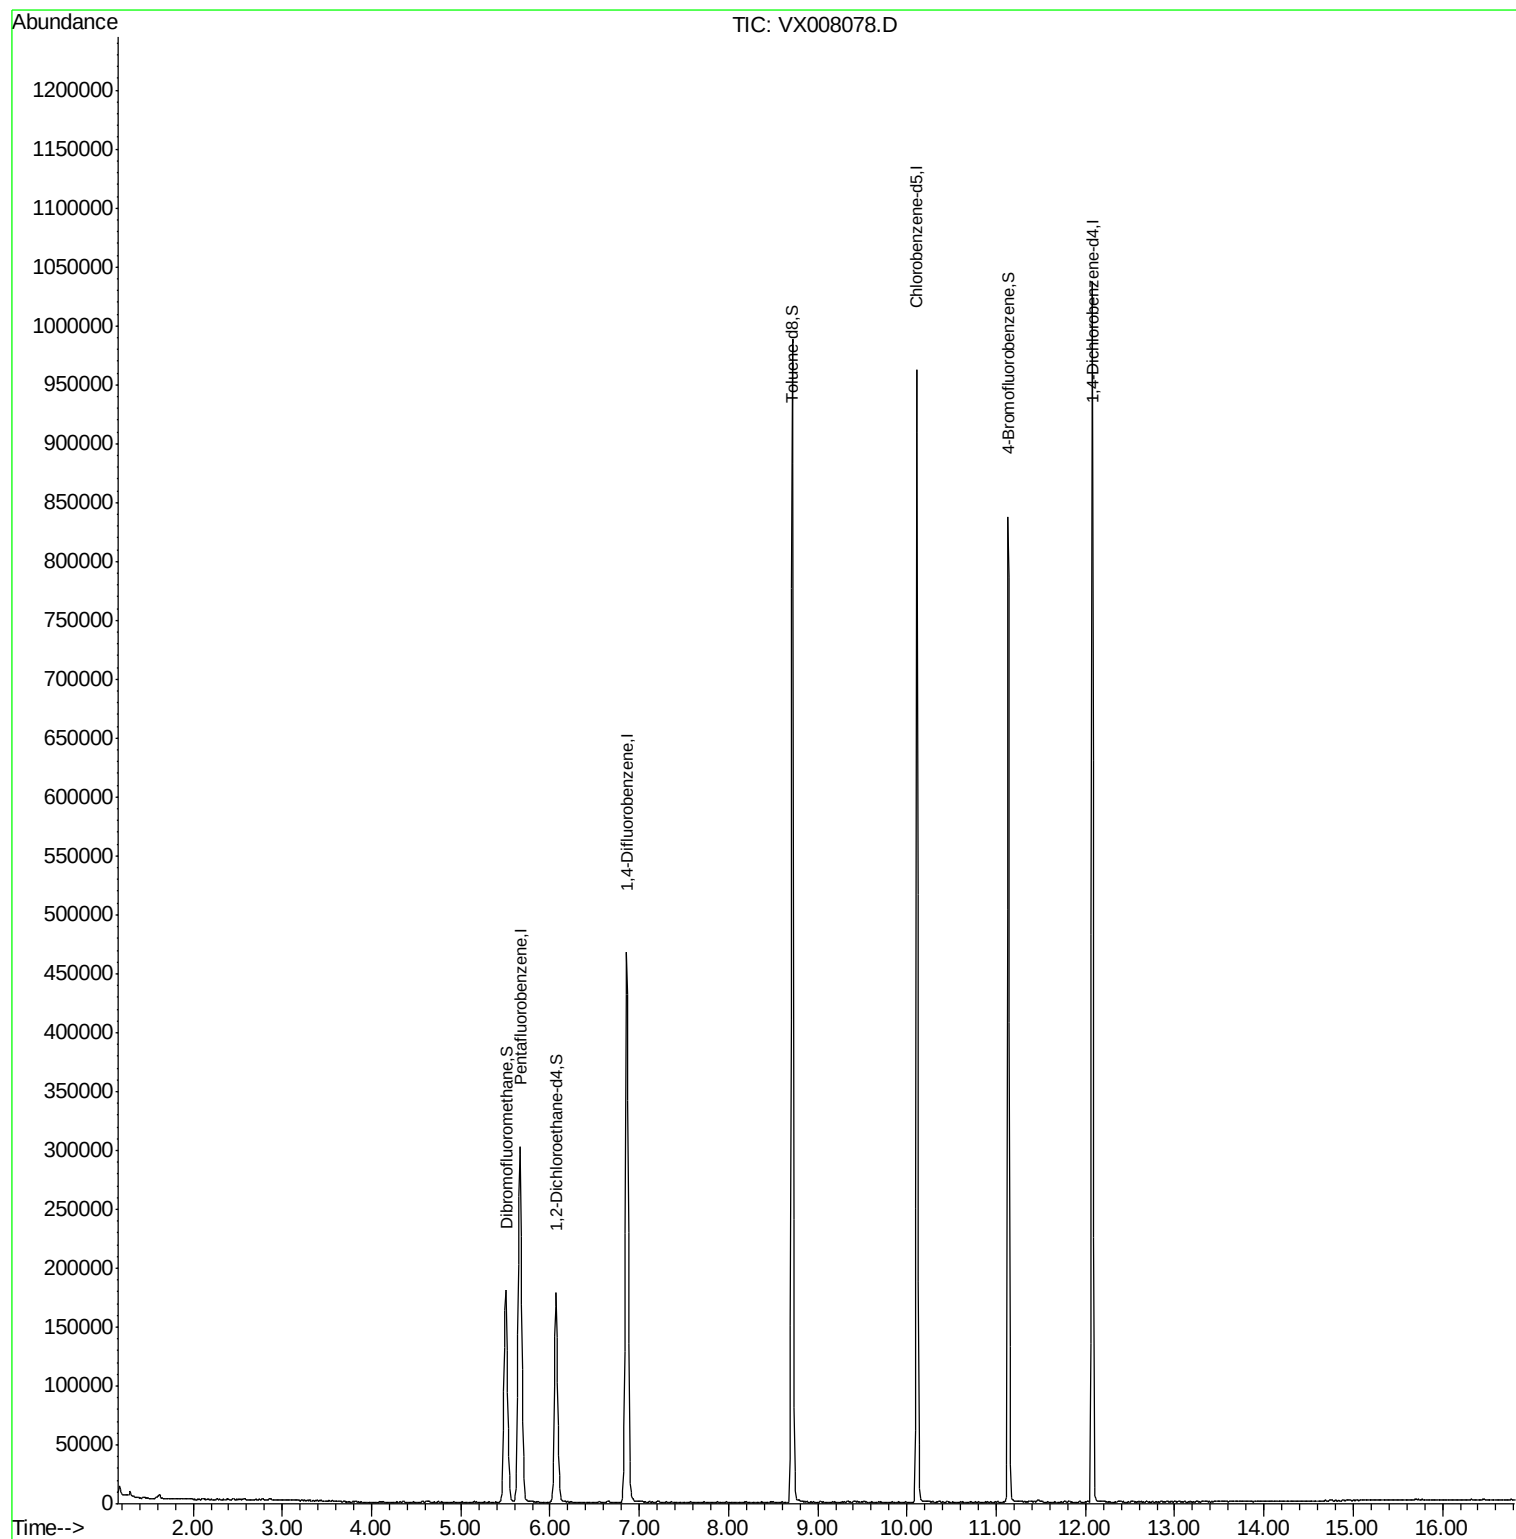

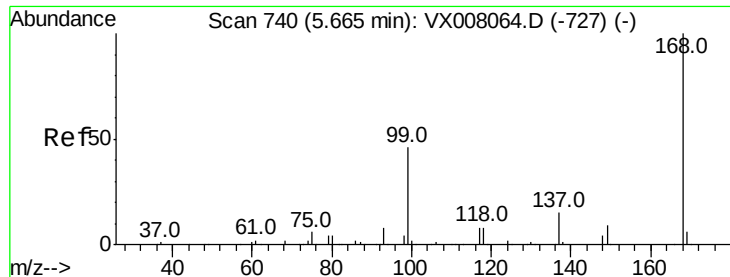

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.00 min

Lab File: VX008078.D

Acq: 14 Mar 2019 19:21

Instrument :

MSVOA_X

ClientSampleId :


VX0314WBL02

Tot Ion:168 Resp: 329258

Ion Ratio Lower Upper

168 100

99 46.6 37.6 56.4

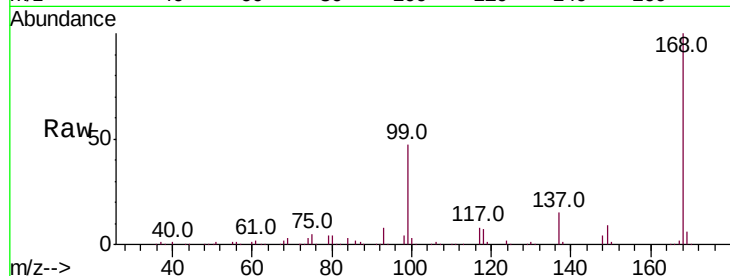

Abundance Ion 167.90 (167.60 to 168.60): VX0

Ion 98.90 (98.60 to 99.60): VX0



5.67

100000

50000

0

Time--> 5.50 5.60 5.70 5.80

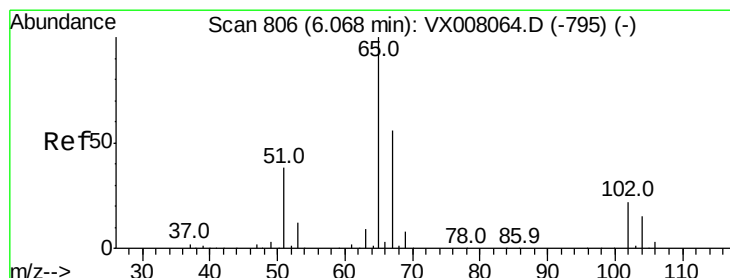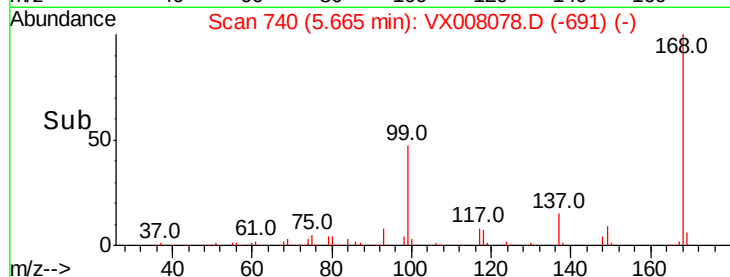

#33

1,2-Dichloroethane-d4

Concen: 48.844 ug/l

RT: 6.07 min Scan# 806

Delta R.T. -0.00 min

Lab File: VX008078.D


Acq: 14 Mar 2019 19:21

Tgt Ion: 65 Resp: 162230

Ion Ratio Lower Upper

65 100

67 55.1 0.0 110.0

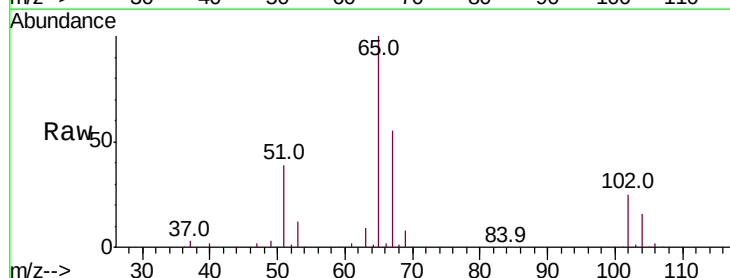

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07


60000


40000

20000

0

Time--> 5.90 6.00 6.10 6.20

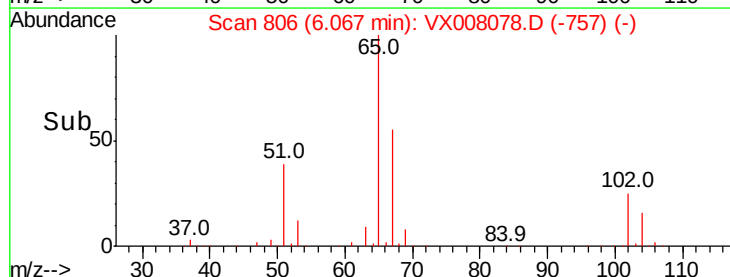


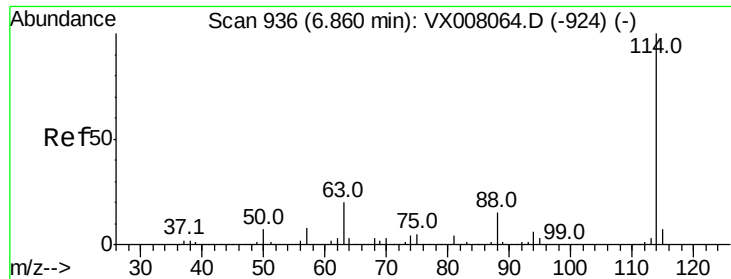




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.86 min Scan# 936
Delta R.T. -0.00 min
Lab File: VX008078.D
Acq: 14 Mar 2019 19:21

Instrument :
MSVOA_X
ClientSampleId :
VX0314WBL02

Tot Ion:114 Resp: 502484
Ion Ratio Lower Upper
114 100
63 18.5 0.0 39.8
88 15.8 0.0 31.4

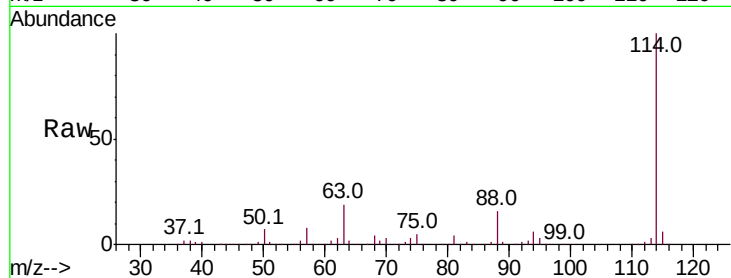


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VX0
Ion 87.90 (87.60 to 88.60): VX0

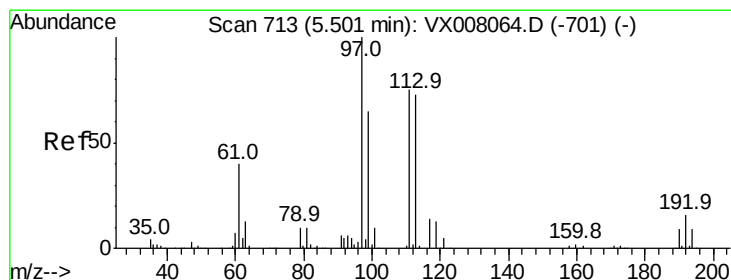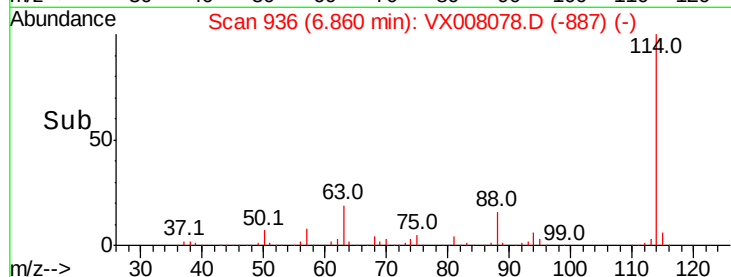
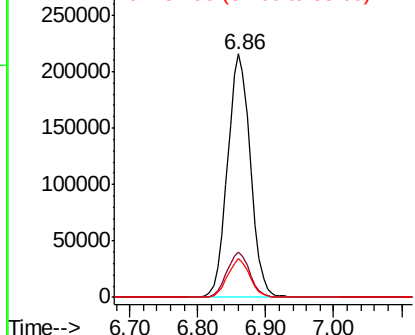



#35
Dibromofluoromethane
Concen: 49.698 ug/l
RT: 5.51 min Scan# 714
Delta R.T. 0.01 min
Lab File: VX008078.D
Acq: 14 Mar 2019 19:21

Tgt Ion:113 Resp: 158362
Ion Ratio Lower Upper
113 100
111 101.0 81.4 122.0
192 25.2 19.4 29.0

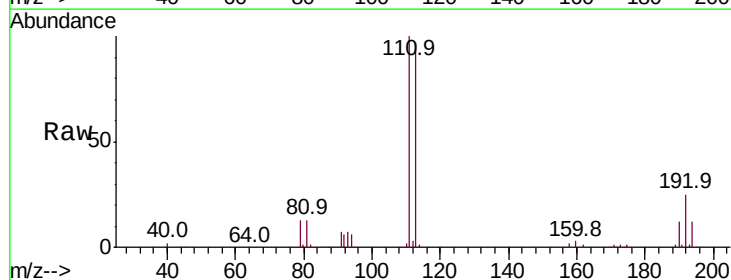

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V



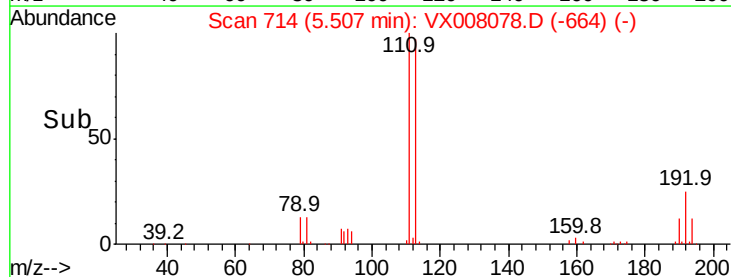
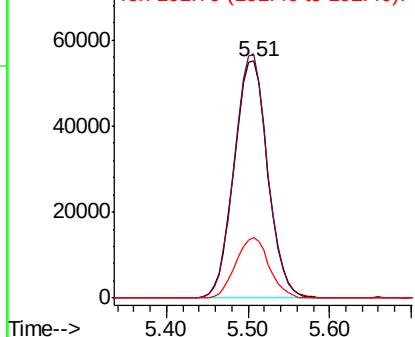


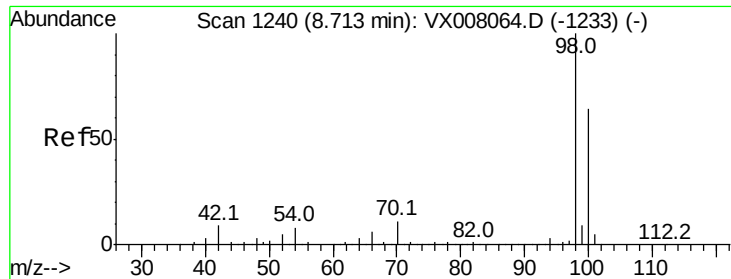

#50
Toluene-d8
Concen: 49.787 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. -0.00 min
Lab File: VX008078.D
Acq: 14 Mar 2019 19:21




Instrument :
MSVOA_X
ClientSampleId :
VX0314WBL02


Tot Ion: 98 Resp: 603377
Ion Ratio Lower Upper
98 100
100 64.9 51.7 77.5

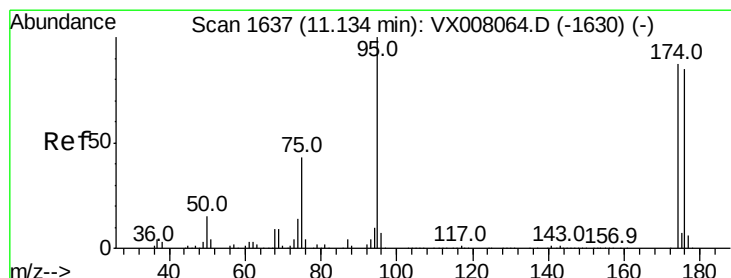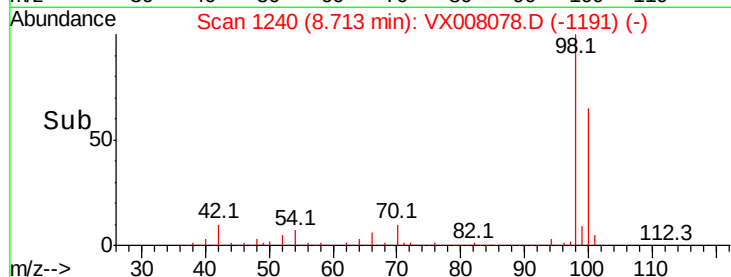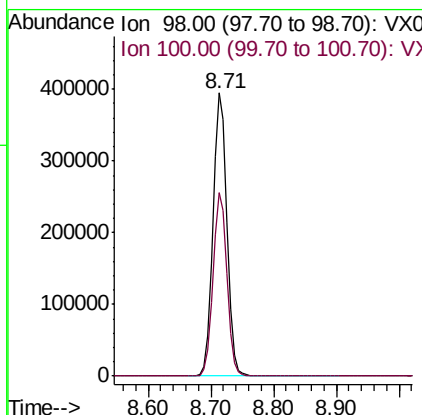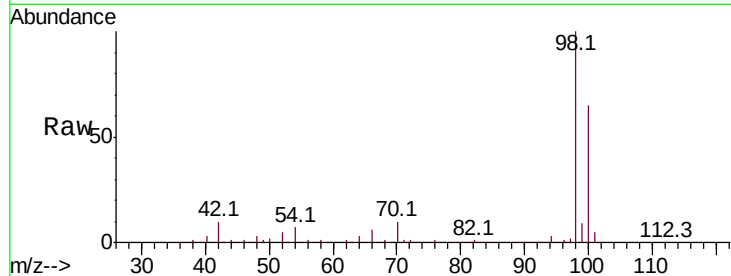

#62
4-Bromofluorobenzene
Concen: 51.237 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX008078.D
Acq: 14 Mar 2019 19:21

Tgt Ion: 95 Resp: 222444
Ion Ratio Lower Upper
95 100
174 94.5 0.0 182.8
176 92.7 0.0 178.0

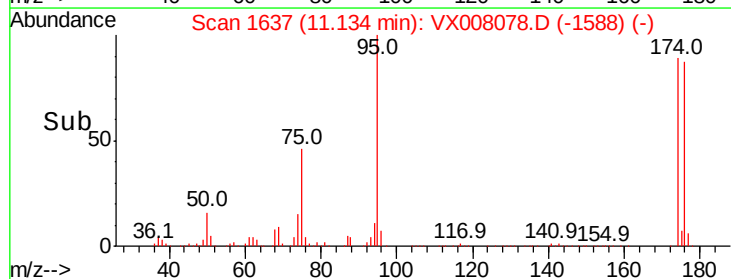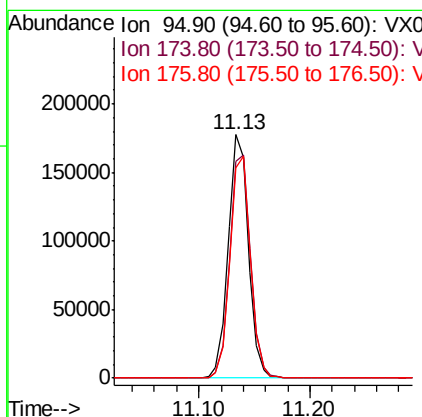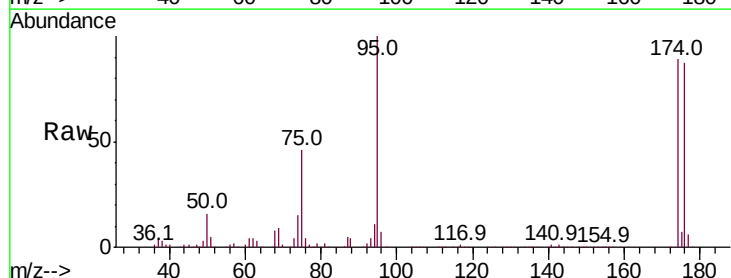


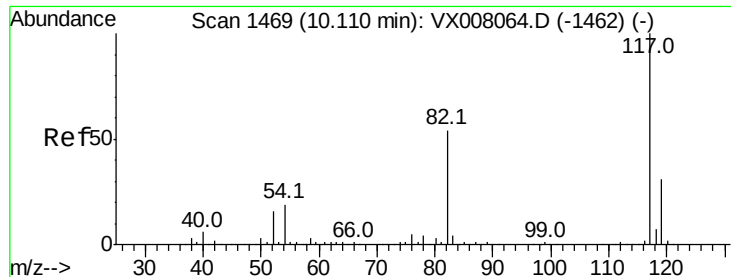




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. -0.00 min
Lab File: VX008078.D
Acq: 14 Mar 2019 19:21

Instrument :
MSVOA_X
ClientSampleId :
VX0314WBL02

Tot Ion:117 Resp: 474939
Ion Ratio Lower Upper
117 100
82 53.8 44.3 66.5
119 31.5 25.3 37.9

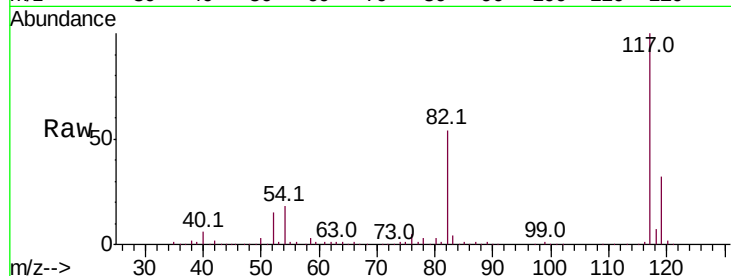


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

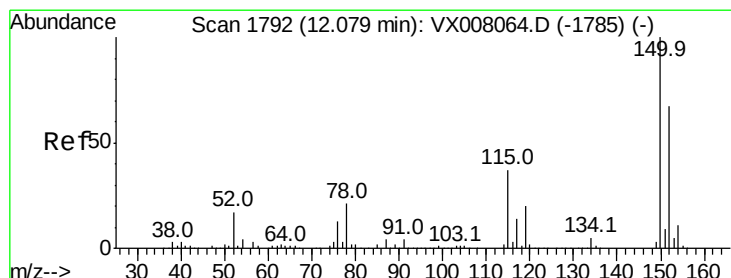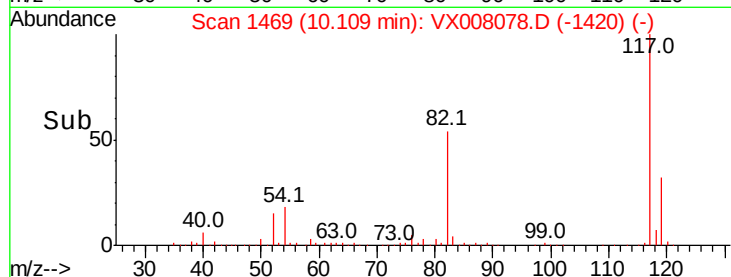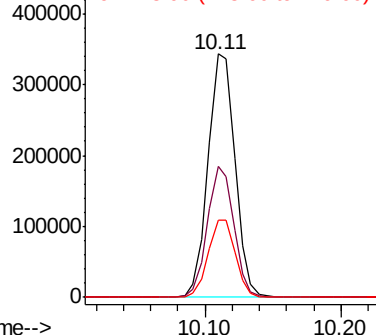

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX008078.D
Acq: 14 Mar 2019 19:21

Tgt Ion:152 Resp: 235827
Ion Ratio Lower Upper
152 100
115 54.4 38.6 115.7
150 154.9 0.0 348.4

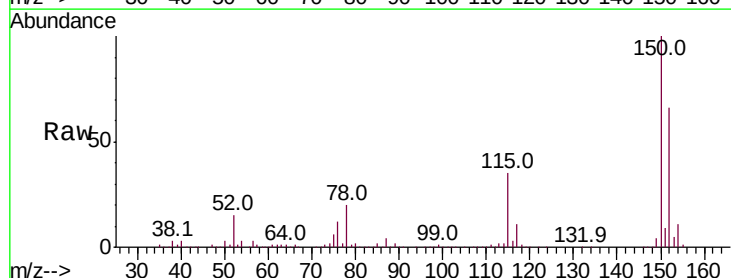

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

