


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX031419\
 Data File : VX008060.D
 Acq On : 14 Mar 2019 09:04
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X031419W.M
 Title : SW846 8260
 Last Update : Fri Mar 15 03:56:35 2019

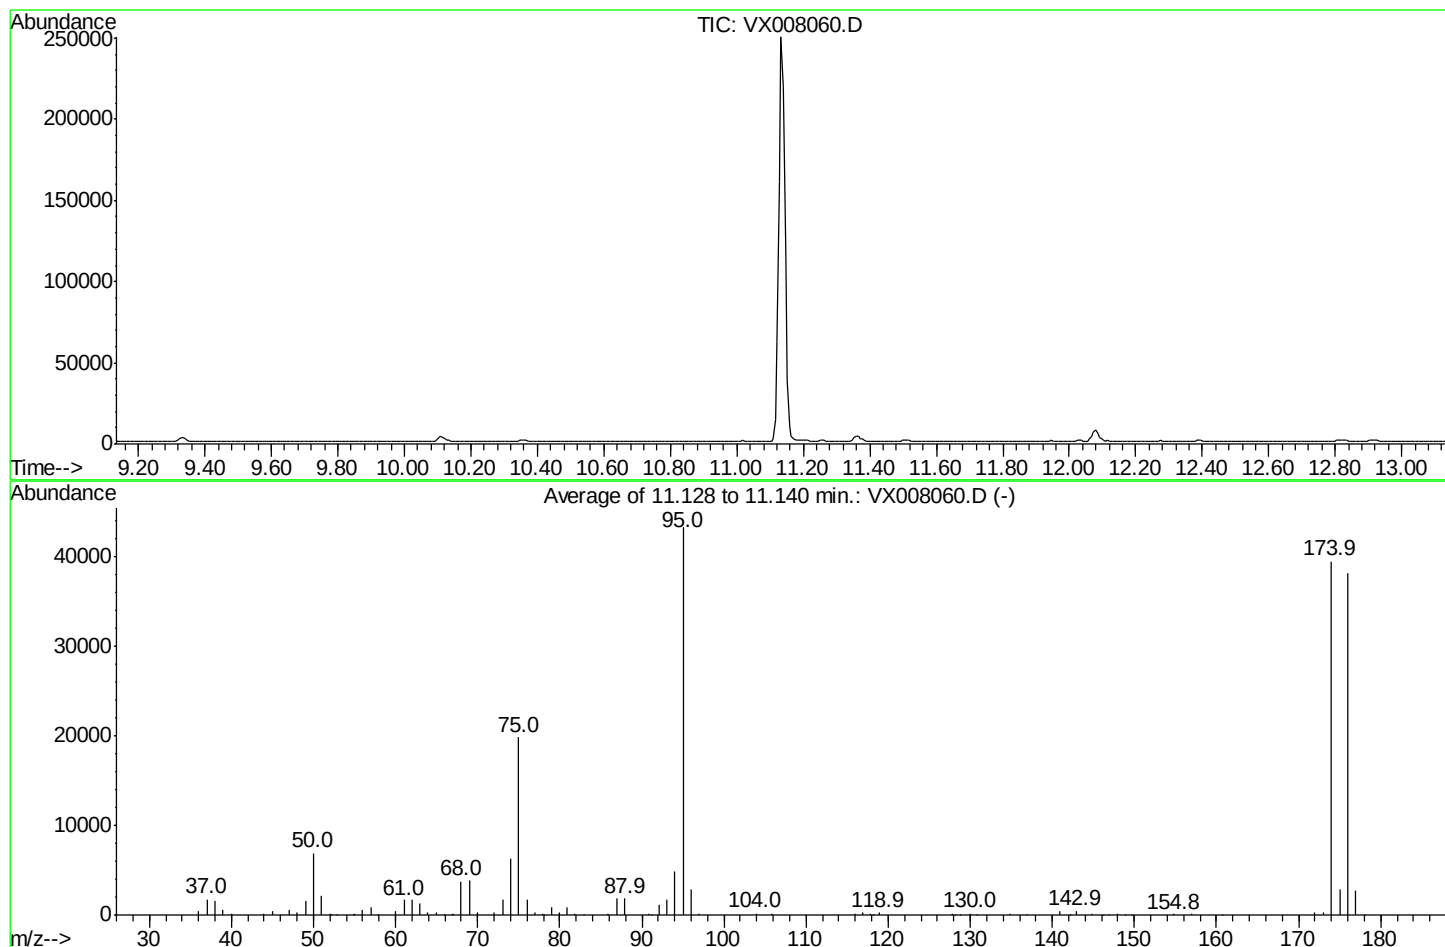

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	6911	PASS
75	95	30	60	45.9	19850	PASS
95	95	100	100	100.0	43264	PASS
96	95	5	9	6.7	2919	PASS
173	174	0.00	2	0.8	321	PASS
174	95	50	100	91.2	39453	PASS
175	174	5	9	7.4	2927	PASS
176	174	95	101	96.8	38178	PASS
177	176	5	9	7.1	2724	PASS