

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
 Data File : VX034487.D
 Acq On : 15 Mar 2023 06:37
 Operator : JC/MD
 Sample : 01903-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BPOW1-7-20230310

Quant Time: Mar 15 08:26:56 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
 Quant Title : SW846 8260
 QLast Update : Mon Mar 13 10:29:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	247470	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	422481	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	382655	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	173402	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	166057	46.125	ug/l	0.01
Spiked Amount	50.000	Range	78 - 117	Recovery	=	92.240%
35) Dibromofluoromethane	5.385	113	133573	47.886	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.780%
50) Toluene-d8	8.647	98	515271	49.483	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.960%
62) 4-Bromofluorobenzene	11.079	95	196941	46.823	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	93.640%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034487.D
Acq On : 15 Mar 2023 06:37
Operator : JC/MD
Sample : 01903-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPOW1-7-20230310

Quant Time: Mar 15 08:26:56 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260
QLast Update : Mon Mar 13 10:29:32 2023
Response via : Initial Calibration




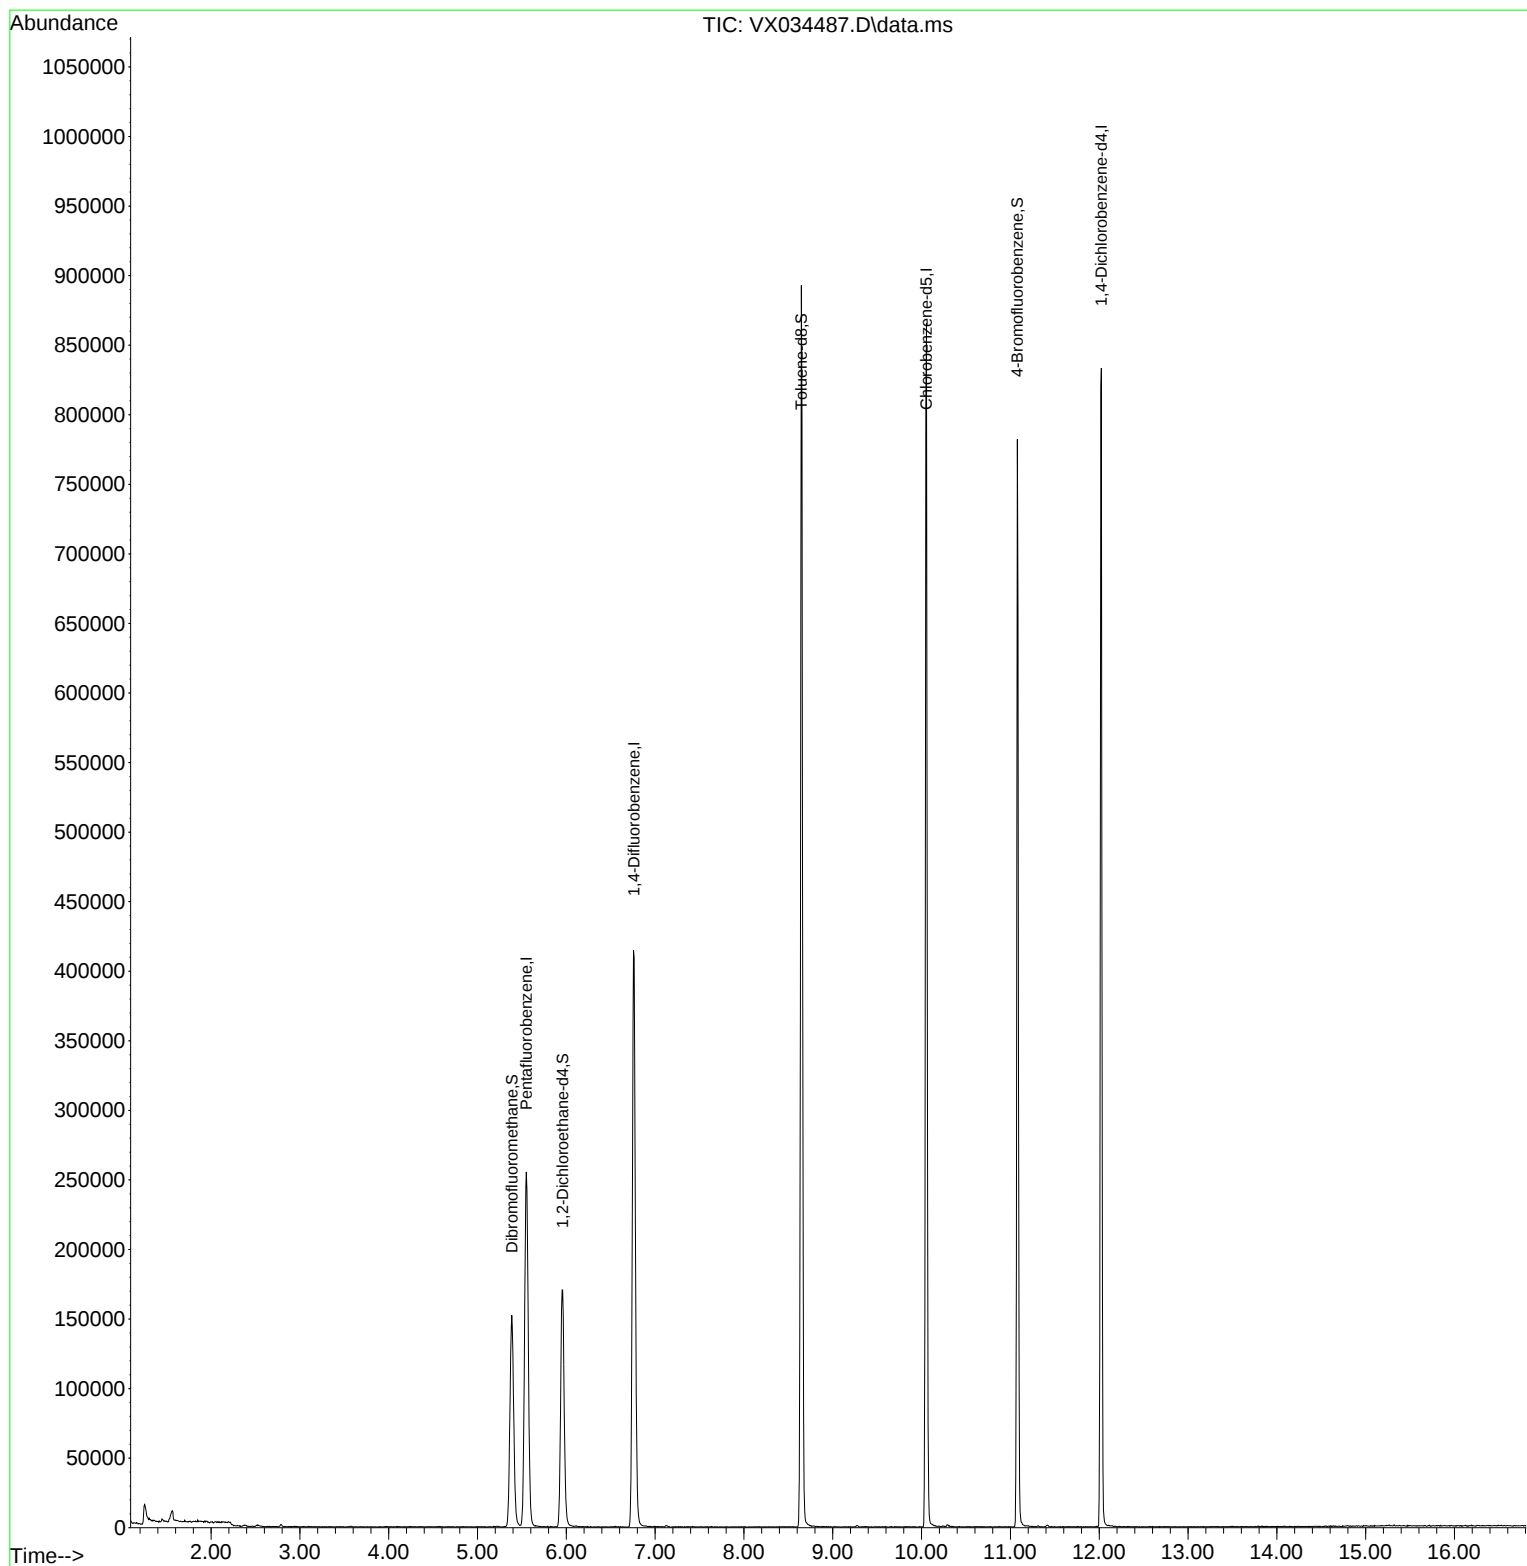




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX034487.D
Acq: 15 Mar 2023 06:37




Instrument :
MSVOA_X
ClientSampleId :
BPOW1-7-20230310


Tgt Ion:168 Resp: 247470
Ion Ratio Lower Upper
168 100
99 58.0 45.7 68.5

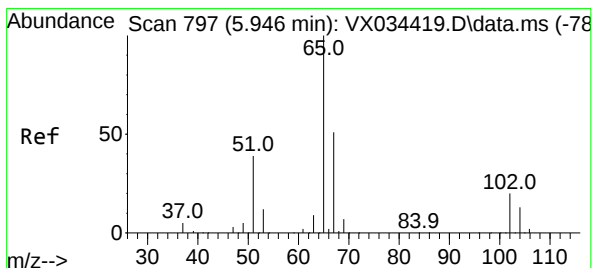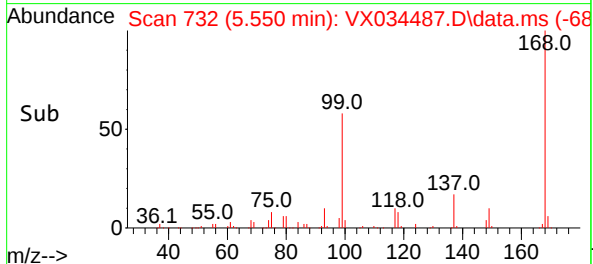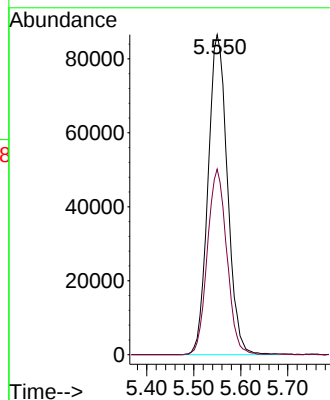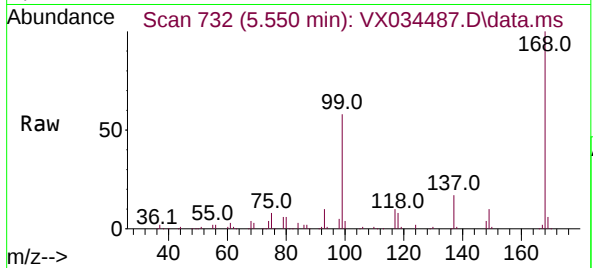

#33
1,2-Dichloroethane-d4
Concen: 46.125 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.012 min
Lab File: VX034487.D
Acq: 15 Mar 2023 06:37

Tgt Ion: 65 Resp: 166057
Ion Ratio Lower Upper
65 100
67 51.4 0.0 104.0


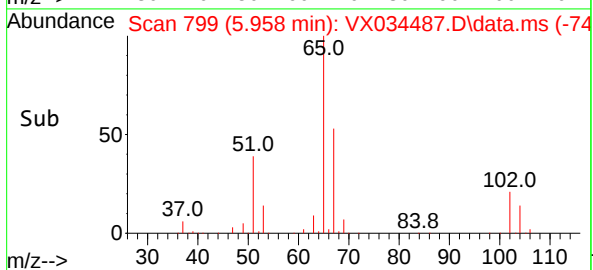
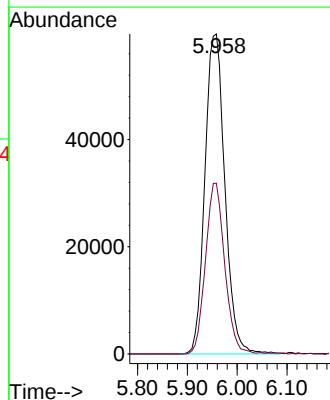
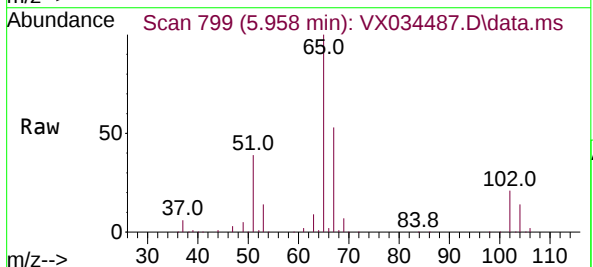


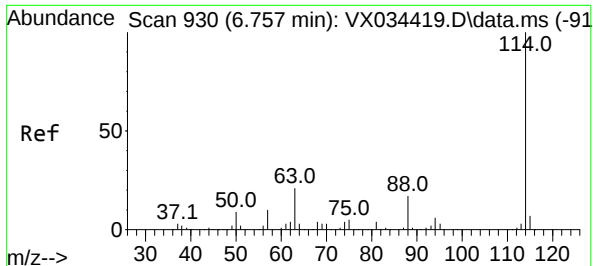

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX034487.D
Acq: 15 Mar 2023 06:37




Instrument :
MSVOA_X
ClientSampleId :
BPOW1-7-20230310


Tgt Ion:114 Resp: 422481
Ion Ratio Lower Upper
114 100
63 20.2 0.0 42.2
88 15.2 0.0 33.2

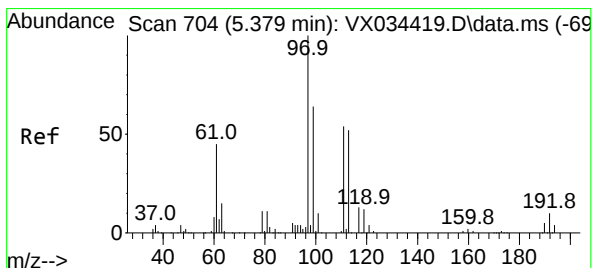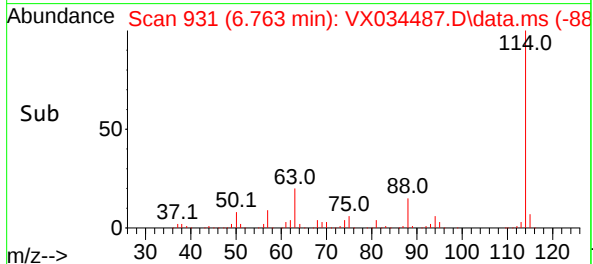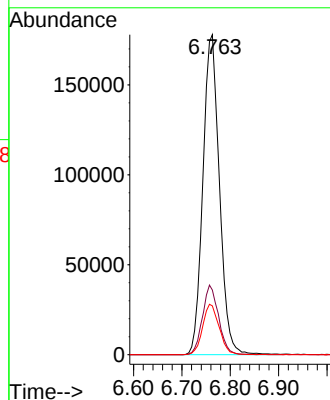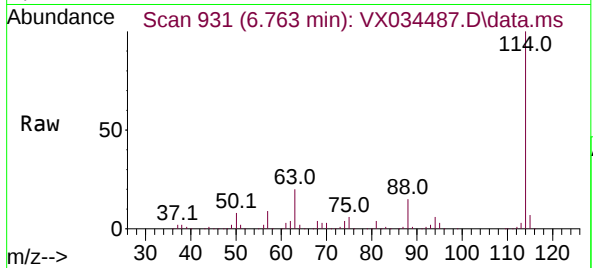

#35
Dibromofluoromethane
Concen: 47.886 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX034487.D
Acq: 15 Mar 2023 06:37

Tgt Ion:113 Resp: 133573
Ion Ratio Lower Upper
113 100
111 101.1 83.7 125.5
192 19.0 15.4 23.2


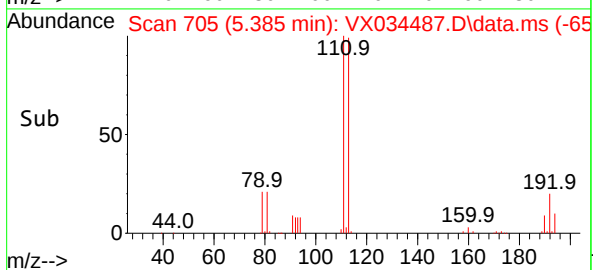
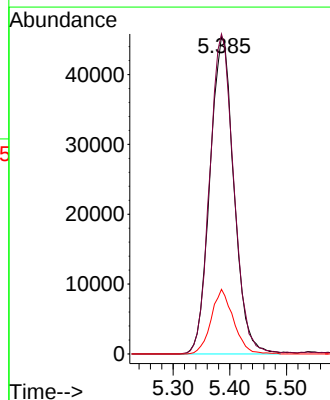
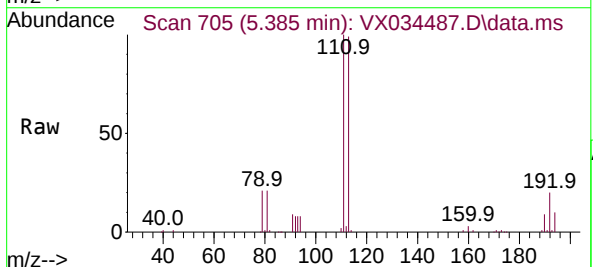


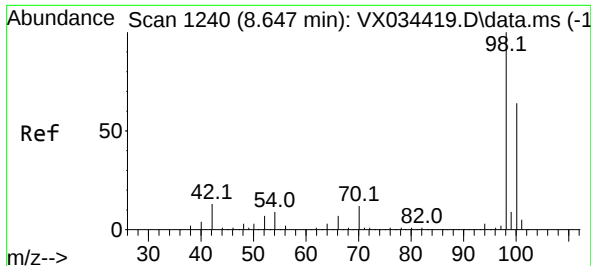

#50
Toluene-d8
Concen: 49.483 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX034487.D
Acq: 15 Mar 2023 06:37




Instrument :
MSVOA_X
ClientSampleId :
BPOW1-7-20230310


Tgt Ion: 98 Resp: 515271
Ion Ratio Lower Upper
98 100
100 64.8 52.5 78.7

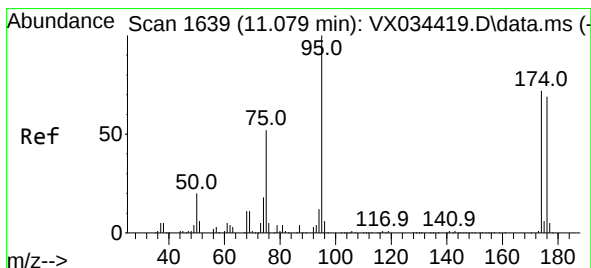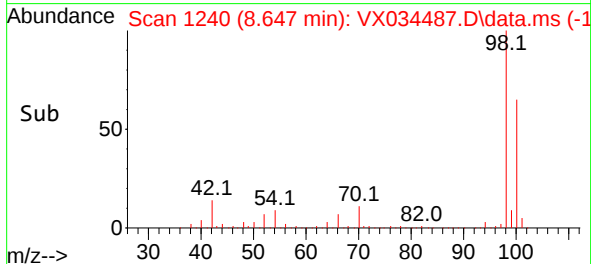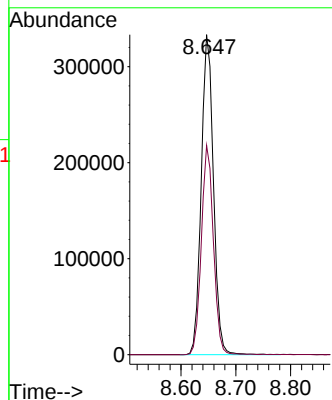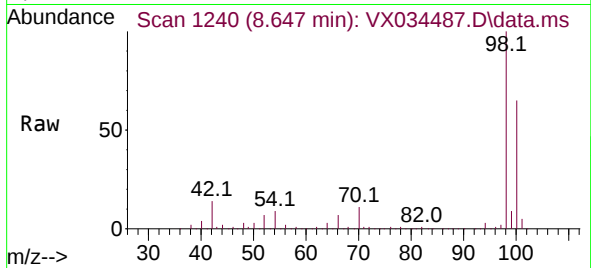

#62
4-Bromofluorobenzene
Concen: 46.823 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX034487.D
Acq: 15 Mar 2023 06:37

Tgt Ion: 95 Resp: 196941
Ion Ratio Lower Upper
95 100
174 77.6 0.0 147.4
176 75.1 0.0 140.6

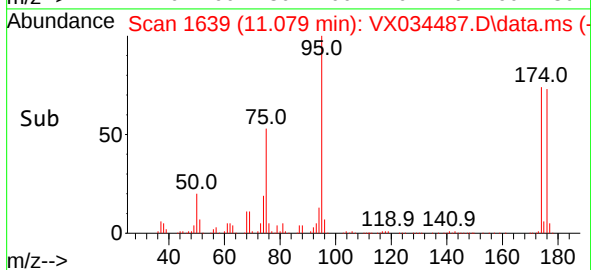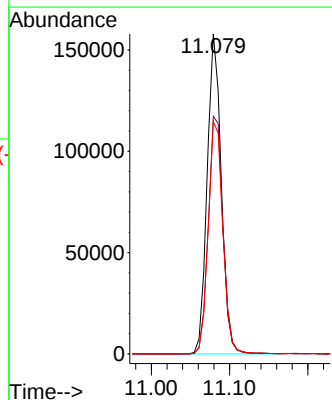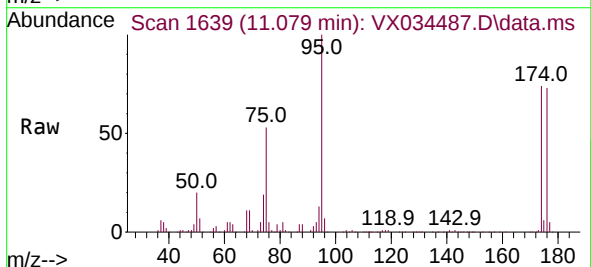

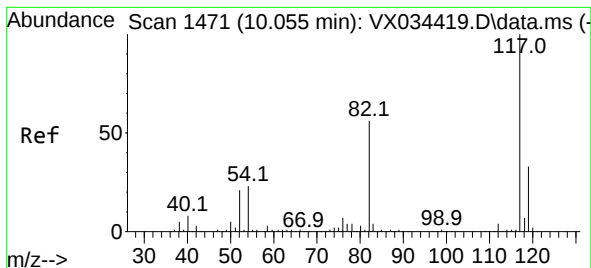

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX034487.D

Acq: 15 Mar 2023 06:37

Instrument :

MSVOA_X

ClientSampleId :

BPOW1-7-20230310





Tgt Ion:117 Resp: 382655

Ion Ratio Lower Upper

117 100

82 56.2 45.0 67.4

119 31.4 26.0 39.0

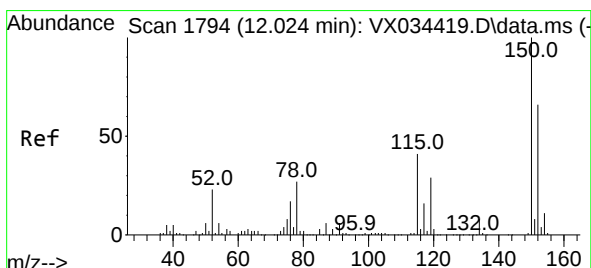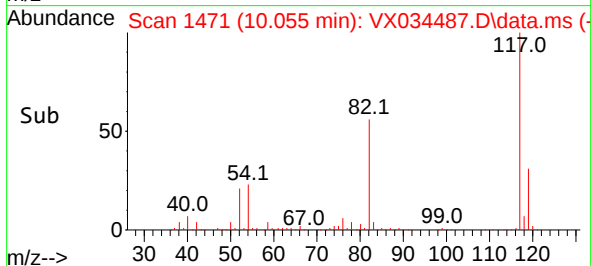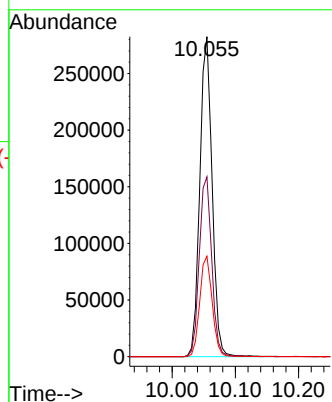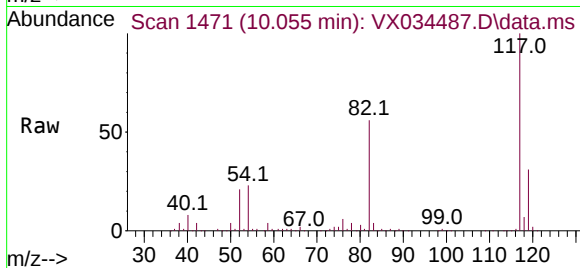

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. -0.000 min

Lab File: VX034487.D

Acq: 15 Mar 2023 06:37

Tgt Ion:152 Resp: 173402

Ion Ratio Lower Upper

152 100

115 58.7 45.0 135.0

150 156.0 0.0 352.4

