

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034450.D
Acq On : 14 Mar 2023 09:22
Operator : JC/MD
Sample : VX0314MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0314MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	31	rBV3	11310	20700	1.28%	0.246%
2	5.385	693	705	721	rBV	177914	527854	32.63%	6.270%
3	5.550	721	732	748	rVB	296757	853958	52.80%	10.144%
4	5.952	787	798	813	rBV	203142	546886	33.81%	6.496%
5	6.757	921	930	943	rBV	493229	1169713	72.32%	13.895%
6	8.647	1233	1240	1259	rBV	1044357	1617477	100.00%	19.214%
7	10.055	1465	1471	1484	rBV	999129	1379092	85.26%	16.382%
8	11.079	1634	1639	1652	rBV	825552	1036596	64.09%	12.314%
9	12.018	1788	1793	1804	rBV	956827	1249673	77.26%	14.845%
10	13.725	2068	2073	2077	rBV2	13898	16389	1.01%	0.195%




Sum of corrected areas: 8418338

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034450.D
Acq On : 14 Mar 2023 09:22
Operator : JC/MD
Sample : VX0314MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0314MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

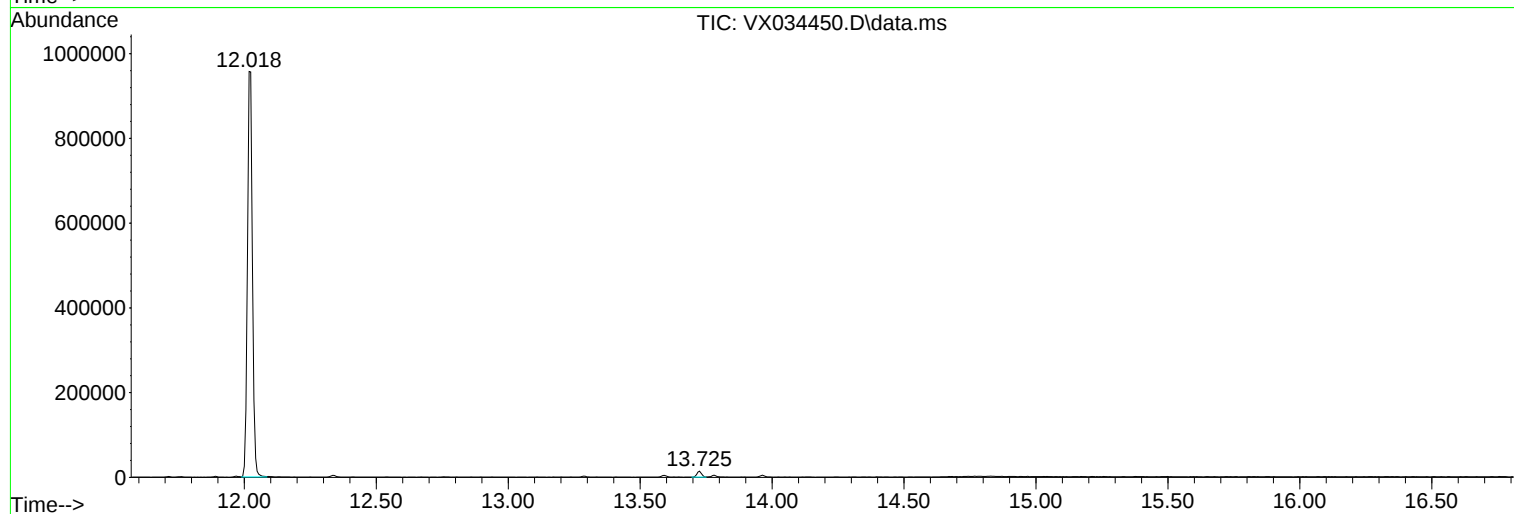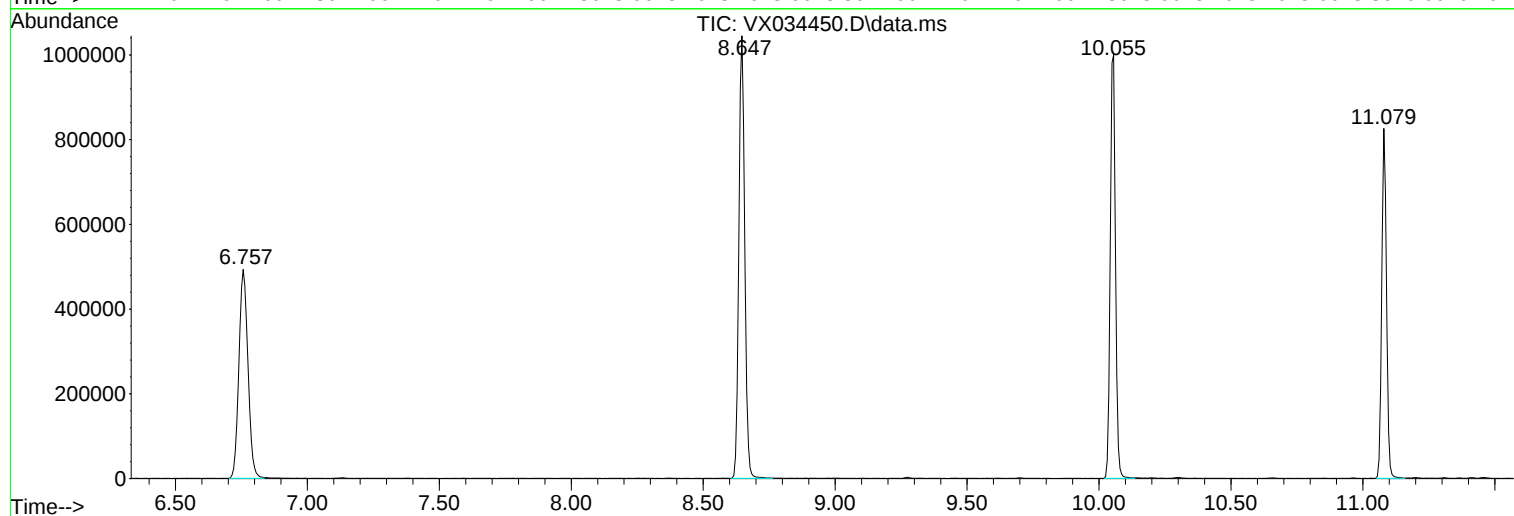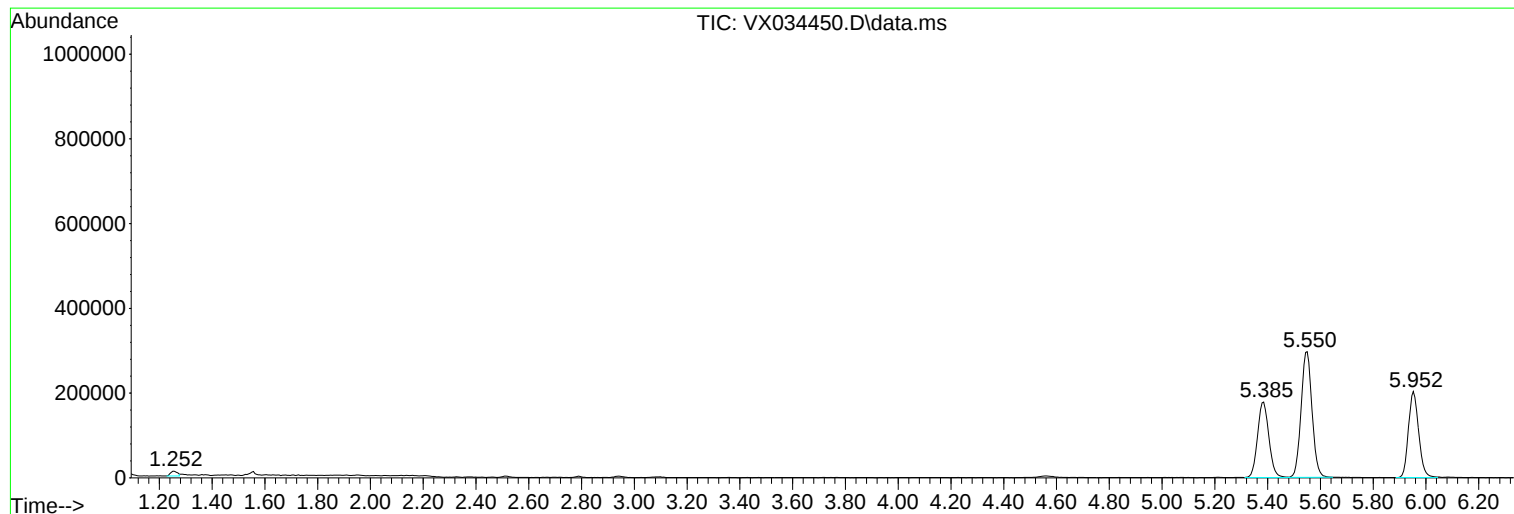

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034450.D
Acq On : 14 Mar 2023 09:22
Operator : JC/MD
Sample : VX0314MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0314MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034450.D
Acq On : 14 Mar 2023 09:22
Operator : JC/MD
Sample : VX0314MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0314MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------