

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034462.D
Acq On : 14 Mar 2023 14:09
Operator : JC/MD
Sample : 01880-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D3-20230310

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034462.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	33	rBV	20737	40825	2.94%	0.560%
2	1.563	70	78	82	rBV4	8595	17291	1.25%	0.237%
3	5.385	694	705	721	rBV2	155066	446860	32.18%	6.125%
4	5.550	721	732	752	rVB	259677	739753	53.27%	10.139%
5	5.952	787	798	811	rBV	175710	472792	34.04%	6.480%
6	6.763	919	931	947	rBV	424114	1007792	72.56%	13.813%
7	7.129	979	991	1000	rBV2	29607	70163	5.05%	0.962%
8	8.647	1233	1240	1252	rBV	890674	1388816	100.00%	19.036%
9	10.055	1465	1471	1485	rBV	828299	1171928	84.38%	16.063%
10	11.079	1634	1639	1649	rBV	757891	945824	68.10%	12.964%
11	12.024	1788	1794	1805	rBV	779496	993828	71.56%	13.622%




Sum of corrected areas: 7295872

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034462.D
Acq On : 14 Mar 2023 14:09
Operator : JC/MD
Sample : 01880-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D3-20230310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

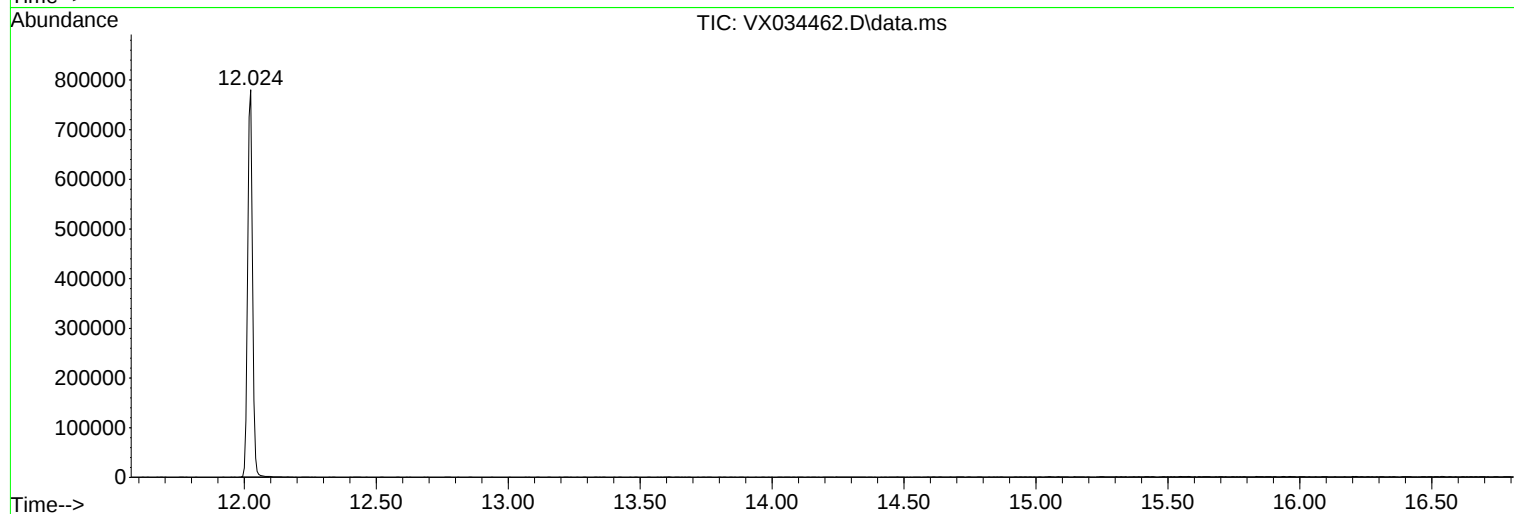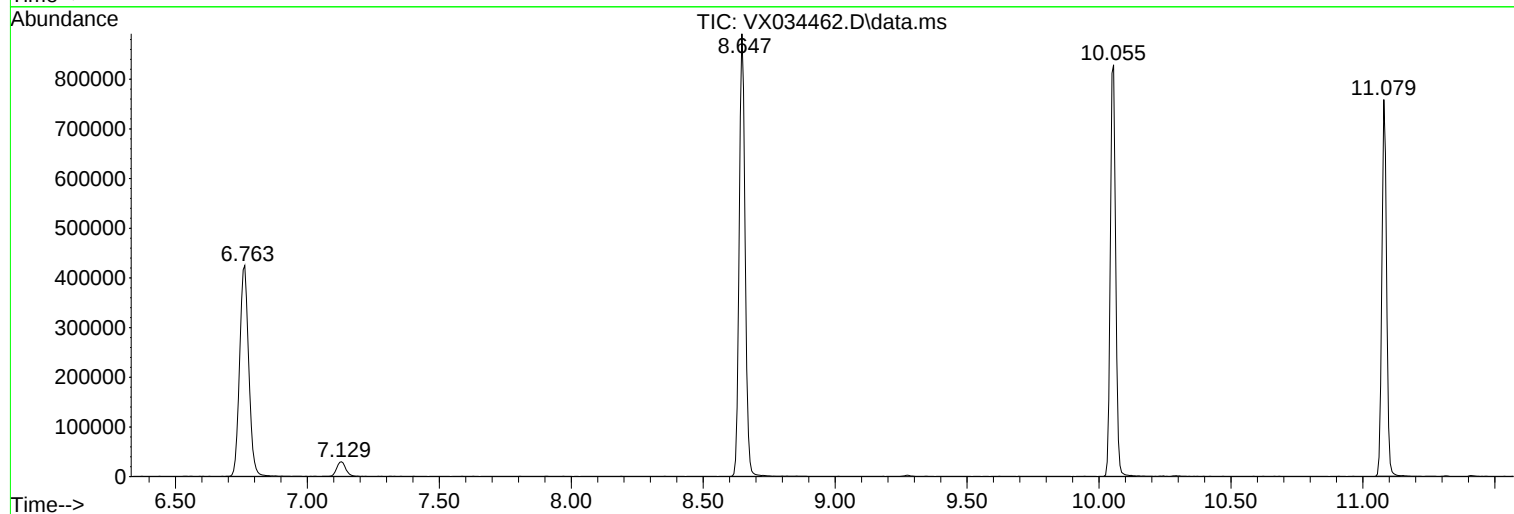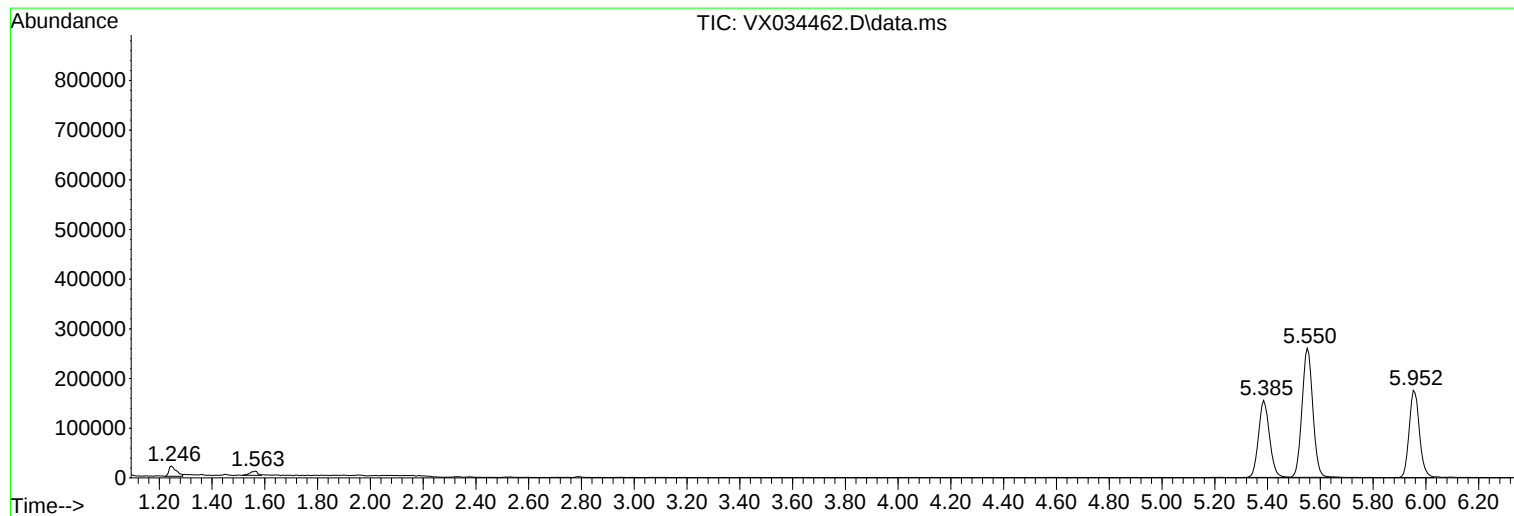

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034462.D
Acq On : 14 Mar 2023 14:09
Operator : JC/MD
Sample : 01880-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D3-20230310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034462.D
Acq On : 14 Mar 2023 14:09
Operator : JC/MD
Sample : 01880-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D3-20230310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------