

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
 Data File : VX034466.D
 Acq On : 14 Mar 2023 15:43
 Operator : JC/MD
 Sample : 01880-14DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE125D1-20230310DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034466.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	39	rBV	17227	42492	3.10%	0.532%
2	1.569	70	79	83	rBV2	8633	15971	1.16%	0.200%
3	2.940	296	304	312	rBV	14678	34406	2.51%	0.430%
4	4.562	563	570	583	rVB2	7817	27794	2.03%	0.348%
5	5.385	692	705	719	rBV2	153996	442797	32.30%	5.540%
6	5.550	721	732	749	rVB	255555	730097	53.25%	9.135%
7	5.958	787	799	812	rBV2	171646	469316	34.23%	5.872%
8	6.757	920	930	950	rBV	408141	988464	72.10%	12.368%
9	7.123	981	990	1014	rBV	372340	795375	58.02%	9.952%
10	8.647	1233	1240	1257	rBV	887194	1370955	100.00%	17.153%
11	9.275	1338	1343	1351	rBV2	36877	56251	4.10%	0.704%
12	10.055	1465	1471	1488	rBV	826179	1134466	82.75%	14.194%
13	11.079	1634	1639	1658	rBV	717430	919594	67.08%	11.506%
14	12.024	1788	1794	1807	rBV	744644	964335	70.34%	12.066%




Sum of corrected areas: 7992313

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034466.D
Acq On : 14 Mar 2023 15:43
Operator : JC/MD
Sample : 01880-14DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D1-20230310DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

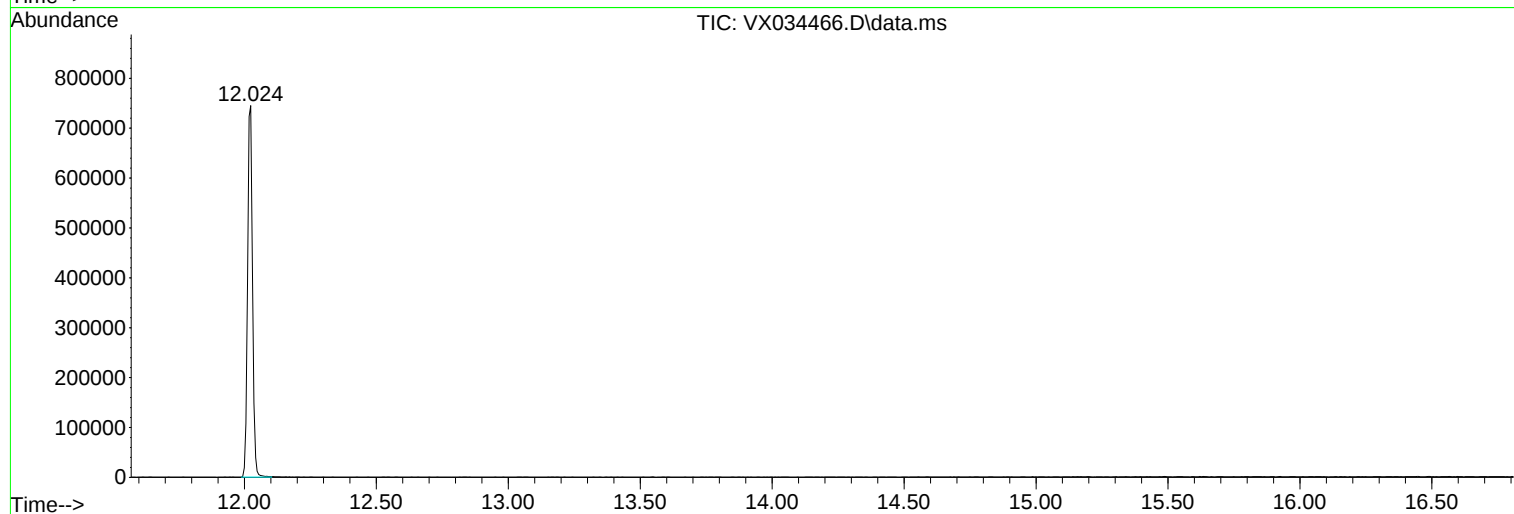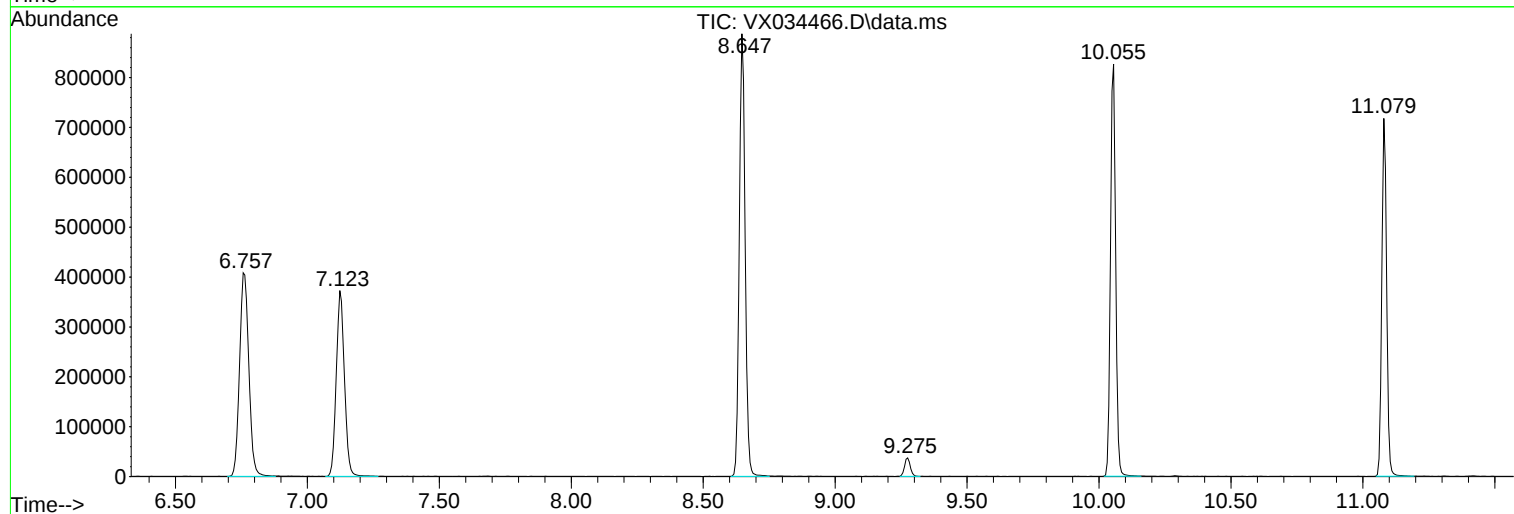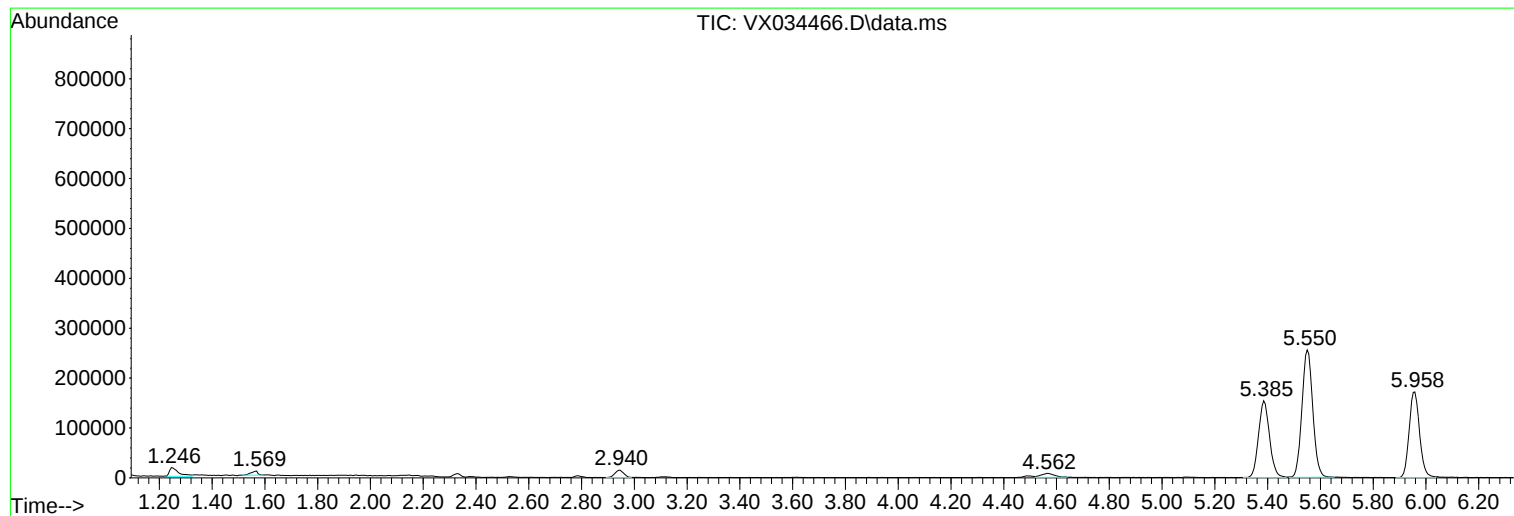

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034466.D
Acq On : 14 Mar 2023 15:43
Operator : JC/MD
Sample : 01880-14DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D1-20230310DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034466.D
Acq On : 14 Mar 2023 15:43
Operator : JC/MD
Sample : 01880-14DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D1-20230310DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------