

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
 Data File : VX034471.D
 Acq On : 14 Mar 2023 17:41
 Operator : JC/MD
 Sample : 01880-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE125D2-20230310

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034471.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.325	197	203	211	rBV2	81487	162683	2.73%	1.201%
2	4.489	547	558	569	rBV2	23301	68241	1.14%	0.504%
3	5.385	694	705	719	rBV	150133	436604	7.32%	3.224%
4	5.550	722	732	746	rVB	255607	716367	12.01%	5.289%
5	5.952	788	798	818	rBV	172450	466065	7.81%	3.441%
6	6.757	921	930	943	rBV	409912	978801	16.40%	7.227%
7	7.123	980	990	1016	rBV	2747278	5966585	100.00%	44.054%
8	8.647	1233	1240	1252	rBV	882312	1365680	22.89%	10.084%
9	9.275	1337	1343	1350	rBV	160105	238112	3.99%	1.758%
10	10.055	1465	1471	1487	rBV	840020	1165312	19.53%	8.604%
11	11.079	1634	1639	1656	rBV	763229	950042	15.92%	7.015%
12	12.024	1788	1794	1804	rBV	797502	1029185	17.25%	7.599%




Sum of corrected areas: 13543677

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034471.D
Acq On : 14 Mar 2023 17:41
Operator : JC/MD
Sample : 01880-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D2-20230310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

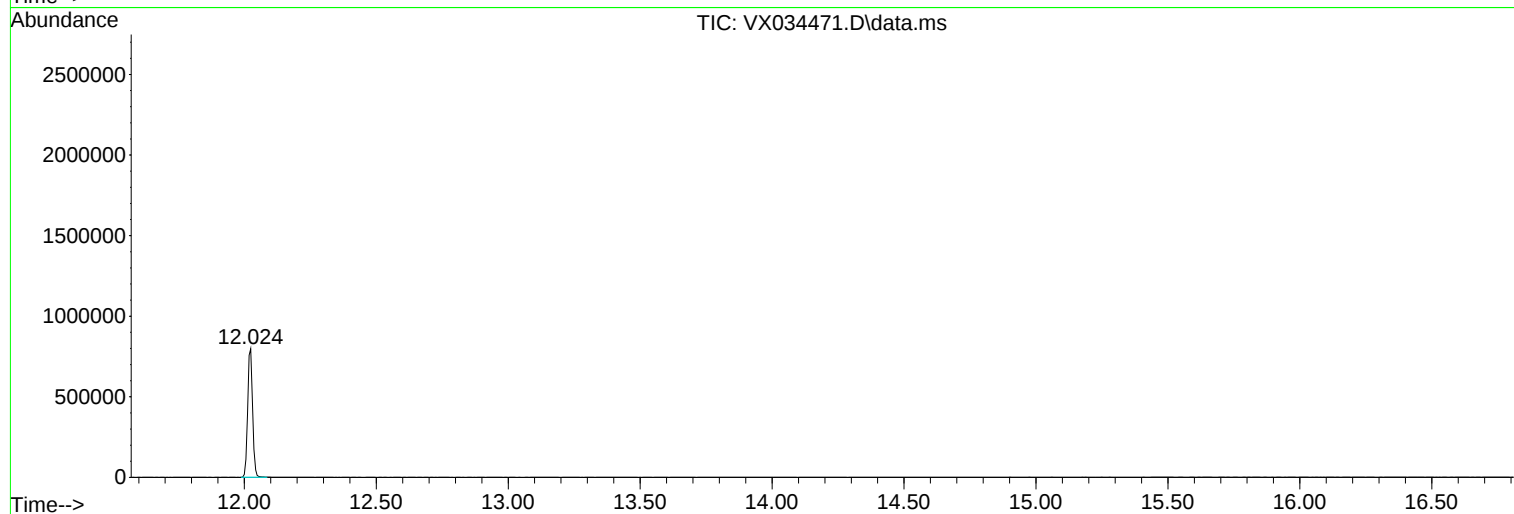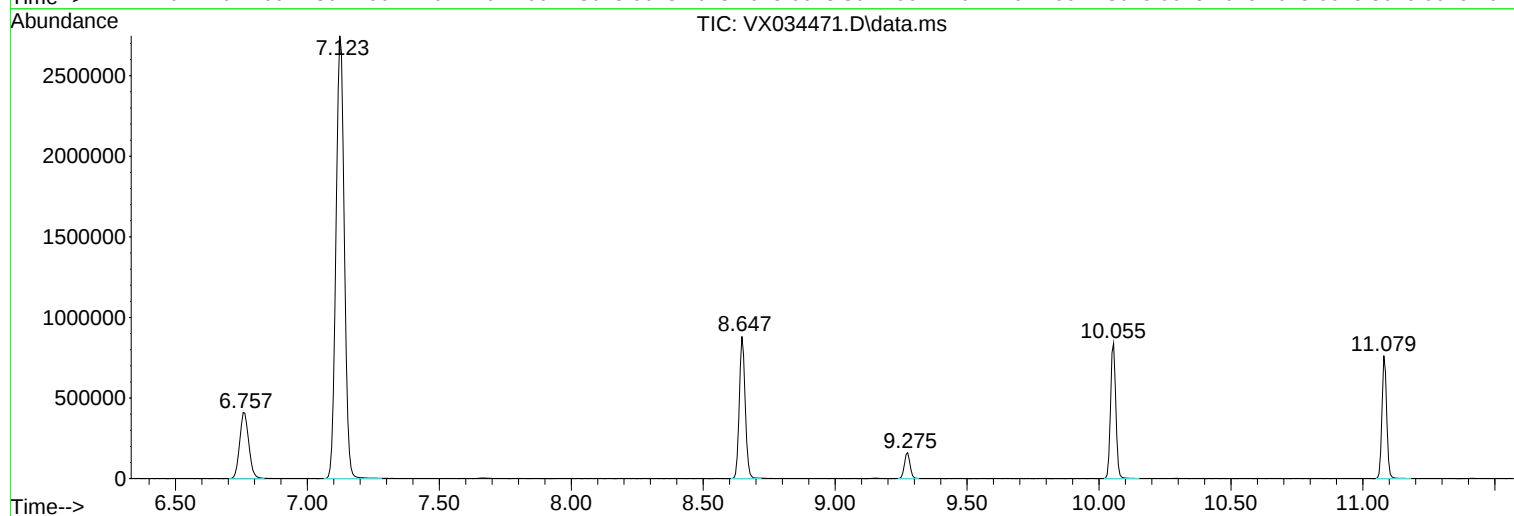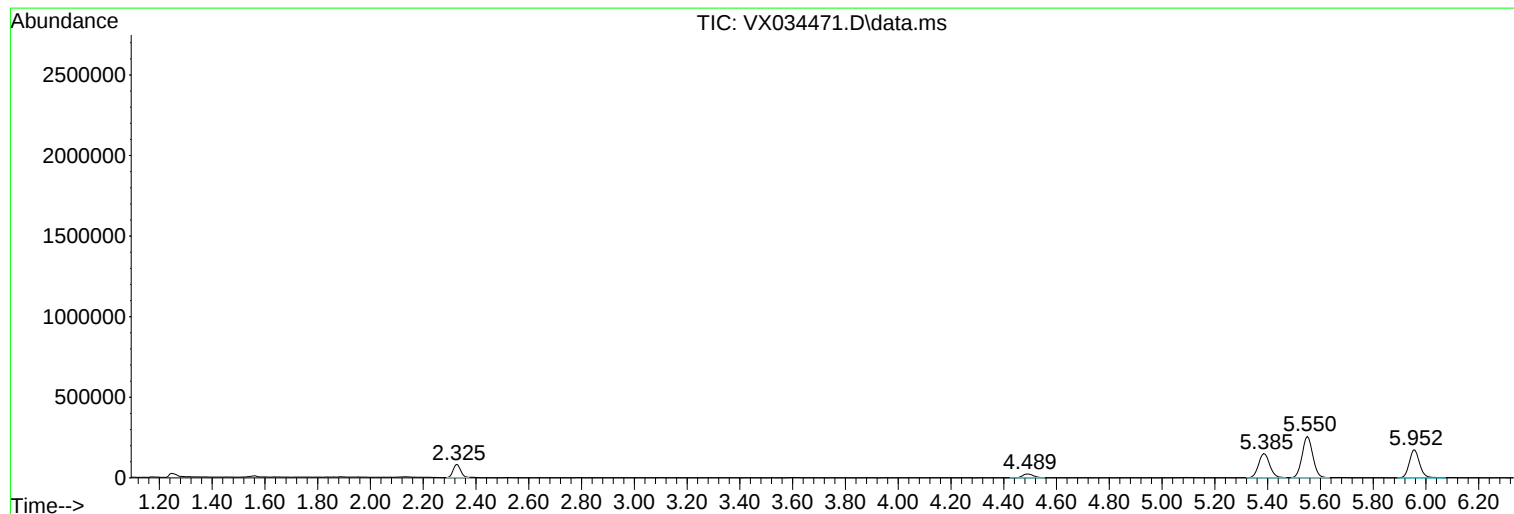

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034471.D
Acq On : 14 Mar 2023 17:41
Operator : JC/MD
Sample : 01880-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D2-20230310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031423\
Data File : VX034471.D
Acq On : 14 Mar 2023 17:41
Operator : JC/MD
Sample : 01880-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D2-20230310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------